

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
 Data File : PD076855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2023 23:06
 Operator : AR\AJ
 Sample : 03504-06
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46W3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/19/2023
 Supervised By : Ankita Jodhani 07/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 04:40:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.765	972.7E6	7852370	457.225	7.356 #
27)	SA Decachlor...	9.082	7.903	46292639	19248401	19.054	17.956
Target Compounds							
3)	MA gamma-BHC...	4.338	3.573	5480.7E6	984.8E6	1652.293m	657.340m#
7)	B delta-BHC	4.792	4.130	447.4E6	152.5E6	133.428m	99.908 #
8)	B Heptachlo...	5.686	4.710	630.2E6	297.1E6	210.326	211.171m
10)	B trans-Chl...	5.970	4.945	264.7E6	216.9E6	86.078m	160.406m#
11)	B cis-Chlor...	6.031	5.018	161.0E6	88637833	50.774	62.827
14)	MA Endrin	6.584	5.629	347.9E6	58734990	134.943	47.497m#
17)	MA 4,4'-DDT	7.005	6.017	345.2E6	159.3E6	154.629m	170.054
19)	B Endosulfa...	7.149	6.319	40205281	27541933	16.099m	24.685 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
Data File : PD076855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2023 23:06
Operator : AR\AJ
Sample : 03504-06
Misc :
ALS Vial : 46 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 04:40:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

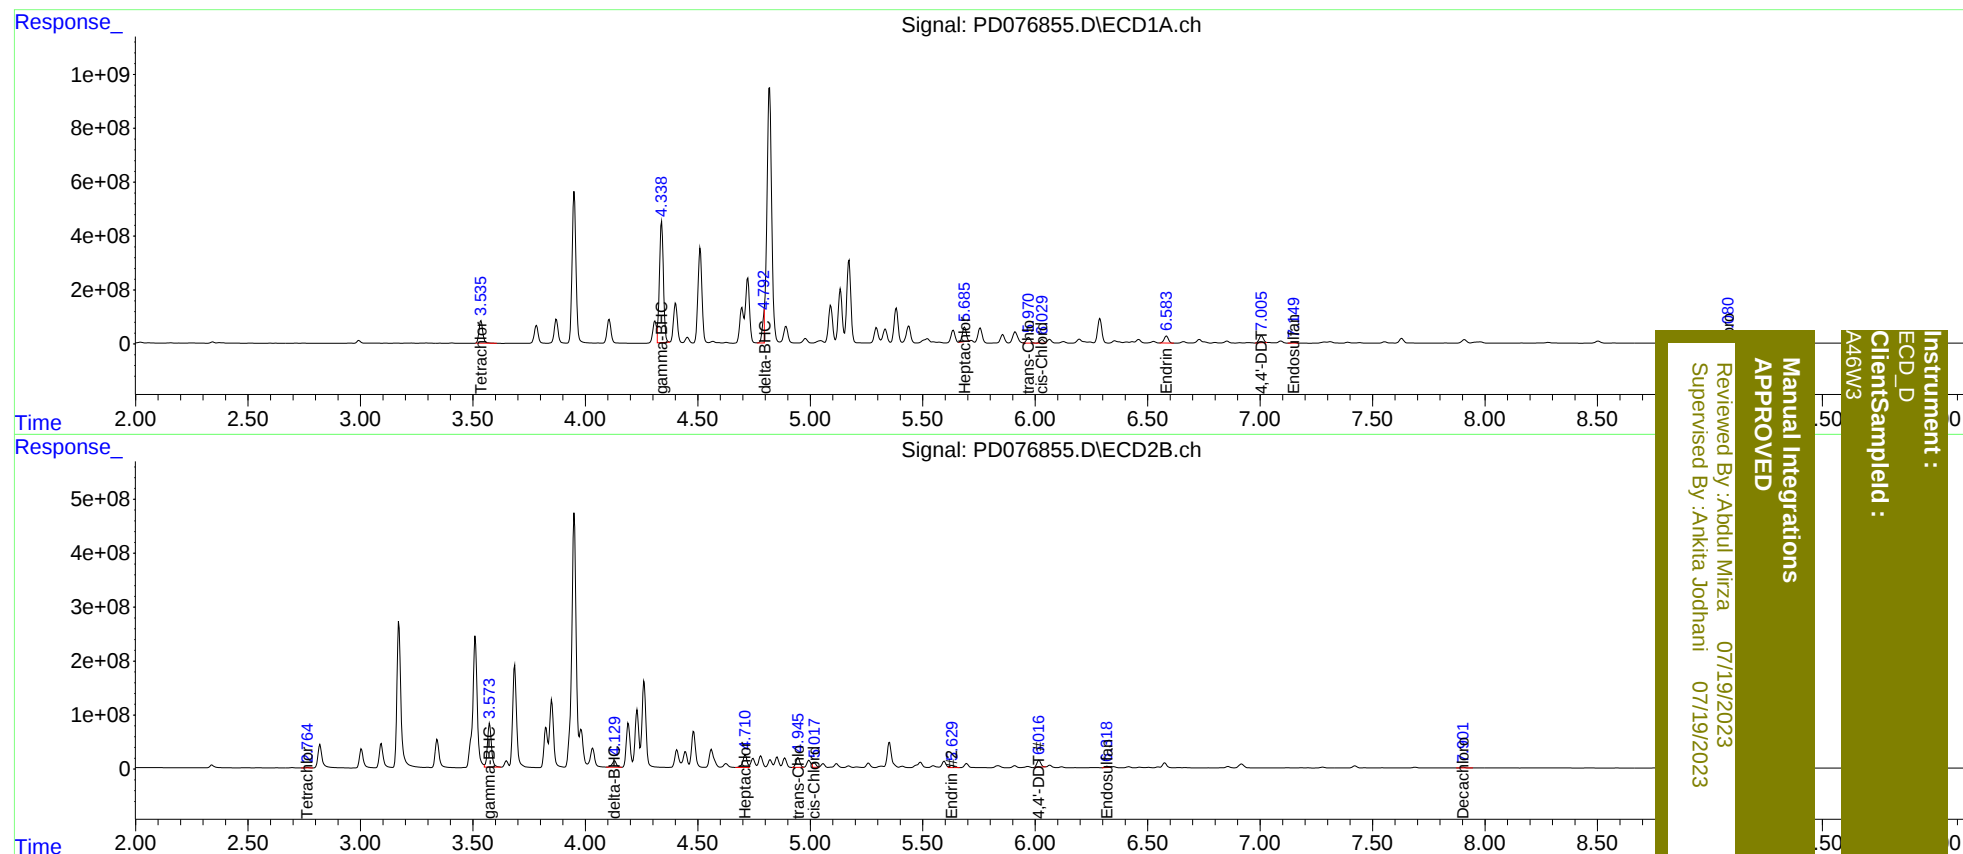

Instrument :
ECD_D
ClientSampled :
A46W3

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/19/2023
Supervised By :Ankita Jodhani 07/19/2023