

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
 Data File : PD076862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2023 00:40
 Operator : AR\AJ
 Sample : 03504-14
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46R7

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/19/2023
 Supervised By : Ankita Jodhani 07/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 13:24:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.765	15369667	7142861	7.225	6.692
2) SA Decachlor...	9.080	7.903	28691399	8661246	11.810m	8.080 #
Target Compounds						
3) MA gamma-BHC...	4.337	3.572	12161700	3244028	3.666m	2.165m#
7) B delta-BHC	4.795	4.130	13673379	5179377	4.077m	3.393
10) B trans-Chl...	5.961	4.943	3299149	1966235	1.073m	1.454m#
17) MA 4,4'-DDT	7.007	6.019	2639144	2268336	1.182m	2.421 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
Data File : PD076862.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2023 00:40
Operator : AR\AJ
Sample : 03504-14
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 13:24:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

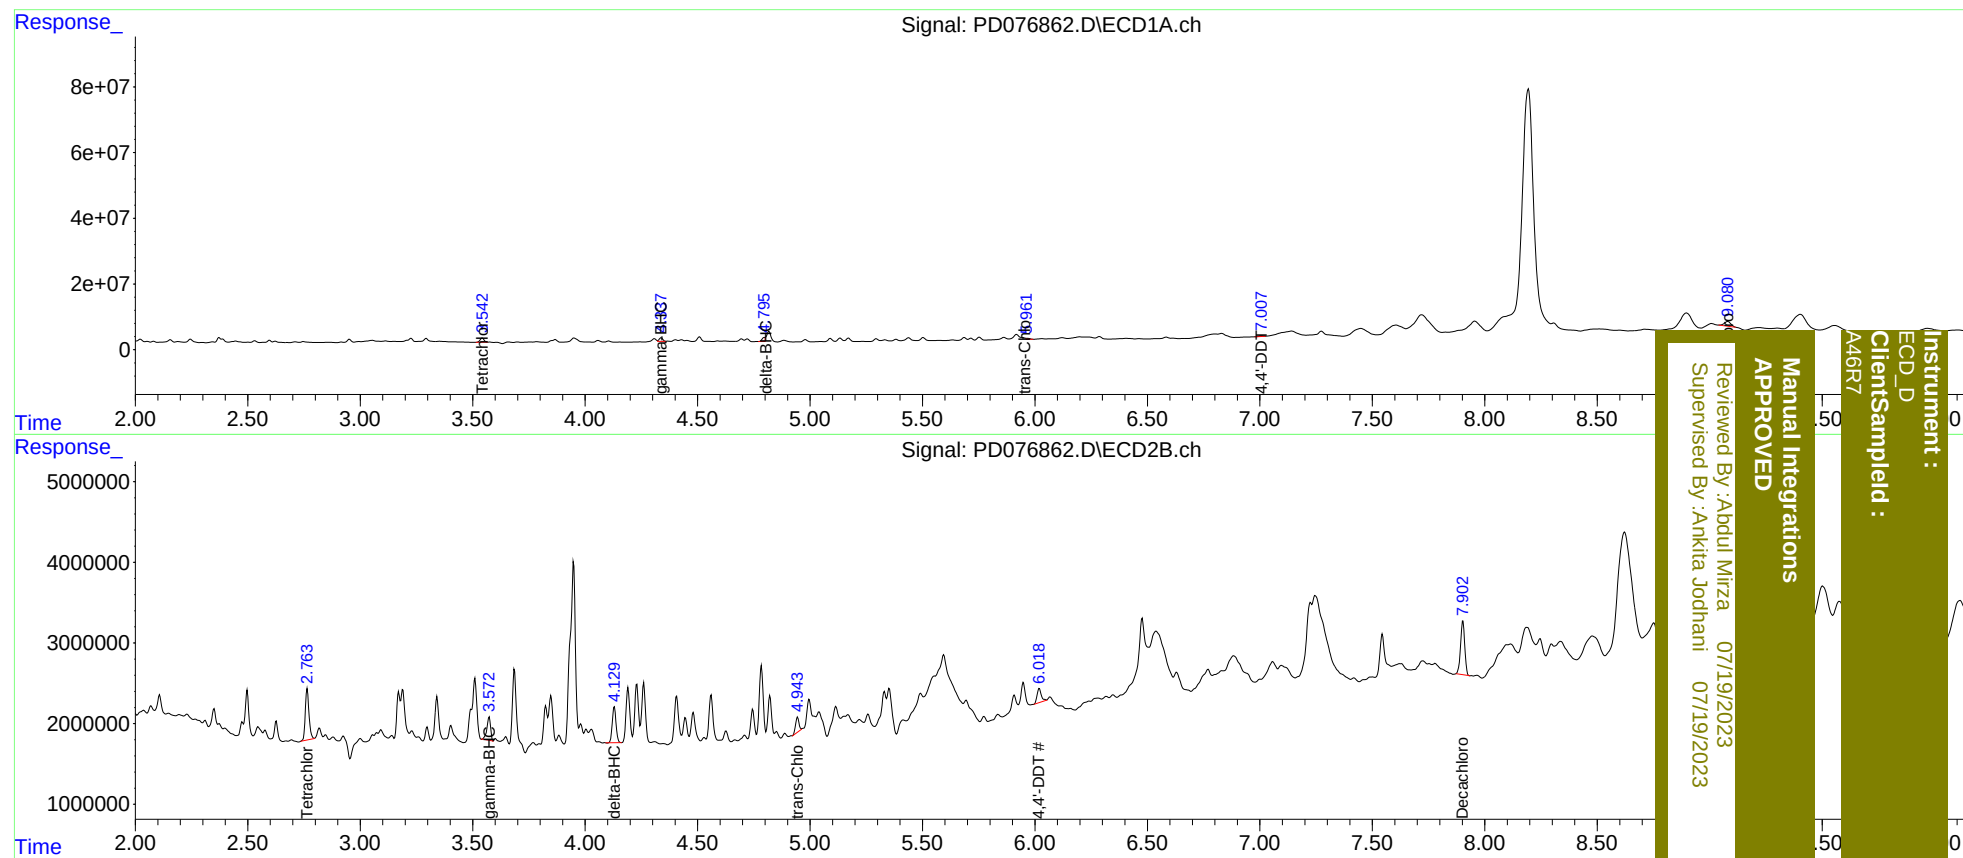

Instrument :
ECD_D
ClientSampled :
A46R7
Manual Integrations
APPROVED
Reviewed By :Abdul Mirza 07/19/2023
Supervised By :Ankita Jodhani 07/19/2023