

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
 Data File : PD076868.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2023 02:01
 Operator : AR\AJ
 Sample : 03504-21MS
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46T5MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/19/2023
 Supervised By : Ankita Jodhani 07/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 13:25:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.765	24693539	9438882	11.608	8.843
27)	SA Decachlor...	9.083	7.903	29478124	14297789	12.133	13.338
Target Compounds							
2)	A alpha-BHC	4.001	3.266	206.2E6	88936409	58.164	56.205
3)	MA gamma-BHC...	4.333	3.594	225.8E6	89787917	68.080m	59.933m
4)	MA Heptachlor	4.925	3.935	184.5E6	123.0E6	53.073	82.293 #
5)	MB Aldrin	5.267	4.213	193.9E6	99916112	56.709	66.391m
6)	B beta-BHC	4.529	3.892	81172766	33118621	53.405m	46.231
7)	B delta-BHC	4.779	4.122	170.6E6	90514227	50.879	59.303
8)	B Heptachlo...	5.692	4.716	185.1E6	74653199	61.779m	53.063
9)	A Endosulfan I	6.081	5.085	153.9E6	59258690	54.024	47.828m
10)	B trans-Chl...	5.950	4.965	177.3E6	79002313	57.647m	58.424m
11)	B cis-Chlor...	6.030	5.030	168.3E6	73971972	53.076	52.432
12)	B 4,4'-DDE	6.202	5.219	310.3E6	143.6E6	106.514	118.828
13)	MA Dieldrin	6.357	5.350	349.9E6	162.2E6	110.882	116.283
14)	MA Endrin	6.587	5.627	304.9E6	133.8E6	118.266	108.165
15)	B Endosulfa...	6.807	5.920	297.6E6	138.9E6	111.911	115.512
16)	A 4,4'-DDD	6.721	5.774	266.6E6	113.5E6	117.968	119.773
17)	MA 4,4'-DDT	7.036	6.024	262.5E6	120.2E6	117.551	128.311
18)	B Endrin al...	6.937	6.100	192.7E6	85103523	103.056	101.458
19)	B Endosulfa...	7.172	6.322	259.7E6	118.4E6	103.988	106.156
20)	A Methoxychlor	7.512	6.600	725.5E6	300.6E6	548.046	563.276
21)	B Endrin ke...	7.659	6.829	288.5E6	132.0E6	104.216	103.188

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071723\
Data File : PD076868.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2023 02:01
Operator : AR\AJ
Sample : 03504-21MS
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 13:25:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

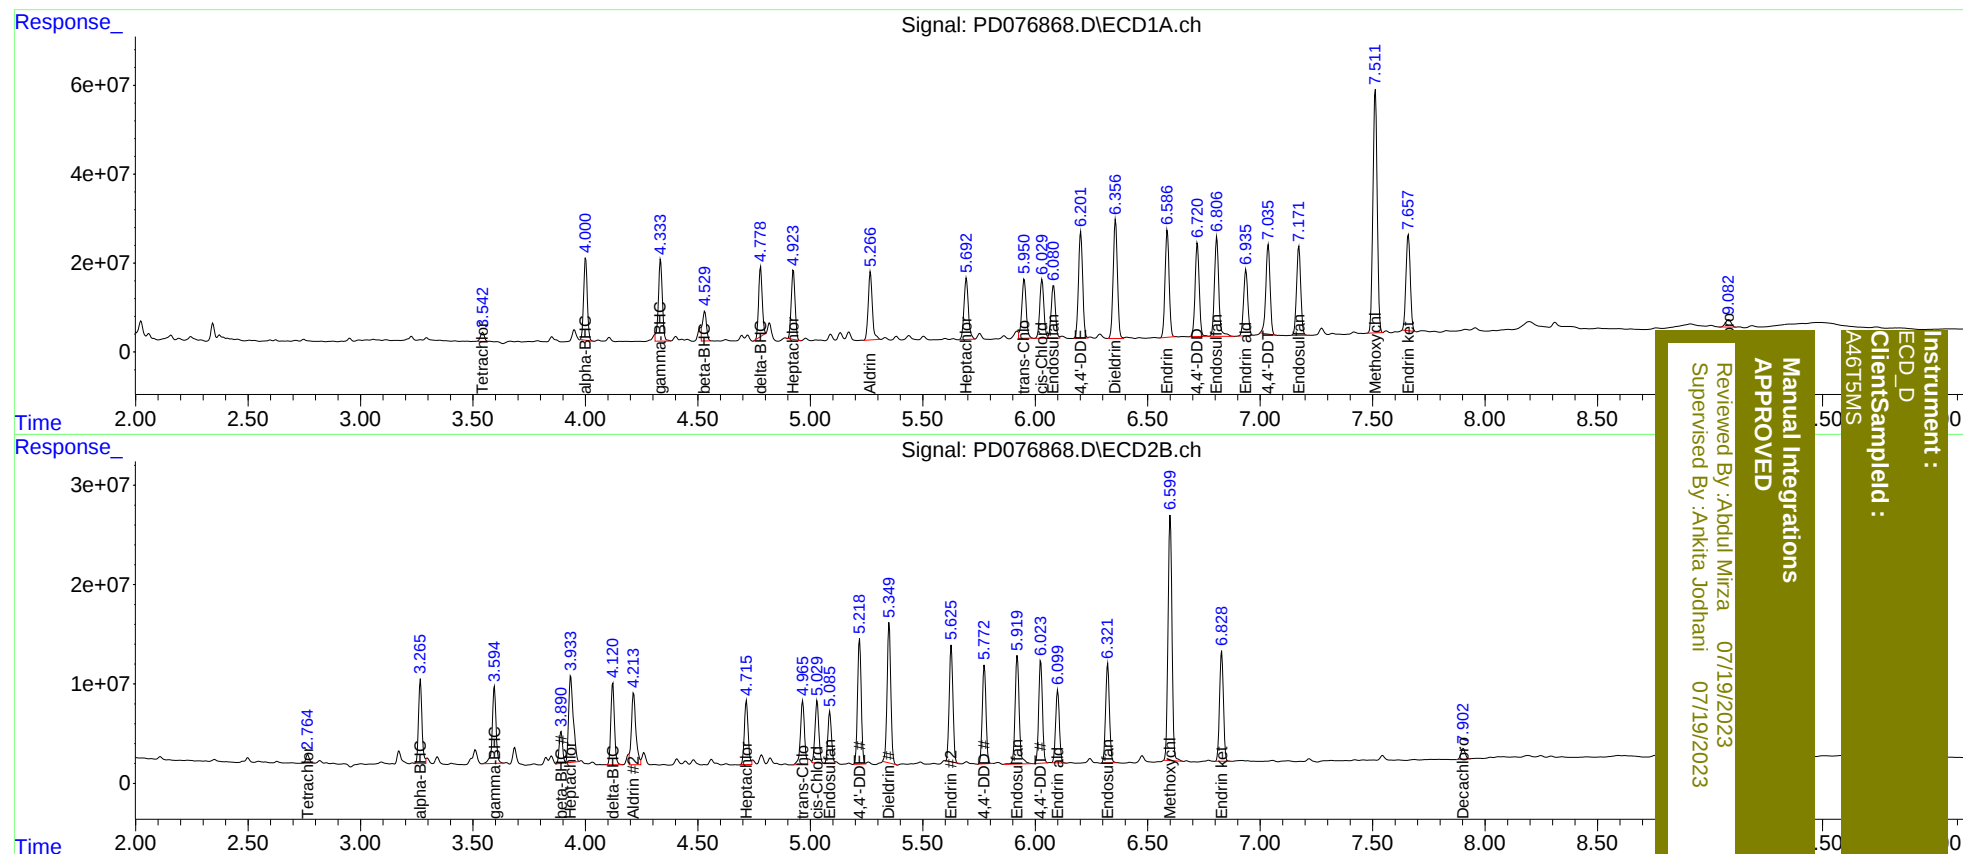

Instrument :
ECD_D
Client Sampled :
A46T5MS
Manual Integrations
APPROVED
Reviewed By : Abdul Miza 07/19/2023
Supervised By : Ankita Jodhani 07/19/2023