

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071725\
 Data File : PD089514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2025 11:49
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 06:49:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071725CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 18 06:48:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.879	15101033	100.3E6	5.462	5.374
27)	SA Decachlor...	9.082	8.074	42620680	245.4E6	11.369	11.469
Target Compounds							
2)	A alpha-BHC	4.006	3.392	26423355	158.8E6	4.840	5.272
3)	MA gamma-BHC...	4.338	3.729	26466311	147.8E6	5.020	5.314
4)	MA Heptachlor	4.937	4.082	27994563	155.0E6	5.198	5.411
9)	A Endosulfan I	6.082	5.247	23644884	130.2E6	5.330	5.476
13)	MA Dieldrin	6.355	5.513	48234236	282.4E6	10.074	11.011
14)	MA Endrin	6.582	5.789	40484531	286.9E6	10.031	12.240
16)	A 4,4'-DDD	6.713	5.930	37449753	233.7E6	11.053	11.133
17)	MA 4,4'-DDT	7.029	6.184	35704204	236.8E6	10.066	10.806
20)	A Methoxychlor	7.501	6.755	102.1E6	588.2E6	53.828	59.389


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071725\
Data File : PD089514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2025 11:49
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 06:49:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071725CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 18 06:48:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

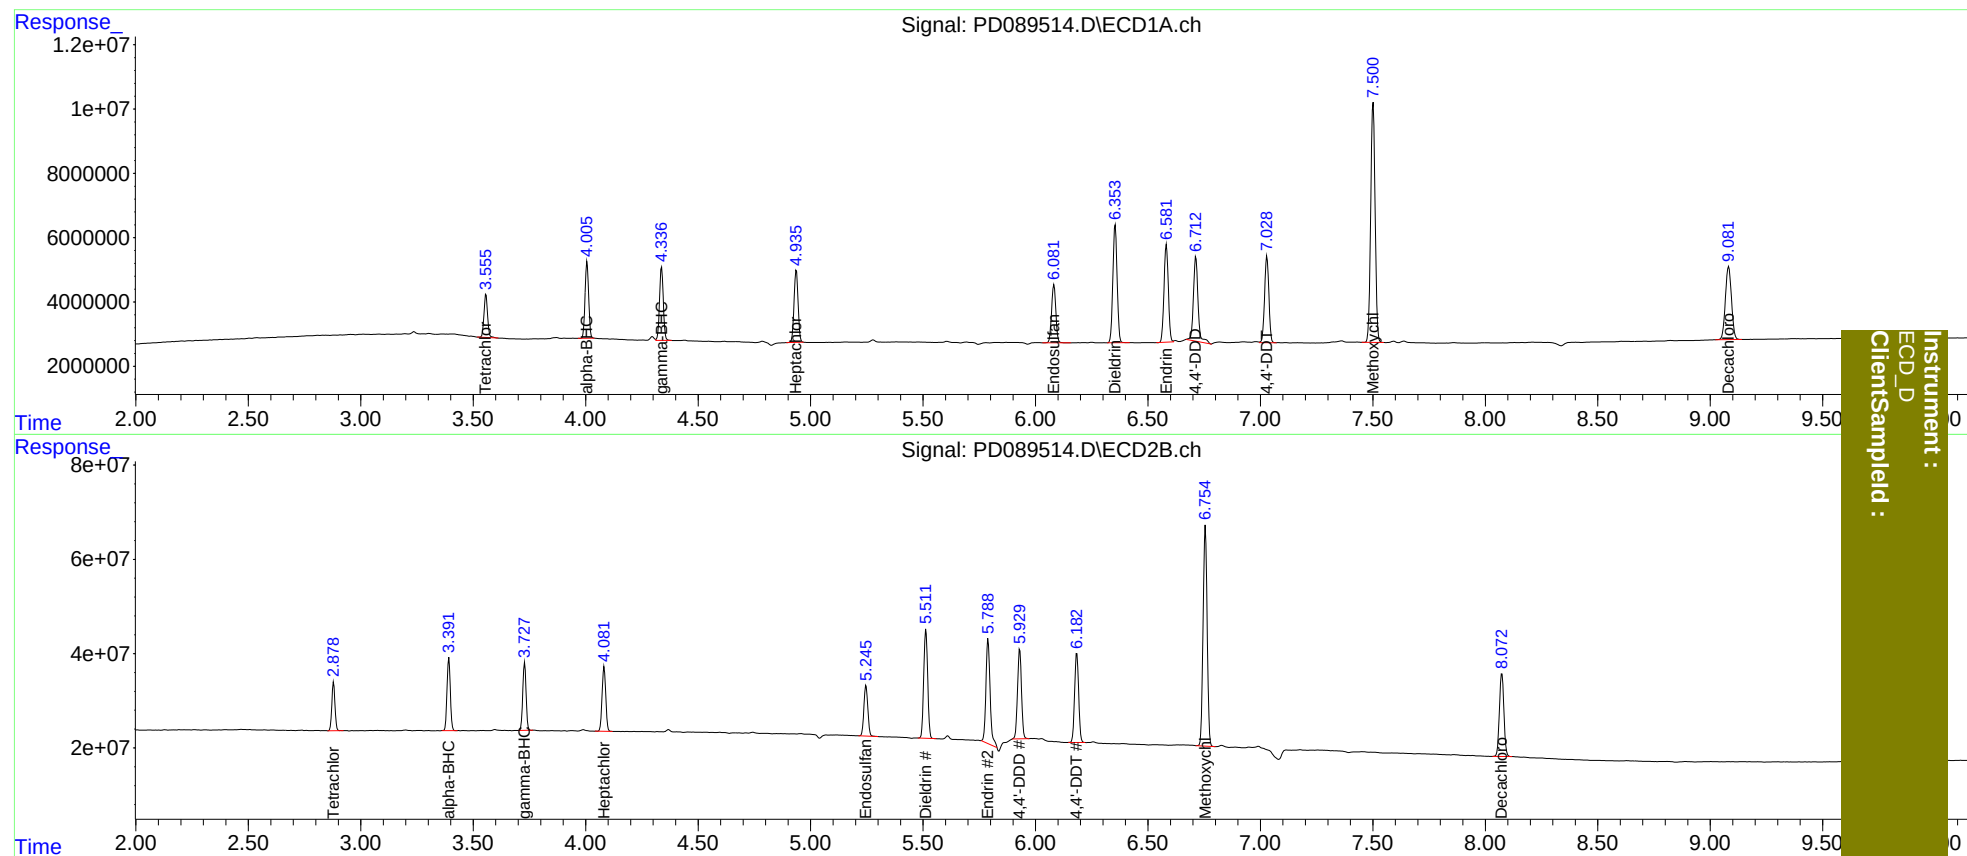


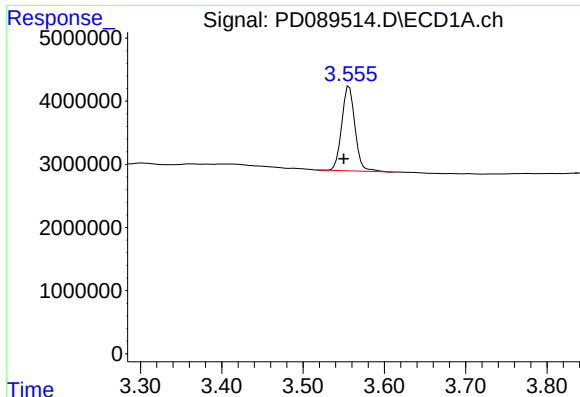

#1 Tetrachloro-m-xylene


R.T.: 3.557 min
Delta R.T.: 0.007 min
Response: 15101033
Conc: 5.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

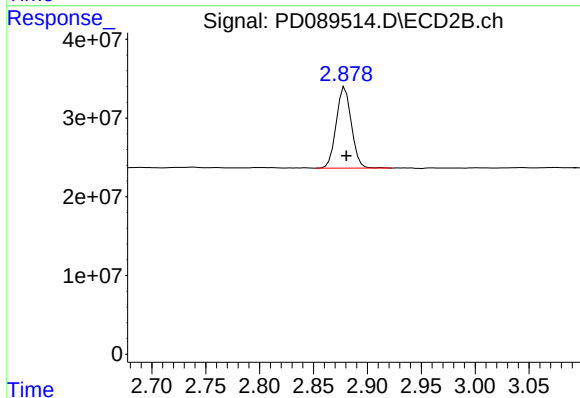


#1 Tetrachloro-m-xylene

R.T.: 2.879 min
Delta R.T.: -0.001 min
Response: 100291166
Conc: 5.37 ng/ml

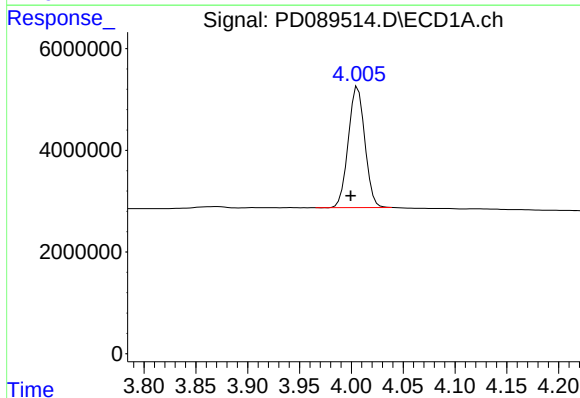


#2 alpha-BHC

R.T.: 4.006 min
Delta R.T.: 0.007 min
Response: 26423355
Conc: 4.84 ng/ml

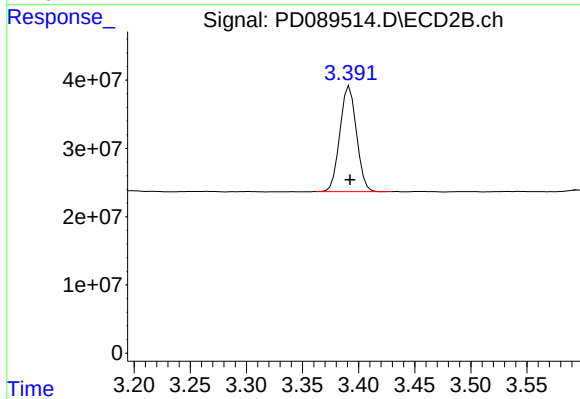

#2 alpha-BHC


R.T.: 3.392 min
Delta R.T.: 0.000 min
Response: 158797864
Conc: 5.27 ng/ml

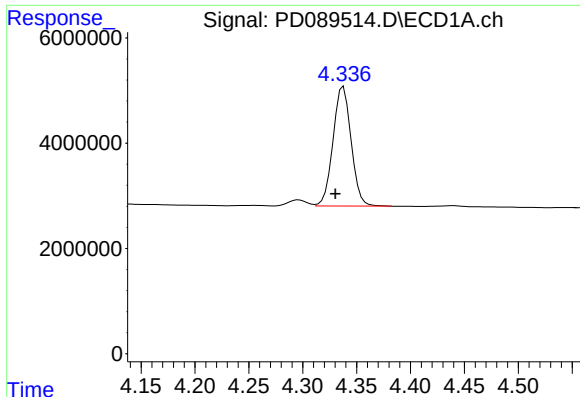

#3 gamma-BHC (Lindane)


R.T.: 4.338 min
Delta R.T.: 0.007 min
Response: 26466311
Conc: 5.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

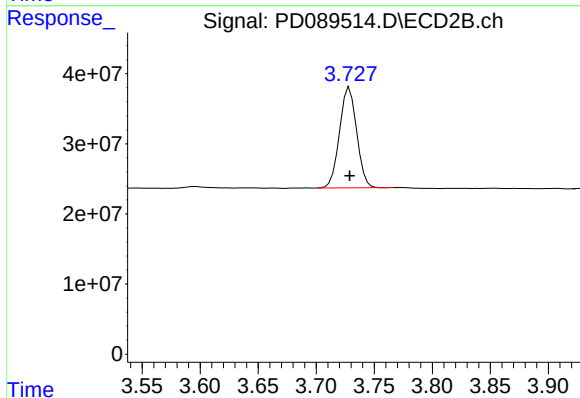


#3 gamma-BHC (Lindane)

R.T.: 3.729 min
Delta R.T.: 0.000 min
Response: 147774319
Conc: 5.31 ng/ml

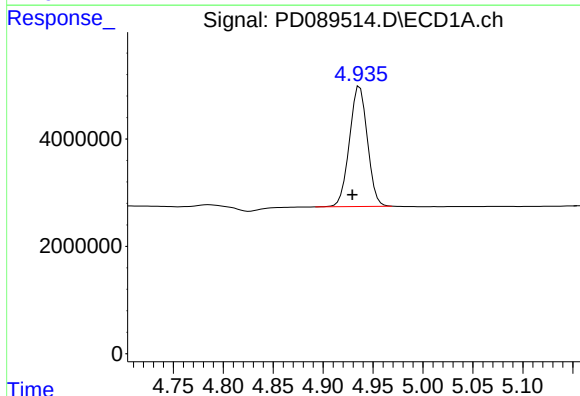


#4 Heptachlor

R.T.: 4.937 min
Delta R.T.: 0.007 min
Response: 27994563
Conc: 5.20 ng/ml

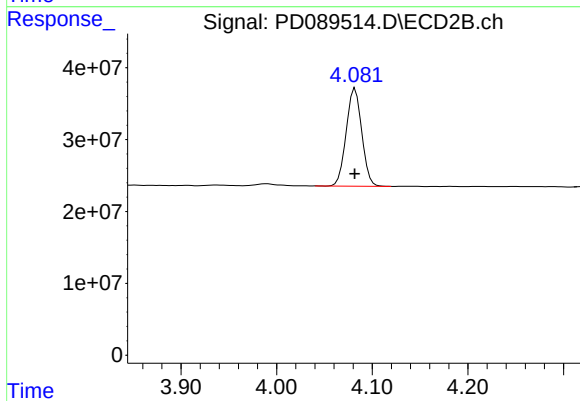

#4 Heptachlor


R.T.: 4.082 min
Delta R.T.: 0.000 min
Response: 155034223
Conc: 5.41 ng/ml

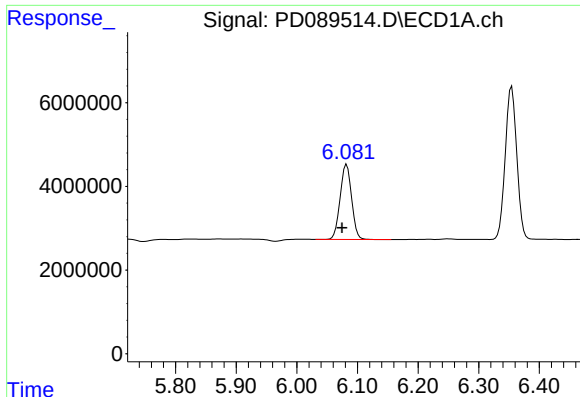

#9 Endosulfan I


R.T.: 6.082 min
Delta R.T.: 0.008 min
Response: 23644884
Conc: 5.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

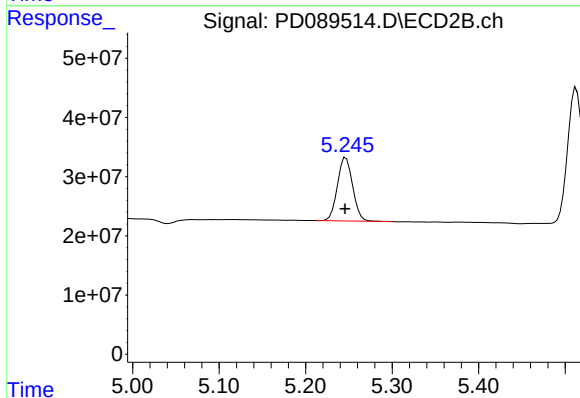


#9 Endosulfan I

R.T.: 5.247 min
Delta R.T.: 0.001 min
Response: 130241612
Conc: 5.48 ng/ml

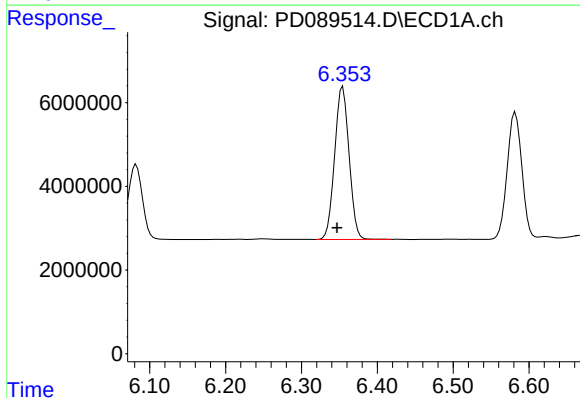


#13 Dieldrin

R.T.: 6.355 min
Delta R.T.: 0.007 min
Response: 48234236
Conc: 10.07 ng/ml

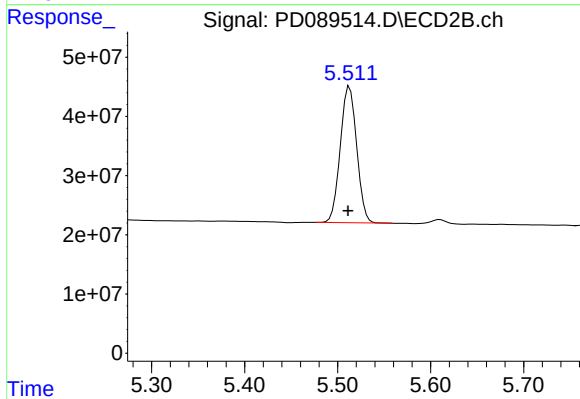

#13 Dieldrin


R.T.: 5.513 min
Delta R.T.: 0.002 min
Response: 282420135
Conc: 11.01 ng/ml

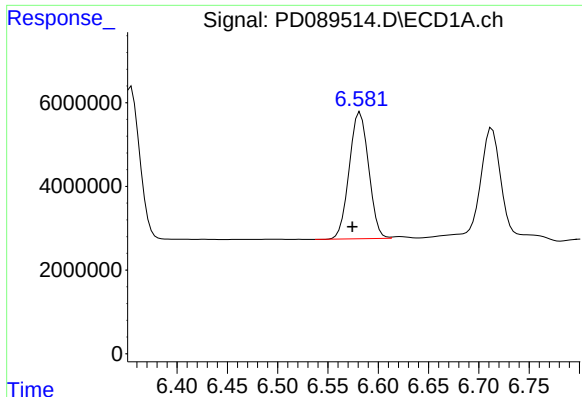

#14 Endrin


R.T.: 6.582 min
Delta R.T.: 0.008 min
Response: 40484531
Conc: 10.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

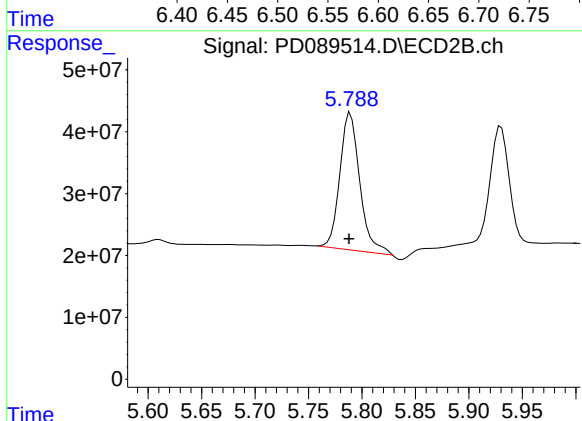


#14 Endrin

R.T.: 5.789 min
Delta R.T.: 0.001 min
Response: 286915213
Conc: 12.24 ng/ml

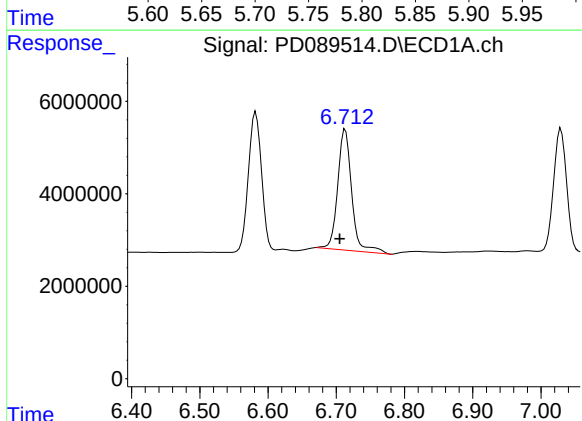


#16 4,4'-DDD

R.T.: 6.713 min
Delta R.T.: 0.008 min
Response: 37449753
Conc: 11.05 ng/ml

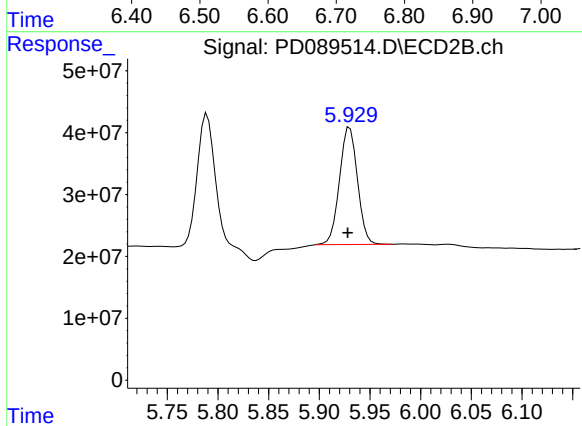

#16 4,4'-DDD


R.T.: 5.930 min
Delta R.T.: 0.002 min
Response: 233657706
Conc: 11.13 ng/ml

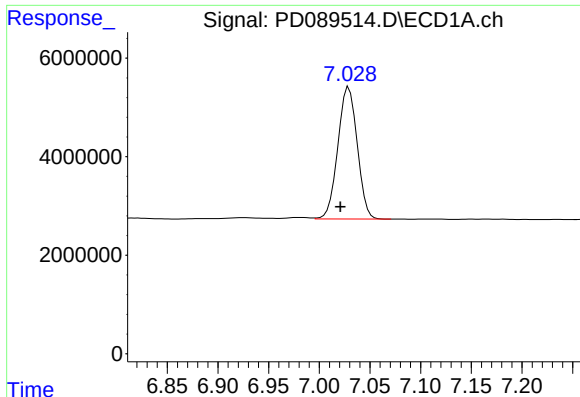

#17 4,4'-DDT


R.T.: 7.029 min
Delta R.T.: 0.008 min
Response: 35704204
Conc: 10.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

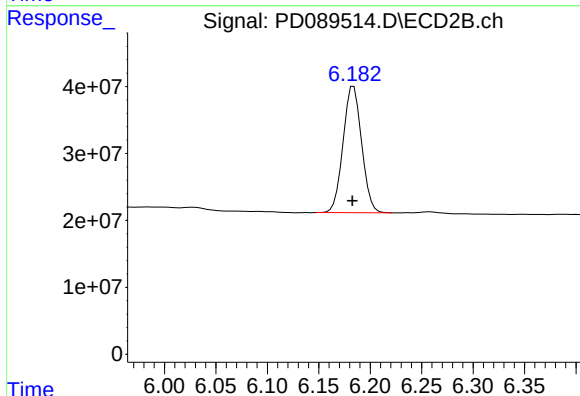


#17 4,4'-DDT

R.T.: 6.184 min
Delta R.T.: 0.001 min
Response: 236797094
Conc: 10.81 ng/ml

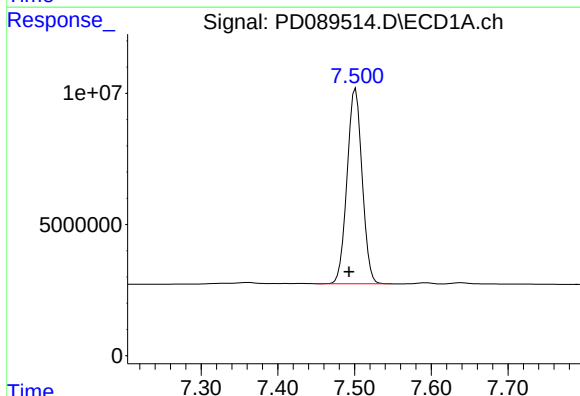


#20 Methoxychlor

R.T.: 7.501 min
Delta R.T.: 0.008 min
Response: 102086297
Conc: 53.83 ng/ml

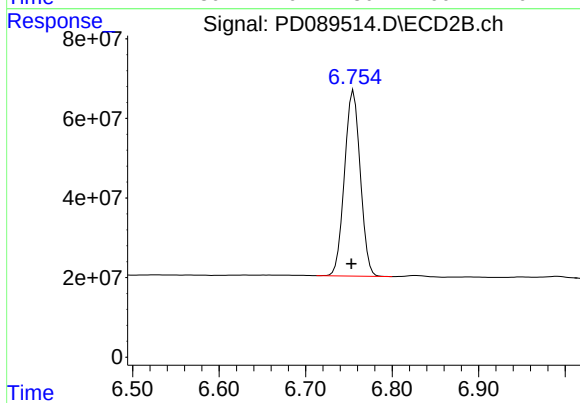

#20 Methoxychlor


R.T.: 6.755 min
Delta R.T.: 0.002 min
Response: 588161294
Conc: 59.39 ng/ml

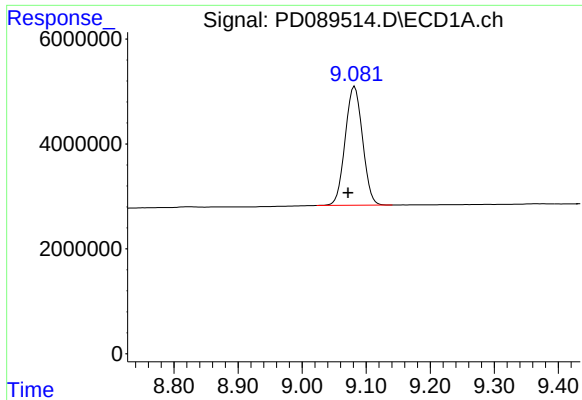

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: 0.010 min
Response: 42620680
Conc: 11.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

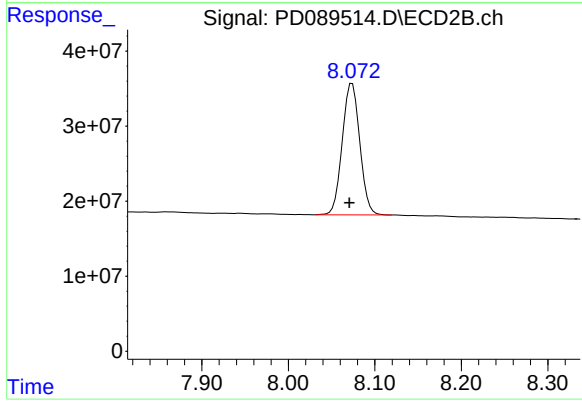

#27 Decachlorobiphenyl

R.T.: 8.074 min
Delta R.T.: 0.003 min
Response: 245359049
Conc: 11.47 ng/ml