

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071725\
 Data File : PD089516.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2025 12:16
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 06:49:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071725CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 18 06:48:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.880	28216387	197.0E6	10.207	10.553
27)	SA Decachlor...	9.072	8.070	79590769	457.8E6	21.231	21.400
Target Compounds							
2)	A alpha-BHC	3.999	3.392	53272011	312.0E6	9.758	10.360
3)	MA gamma-BHC...	4.329	3.728	52651806	288.9E6	9.987	10.390
4)	MA Heptachlor	4.929	4.081	54439761	299.8E6	10.109	10.465
9)	A Endosulfan I	6.073	5.246	46406658	252.0E6	10.462	10.594
13)	MA Dieldrin	6.346	5.511	95051033	541.1E6	19.851	21.095
14)	MA Endrin	6.574	5.788	80552648	523.4E6	19.958	22.330
16)	A 4,4'-DDD	6.704	5.928	67107209	442.0E6	19.805	21.059
17)	MA 4,4'-DDT	7.020	6.182	70407082	456.4E6	19.849	20.825
20)	A Methoxychlor	7.492	6.752	194.7E6	1091.6E6	102.649	110.224

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071725\
Data File : PD089516.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2025 12:16
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 06:49:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071725CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 18 06:48:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

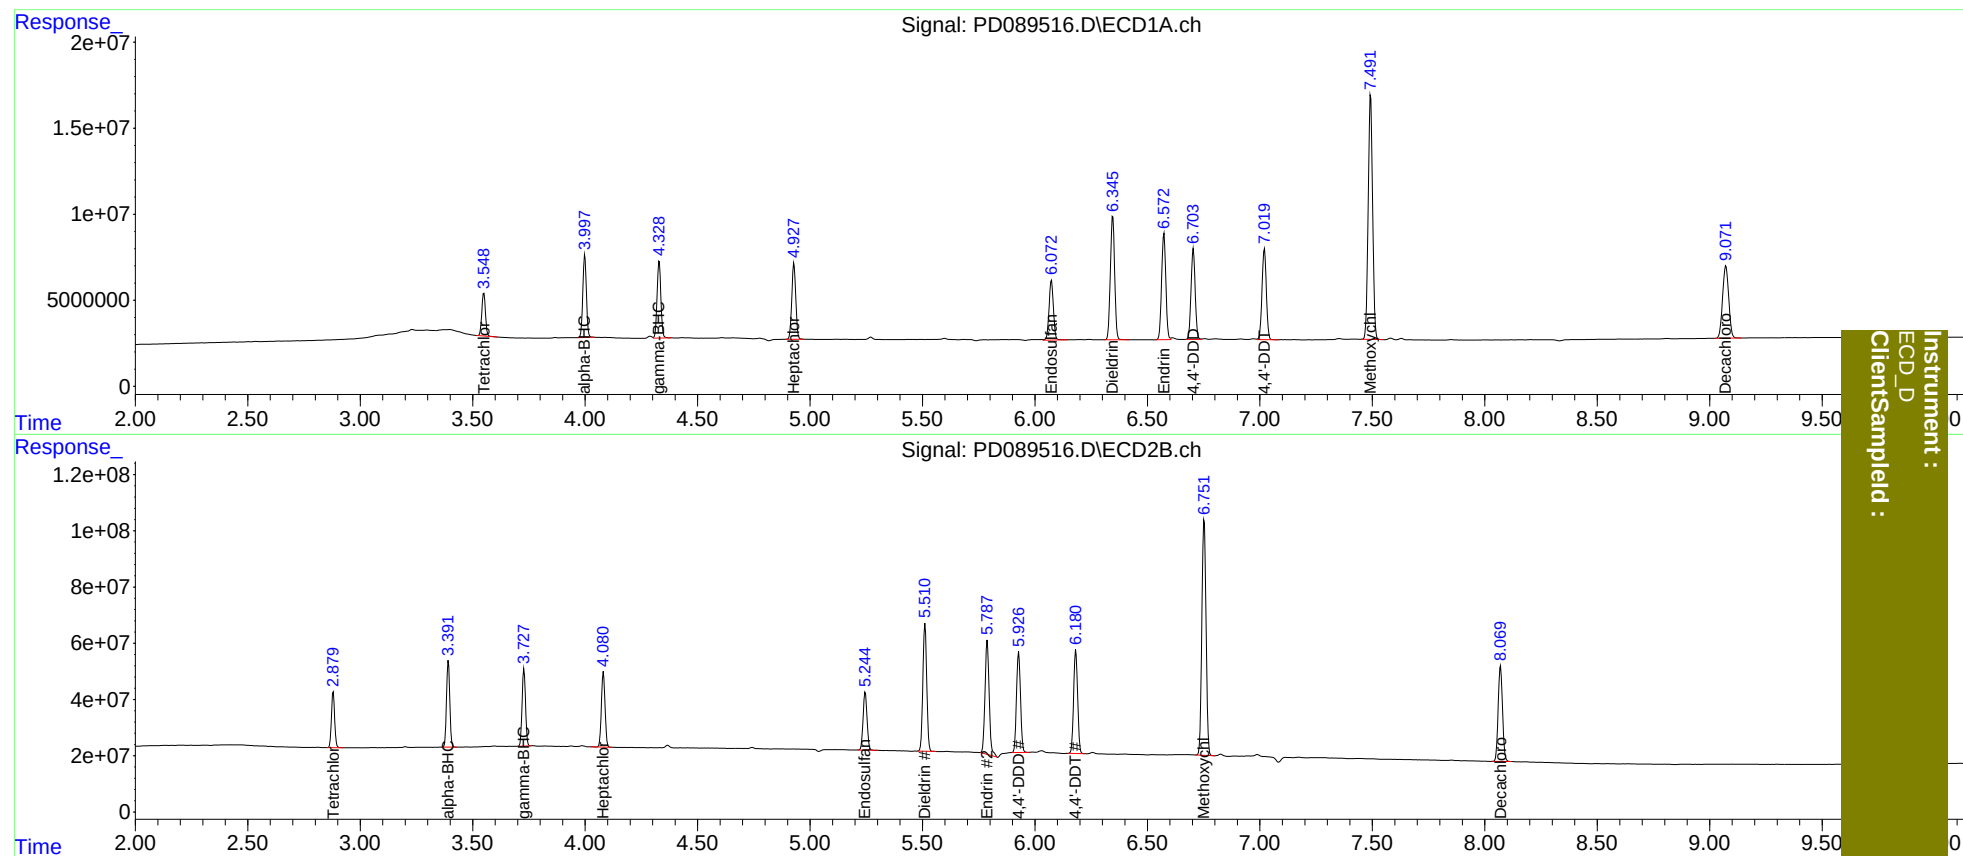


Instrument :
ECD_D
ClientSampled :
0

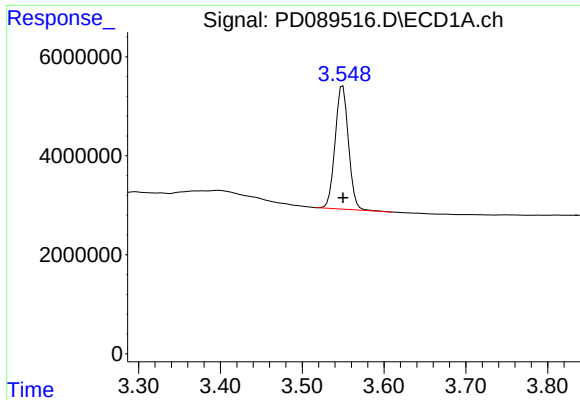

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 28216387
Conc: 10.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

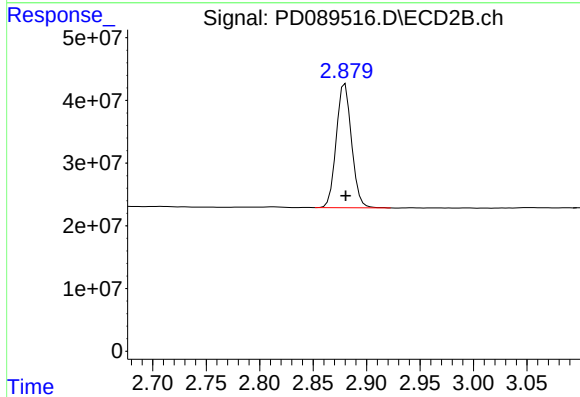


#1 Tetrachloro-m-xylene

R.T.: 2.880 min
Delta R.T.: 0.000 min
Response: 196953284
Conc: 10.55 ng/ml

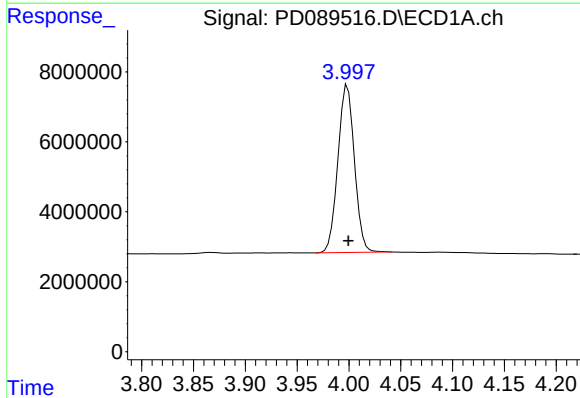


#2 alpha-BHC

R.T.: 3.999 min
Delta R.T.: 0.000 min
Response: 53272011
Conc: 9.76 ng/ml

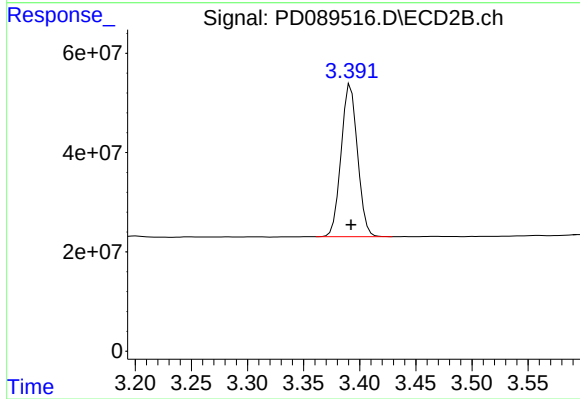

#2 alpha-BHC


R.T.: 3.392 min
Delta R.T.: 0.000 min
Response: 312037631
Conc: 10.36 ng/ml

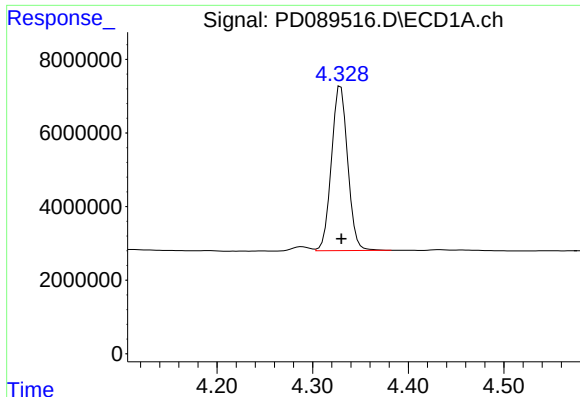

#3 gamma-BHC (Lindane)


R.T.: 4.329 min
Delta R.T.: 0.000 min
Response: 52651806
Conc: 9.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

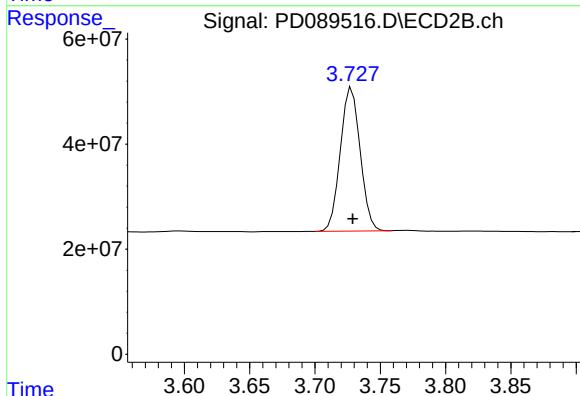


#3 gamma-BHC (Lindane)

R.T.: 3.728 min
Delta R.T.: 0.000 min
Response: 288919915
Conc: 10.39 ng/ml

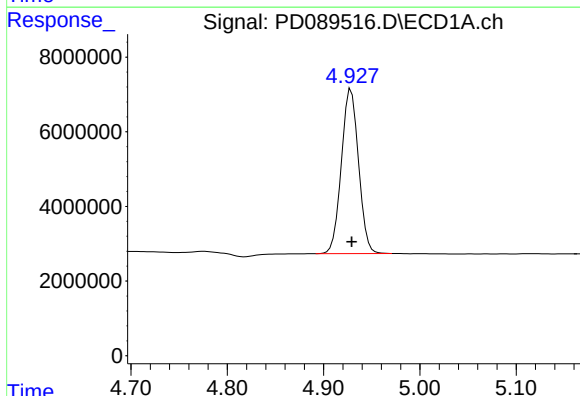


#4 Heptachlor

R.T.: 4.929 min
Delta R.T.: 0.000 min
Response: 54439761
Conc: 10.11 ng/ml

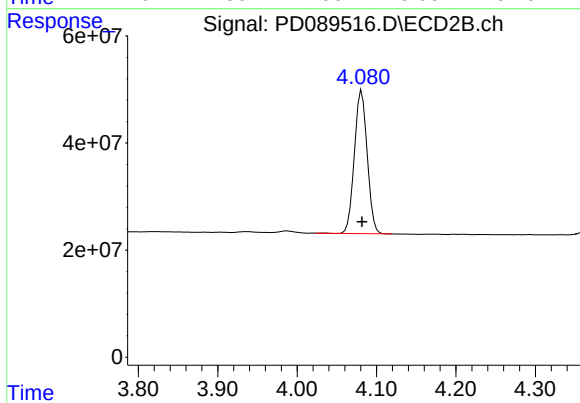

#4 Heptachlor


R.T.: 4.081 min
Delta R.T.: 0.000 min
Response: 299821867
Conc: 10.47 ng/ml

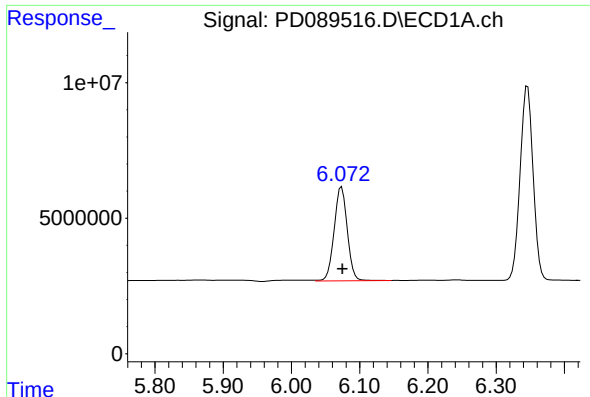

#9 Endosulfan I


R.T.: 6.073 min
Delta R.T.: -0.001 min
Response: 46406658
Conc: 10.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

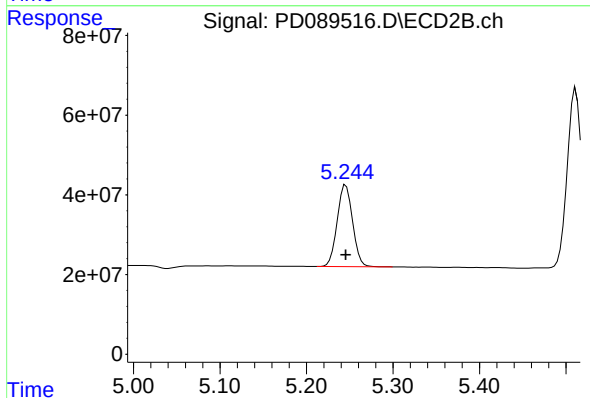


#9 Endosulfan I

R.T.: 5.246 min
Delta R.T.: 0.000 min
Response: 251978460
Conc: 10.59 ng/ml

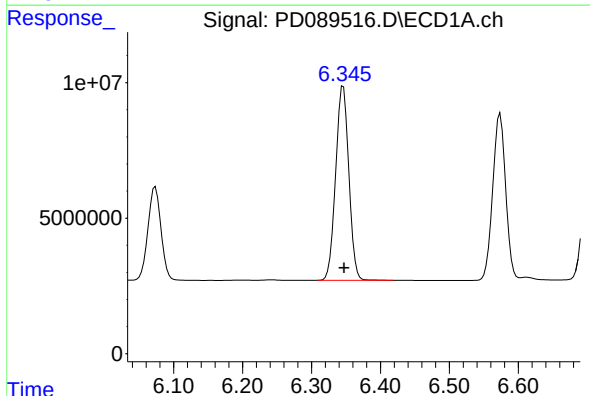


#13 Dieldrin

R.T.: 6.346 min
Delta R.T.: -0.001 min
Response: 95051033
Conc: 19.85 ng/ml

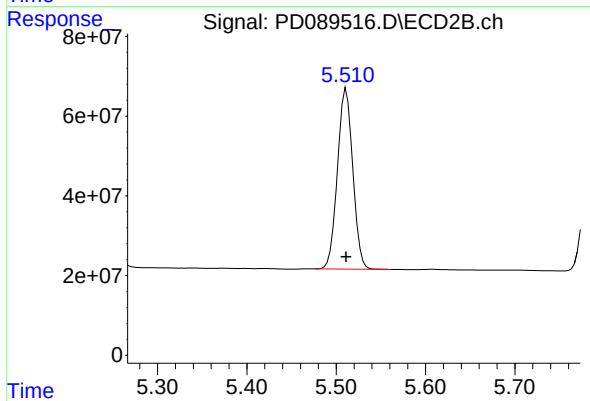

#13 Dieldrin


R.T.: 5.511 min
Delta R.T.: 0.000 min
Response: 541055815
Conc: 21.09 ng/ml

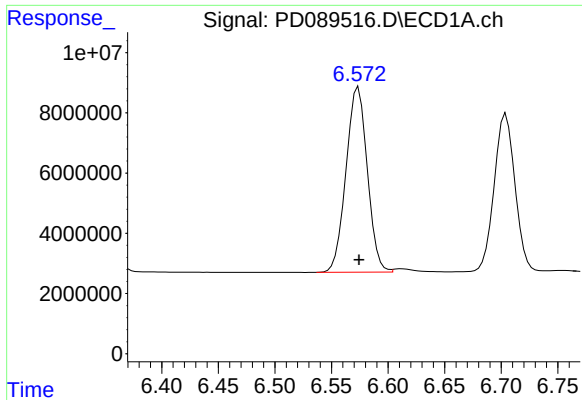

#14 Endrin


R.T.: 6.574 min
Delta R.T.: 0.000 min
Response: 80552648
Conc: 19.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

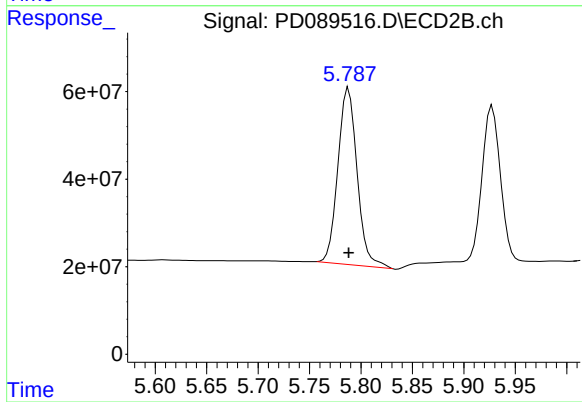


#14 Endrin

R.T.: 5.788 min
Delta R.T.: 0.000 min
Response: 523444712
Conc: 22.33 ng/ml

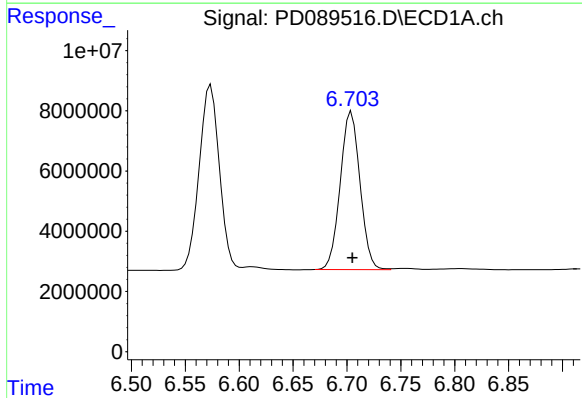


#16 4,4'-DDD

R.T.: 6.704 min
Delta R.T.: 0.000 min
Response: 67107209
Conc: 19.81 ng/ml

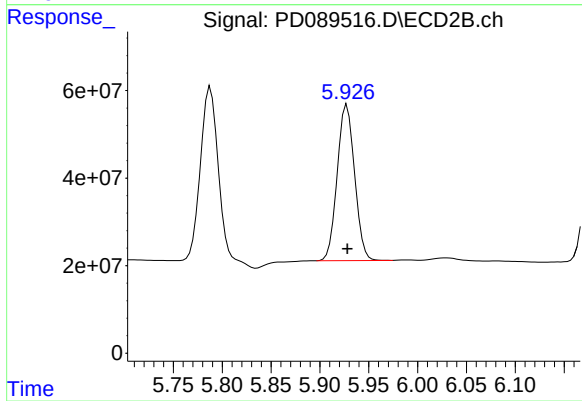

#16 4,4'-DDD


R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 441977998
Conc: 21.06 ng/ml

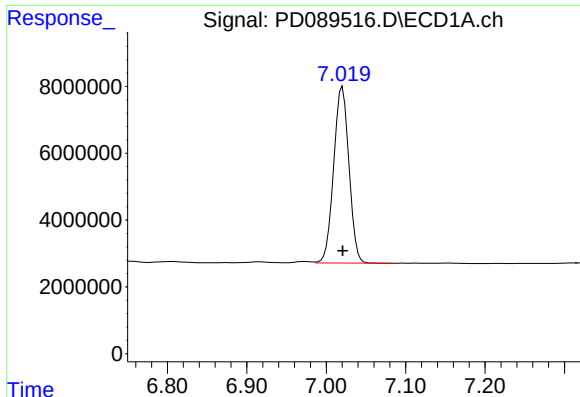

#17 4,4'-DDT


R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 70407082
Conc: 19.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

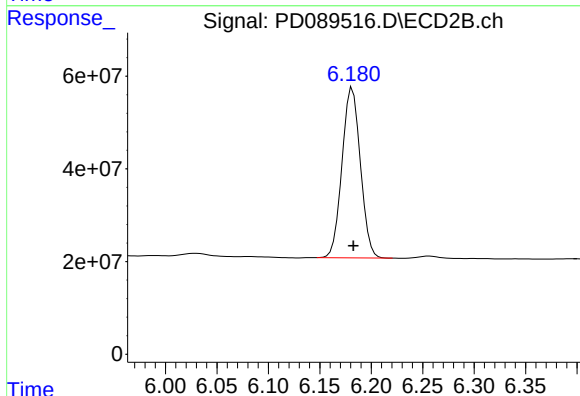


#17 4,4'-DDT

R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 456355884
Conc: 20.82 ng/ml

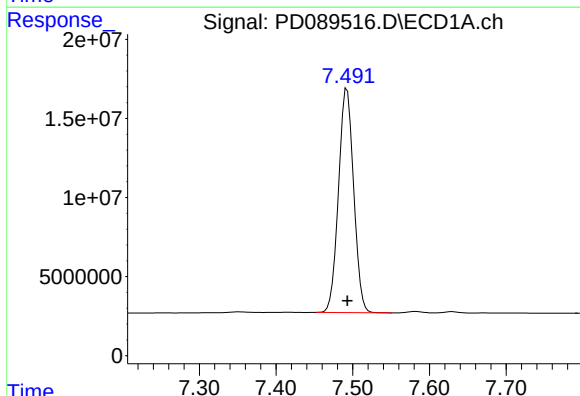


#20 Methoxychlor

R.T.: 7.492 min
Delta R.T.: 0.000 min
Response: 194677590
Conc: 102.65 ng/ml

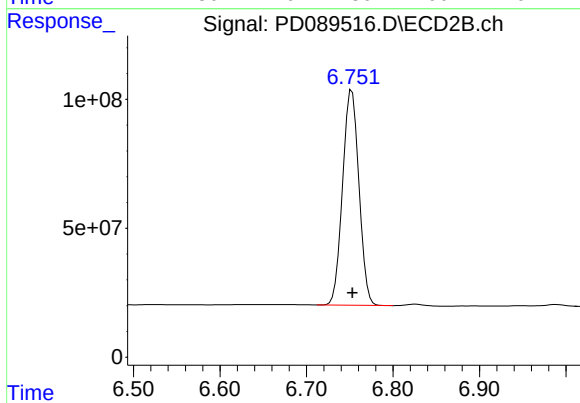

#20 Methoxychlor


R.T.: 6.752 min
Delta R.T.: 0.000 min
Response: 1091606307
Conc: 110.22 ng/ml

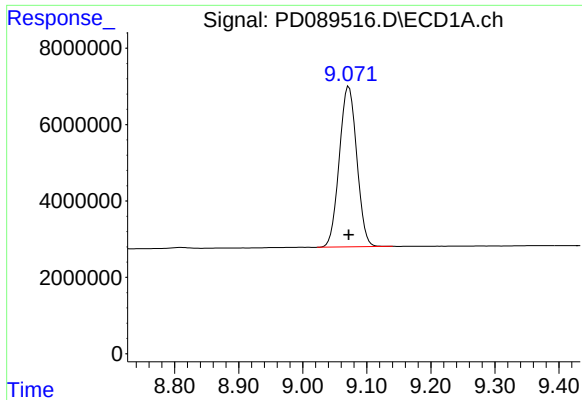

#27 Decachlorobiphenyl

R.T.: 9.072 min
Delta R.T.: 0.000 min
Response: 79590769
Conc: 21.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

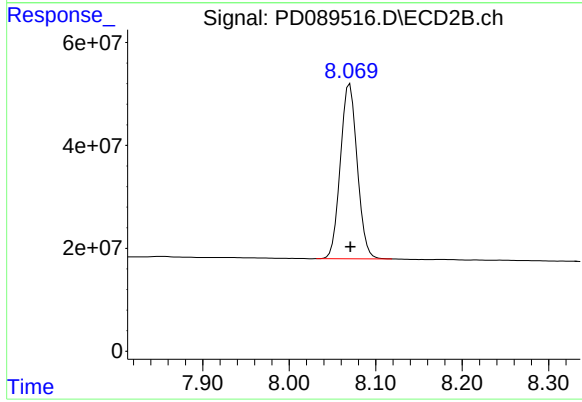

#27 Decachlorobiphenyl

R.T.: 8.070 min
Delta R.T.: 0.000 min
Response: 457814044
Conc: 21.40 ng/ml