

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071725\
 Data File : PD089518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2025 12:43
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 06:49:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071725CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 18 06:48:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.880	55290386	373.3E6	20.000	20.000
27)	SA Decachlor...	9.072	8.071	149.9E6	855.7E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.999	3.392	109.2E6	602.4E6	20.000	20.000
3)	MA gamma-BHC...	4.330	3.729	105.4E6	556.2E6	20.000	20.000
4)	MA Heptachlor	4.929	4.082	107.7E6	573.0E6	20.000	20.000
9)	A Endosulfan I	6.075	5.245	88718850	475.7E6	20.000	20.000
13)	MA Dieldrin	6.347	5.511	191.5E6	1026.0E6	40.000	40.000
14)	MA Endrin	6.574	5.788	161.4E6	937.6E6	40.000	40.000
16)	A 4,4'-DDD	6.705	5.928	135.5E6	839.5E6	40.000	40.000
17)	MA 4,4'-DDT	7.021	6.183	141.9E6	876.6E6	40.000	40.000
20)	A Methoxychlor	7.493	6.753	379.3E6	1980.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071725\
Data File : PD089518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2025 12:43
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 06:49:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071725CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 18 06:48:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

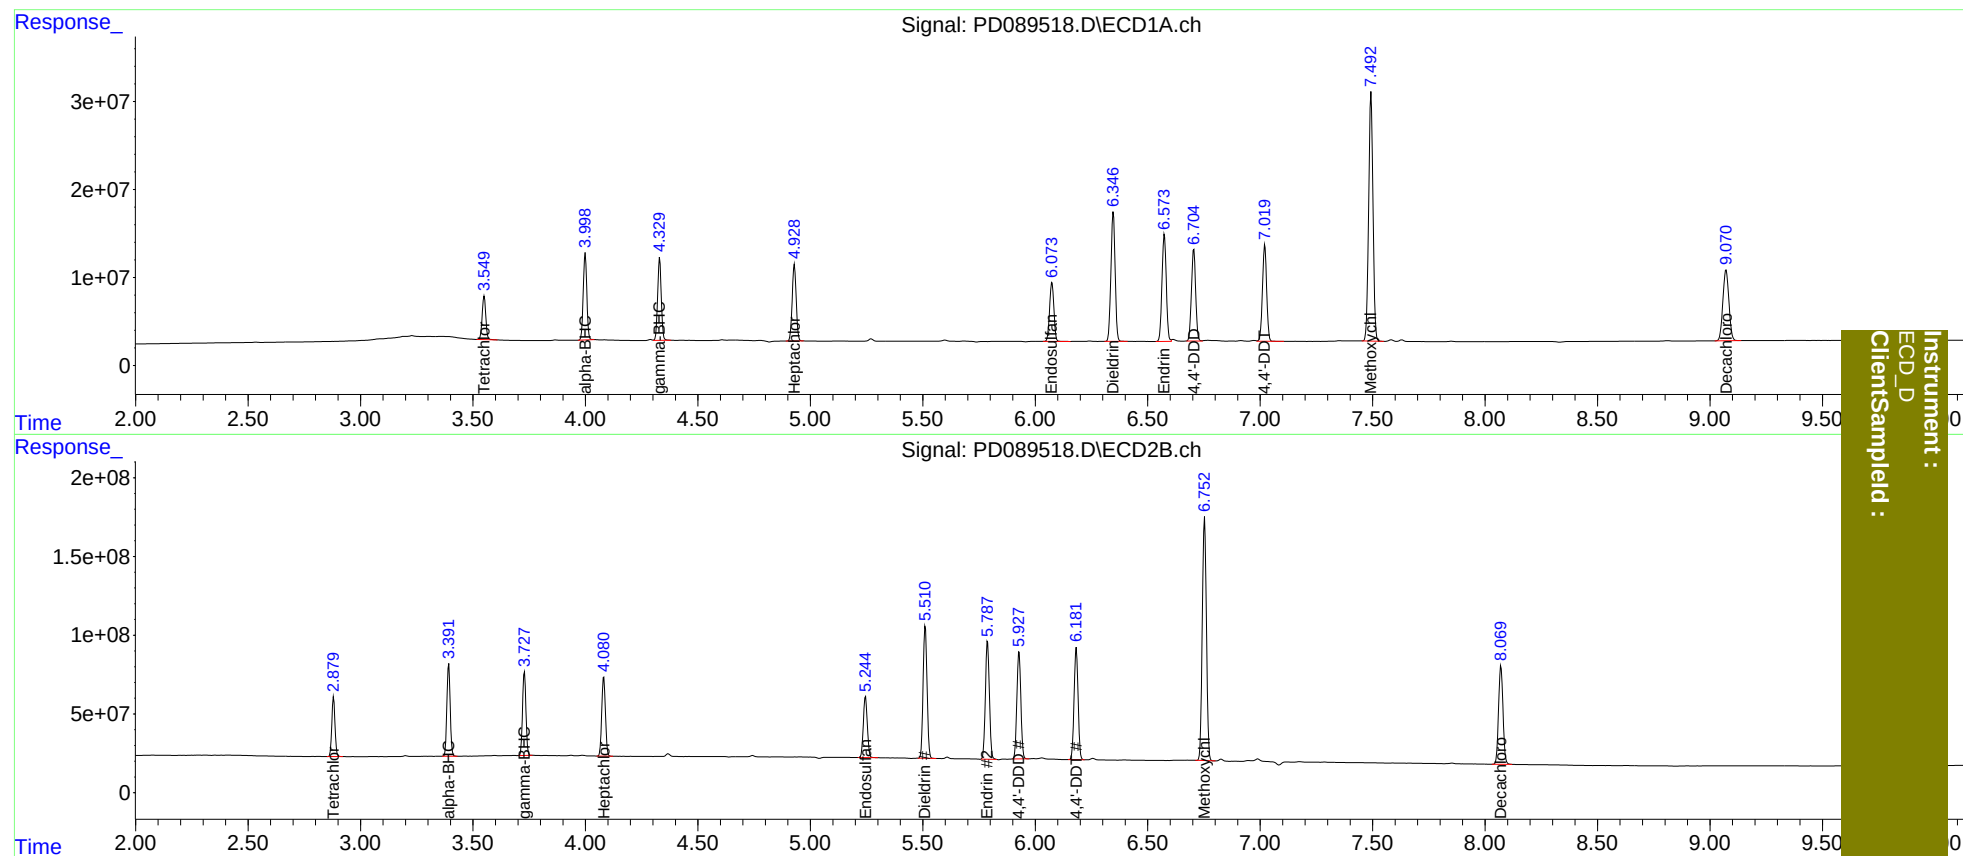


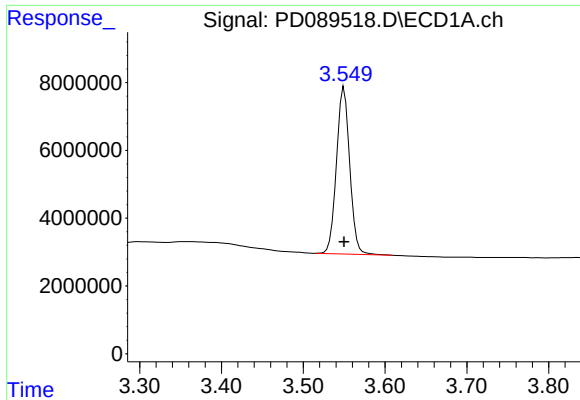

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 55290386
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

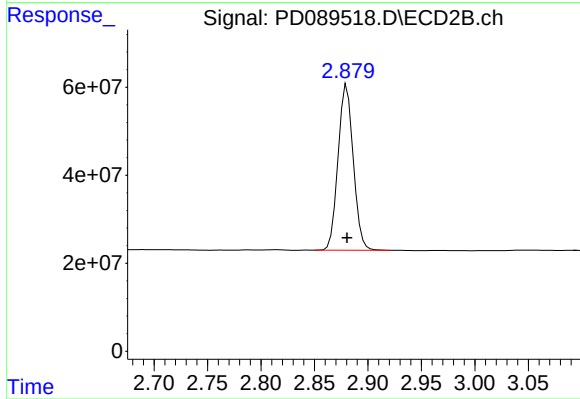


#1 Tetrachloro-m-xylene

R.T.: 2.880 min
Delta R.T.: 0.000 min
Response: 373252298
Conc: 20.00 ng/ml

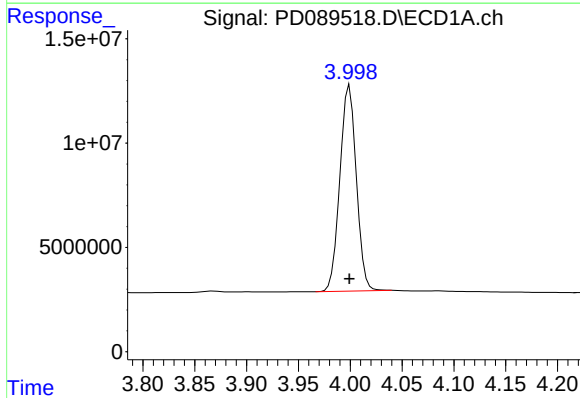


#2 alpha-BHC

R.T.: 3.999 min
Delta R.T.: 0.000 min
Response: 109183356
Conc: 20.00 ng/ml

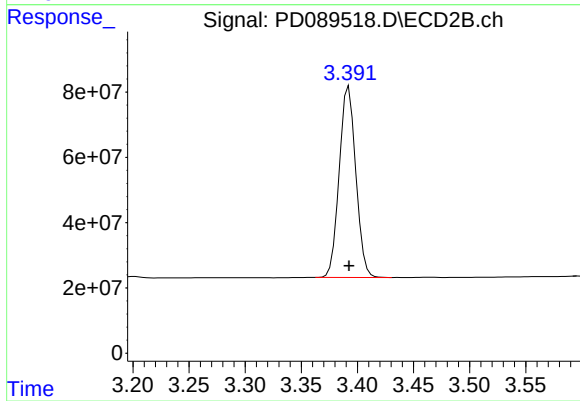

#2 alpha-BHC


R.T.: 3.392 min
Delta R.T.: 0.000 min
Response: 602415827
Conc: 20.00 ng/ml

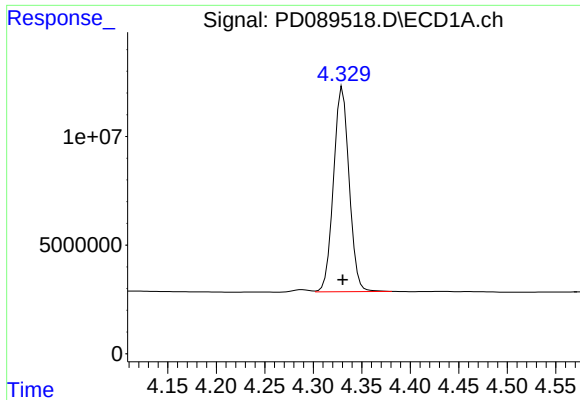

#3 gamma-BHC (Lindane)


R.T.: 4.330 min
Delta R.T.: 0.000 min
Response: 105437036
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

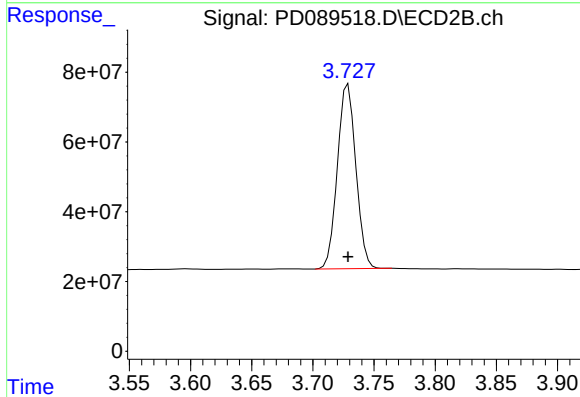


#3 gamma-BHC (Lindane)

R.T.: 3.729 min
Delta R.T.: 0.000 min
Response: 556176335
Conc: 20.00 ng/ml

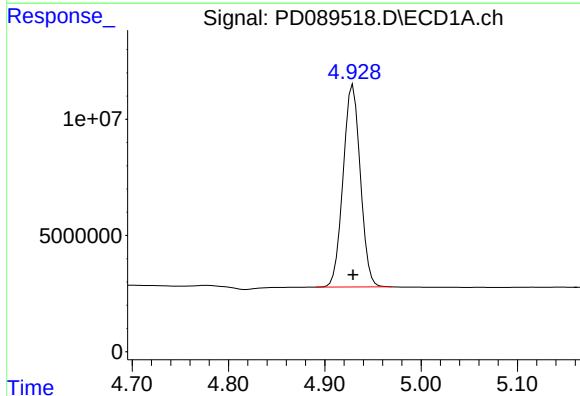


#4 Heptachlor

R.T.: 4.929 min
Delta R.T.: 0.000 min
Response: 107703615
Conc: 20.00 ng/ml

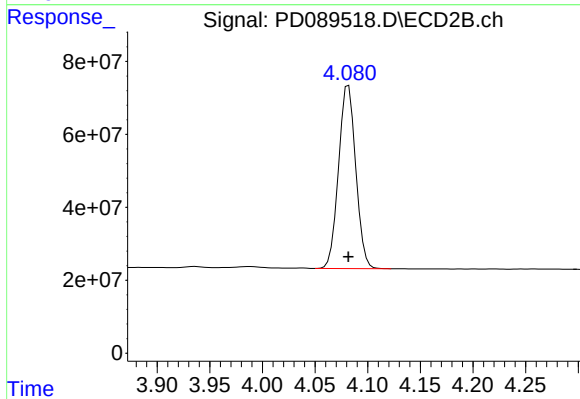

#4 Heptachlor


R.T.: 4.082 min
Delta R.T.: 0.000 min
Response: 572983857
Conc: 20.00 ng/ml

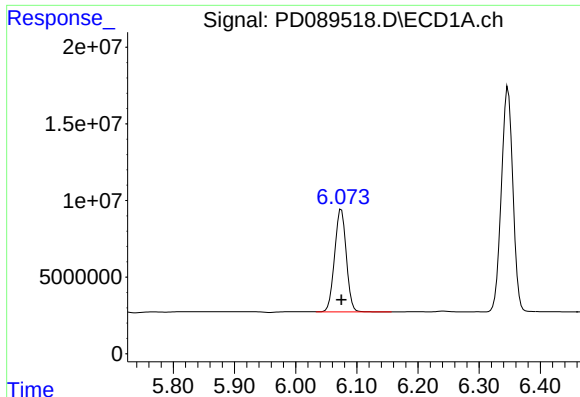

#9 Endosulfan I


R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 88718850
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

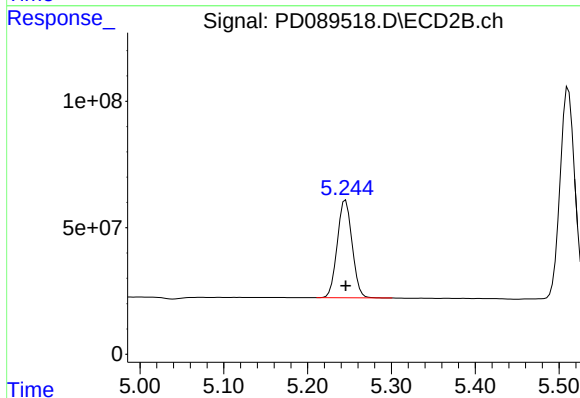


#9 Endosulfan I

R.T.: 5.245 min
Delta R.T.: 0.000 min
Response: 475691990
Conc: 20.00 ng/ml

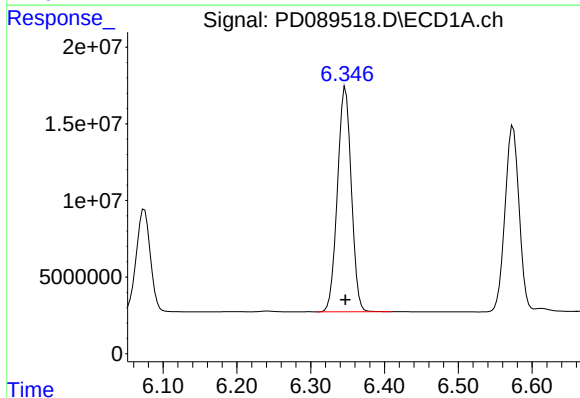


#13 Dieldrin

R.T.: 6.347 min
Delta R.T.: 0.000 min
Response: 191524147
Conc: 40.00 ng/ml

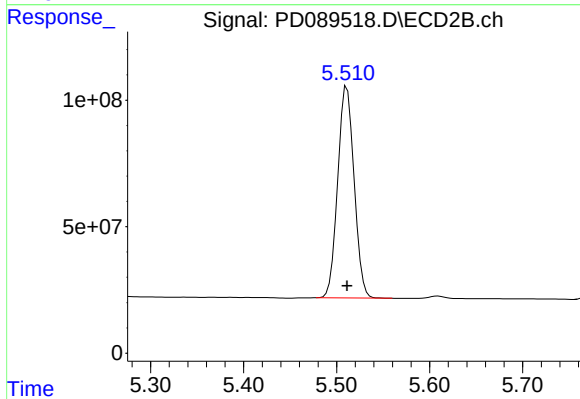

#13 Dieldrin


R.T.: 5.511 min
Delta R.T.: 0.000 min
Response: 1025959270
Conc: 40.00 ng/ml

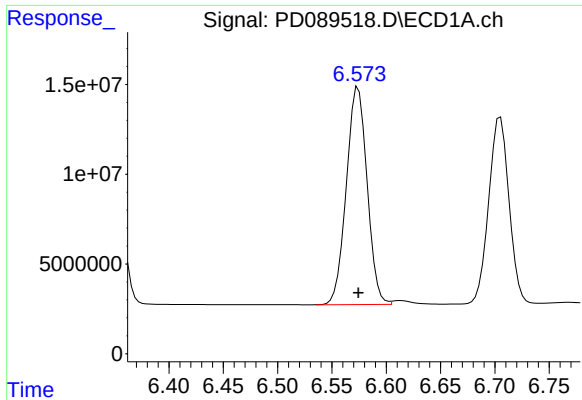

#14 Endrin


R.T.: 6.574 min
Delta R.T.: 0.000 min
Response: 161442041
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

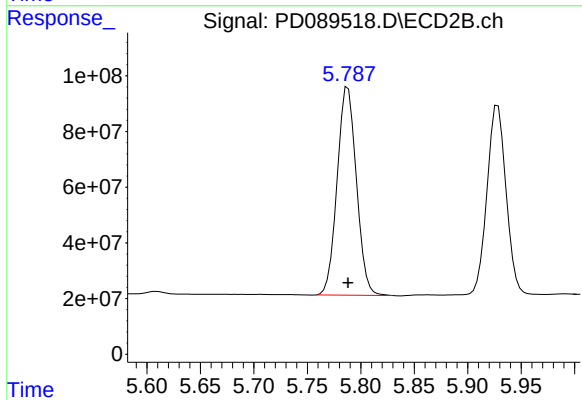


#14 Endrin

R.T.: 5.788 min
Delta R.T.: 0.000 min
Response: 937648580
Conc: 40.00 ng/ml

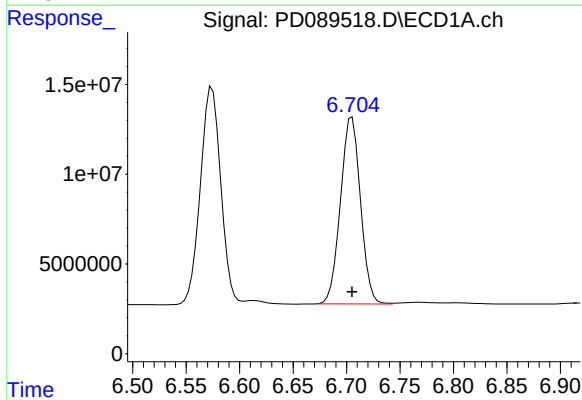


#16 4,4'-DDD

R.T.: 6.705 min
Delta R.T.: 0.000 min
Response: 135532904
Conc: 40.00 ng/ml

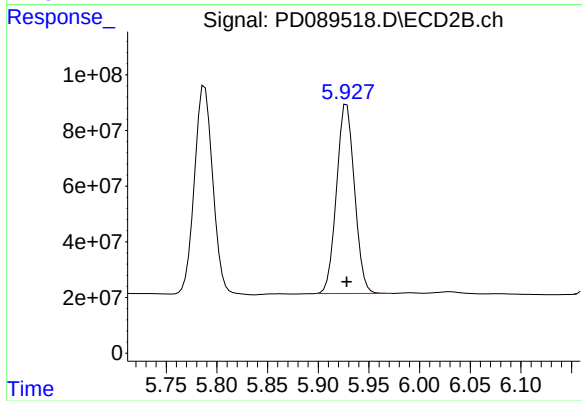

#16 4,4'-DDD


R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 839504693
Conc: 40.00 ng/ml

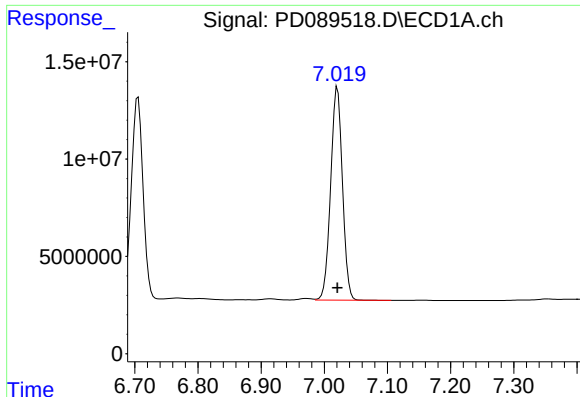

#17 4,4'-DDT


R.T.: 7.021 min
Delta R.T.: 0.000 min
Response: 141881825
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

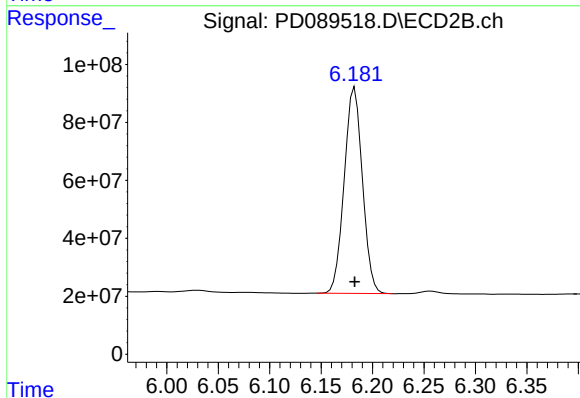


#17 4,4'-DDT

R.T.: 6.183 min
Delta R.T.: 0.000 min
Response: 876564902
Conc: 40.00 ng/ml

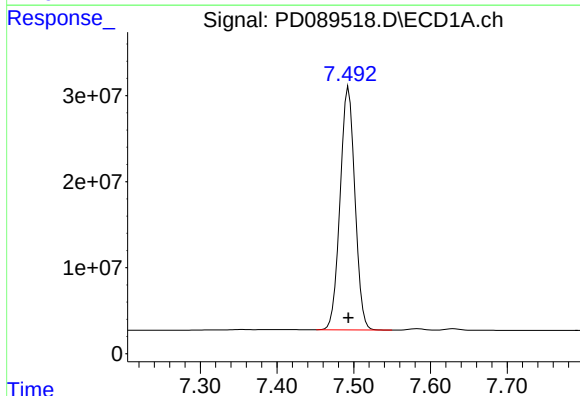


#20 Methoxychlor

R.T.: 7.493 min
Delta R.T.: 0.000 min
Response: 379306558
Conc: 200.00 ng/ml

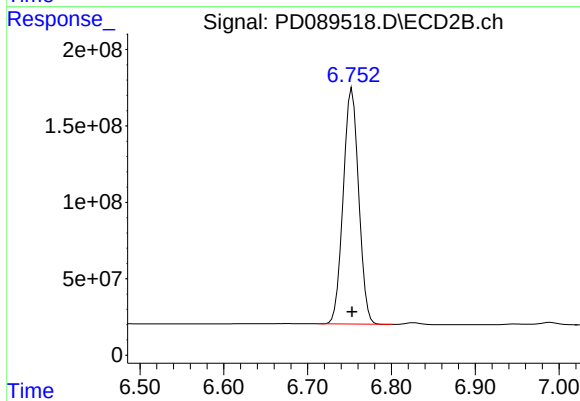

#20 Methoxychlor


R.T.: 6.753 min
Delta R.T.: 0.000 min
Response: 1980713598
Conc: 200.00 ng/ml

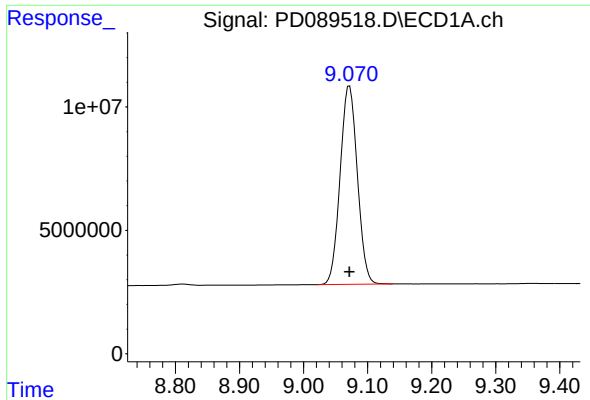

#27 Decachlorobiphenyl

R.T.: 9.072 min
Delta R.T.: 0.000 min
Response: 149949315
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

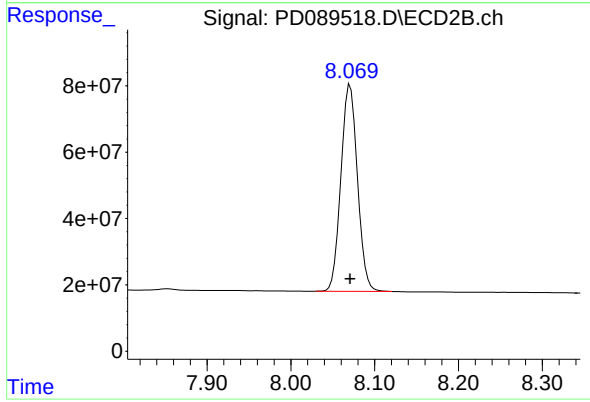

#27 Decachlorobiphenyl

R.T.: 8.071 min
Delta R.T.: 0.000 min
Response: 855715150
Conc: 40.00 ng/ml