

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071725\
 Data File : PD089522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2025 13:38
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 06:50:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071725CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 18 06:48:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.880	216.3E6	1359.5E6	78.231	72.845
27)	SA Decachlor...	9.072	8.071	556.2E6	3180.1E6	148.359	148.653
Target Compounds							
2)	A alpha-BHC	3.999	3.392	489.1E6	2269.6E6	89.595	75.348
3)	MA gamma-BHC...	4.330	3.729	456.5E6	2083.4E6	86.598	74.917
4)	MA Heptachlor	4.929	4.082	454.3E6	2087.4E6	84.367	72.860
9)	A Endosulfan I	6.074	5.246	359.0E6	1715.2E6	80.919	72.113
13)	MA Dieldrin	6.346	5.512	815.3E6	3717.0E6	170.280	144.918
14)	MA Endrin	6.573	5.788	686.9E6	3361.7E6	170.186	143.410
16)	A 4,4'-DDD	6.705	5.929	583.6E6	3059.6E6	172.240	145.779
17)	MA 4,4'-DDT	7.020	6.182	611.5E6	3261.9E6	172.397	148.849
20)	A Methoxychlor	7.493	6.753	1486.4E6	6124.9E6	783.735	618.454


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071725\
Data File : PD089522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2025 13:38
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 06:50:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071725CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 18 06:48:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

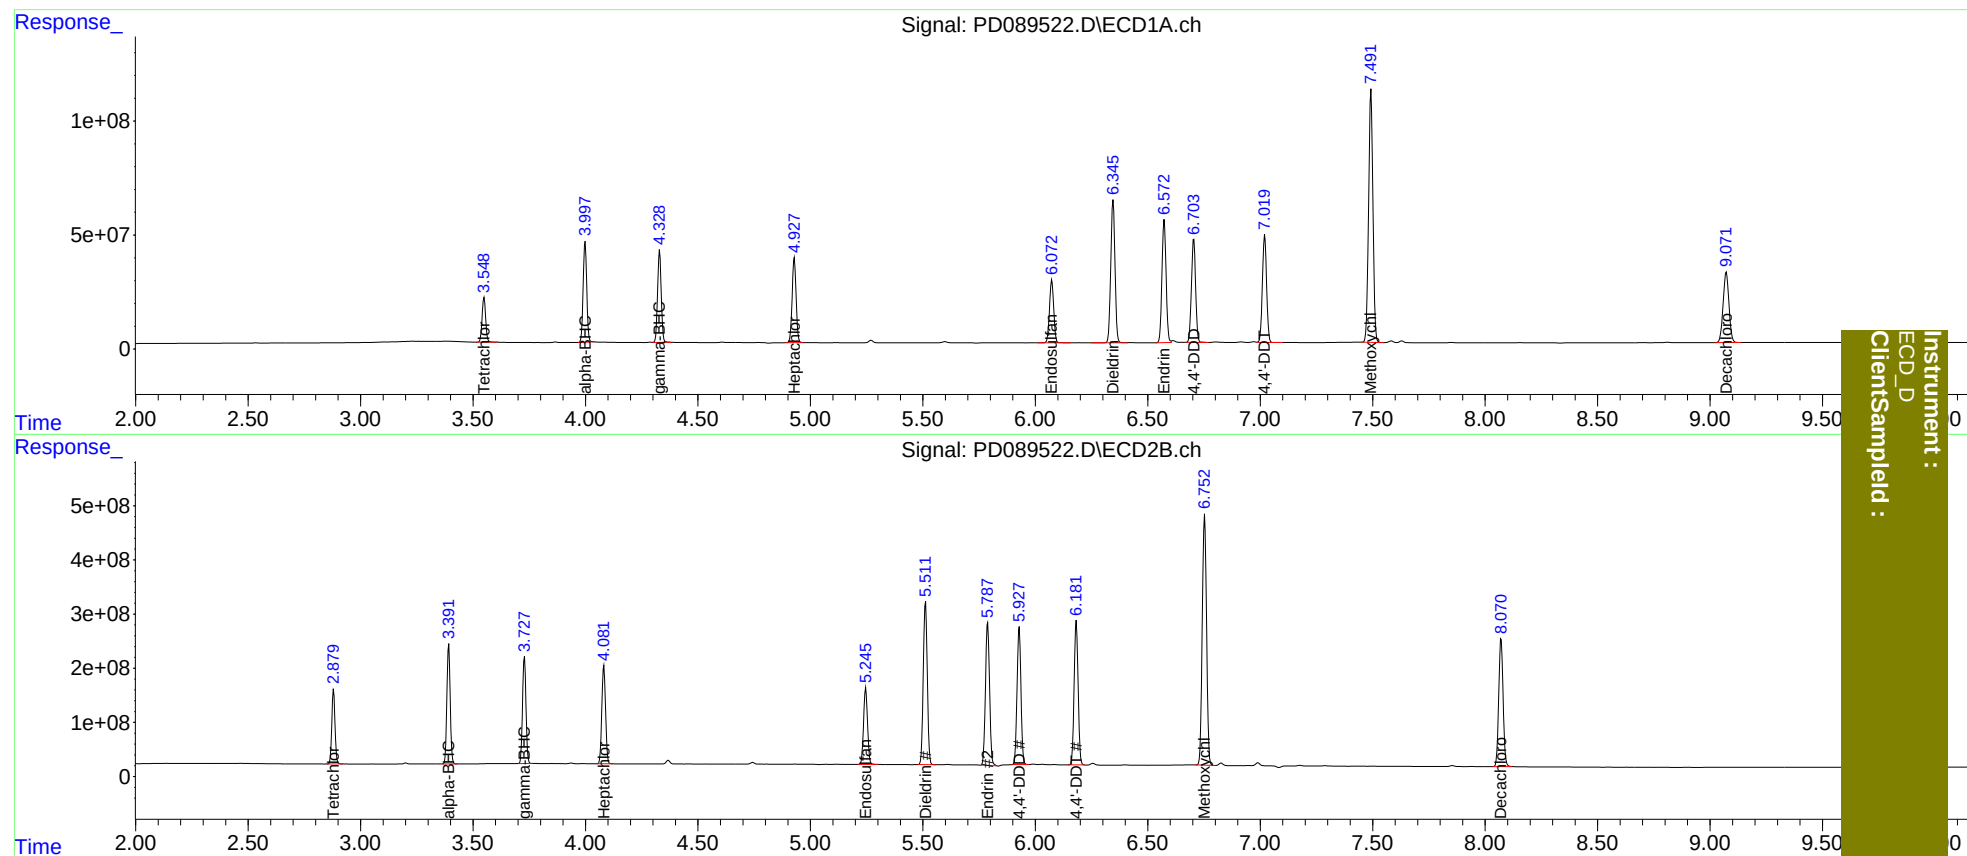


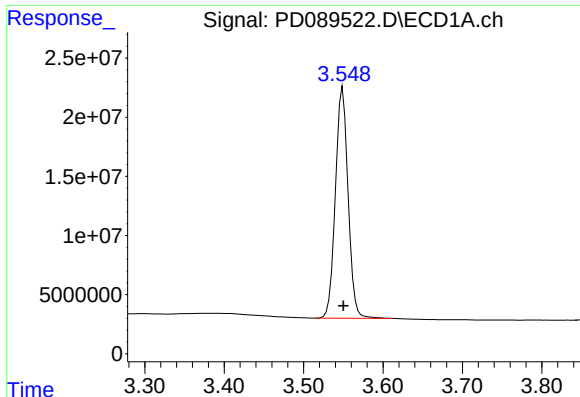

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 216269949
Conc: 78.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

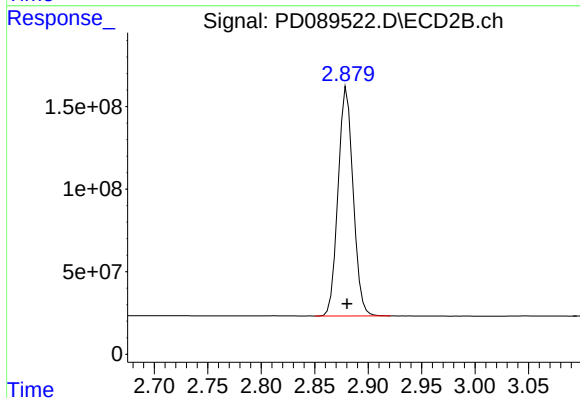


#1 Tetrachloro-m-xylene

R.T.: 2.880 min
Delta R.T.: 0.000 min
Response: 1359471240
Conc: 72.84 ng/ml

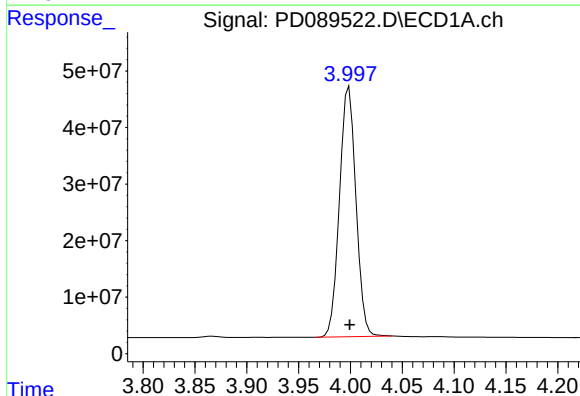


#2 alpha-BHC

R.T.: 3.999 min
Delta R.T.: 0.000 min
Response: 489116266
Conc: 89.60 ng/ml

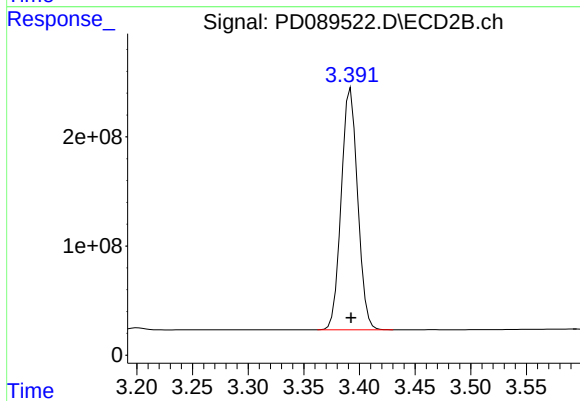

#2 alpha-BHC


R.T.: 3.392 min
Delta R.T.: 0.000 min
Response: 2269550051
Conc: 75.35 ng/ml

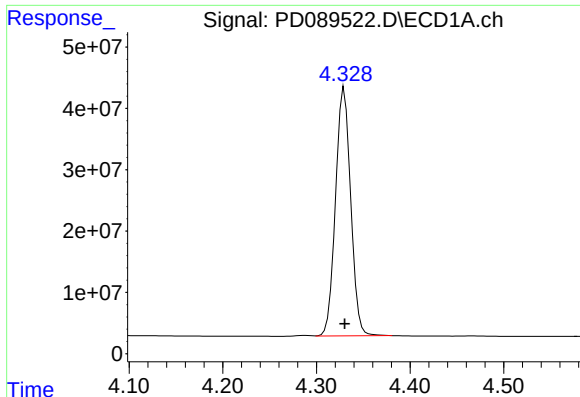

#3 gamma-BHC (Lindane)


R.T.: 4.330 min
Delta R.T.: 0.000 min
Response: 456533627
Conc: 86.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

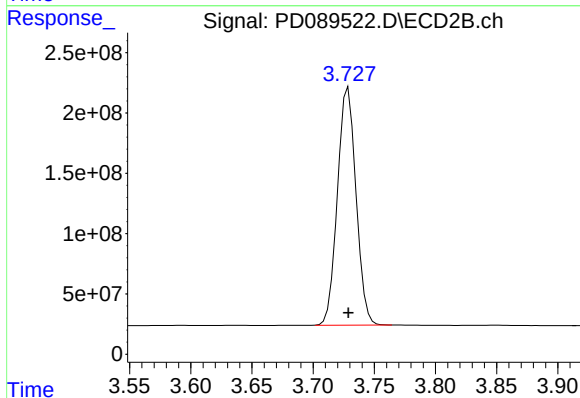


#3 gamma-BHC (Lindane)

R.T.: 3.729 min
Delta R.T.: 0.000 min
Response: 2083355643
Conc: 74.92 ng/ml

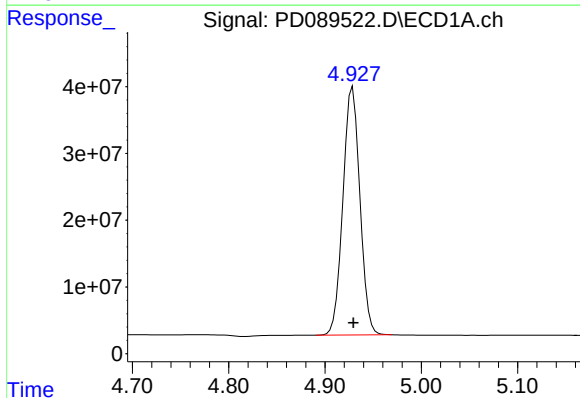


#4 Heptachlor

R.T.: 4.929 min
Delta R.T.: 0.000 min
Response: 454333728
Conc: 84.37 ng/ml

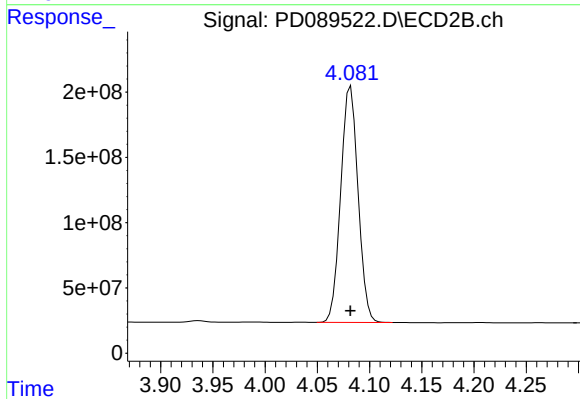

#4 Heptachlor


R.T.: 4.082 min
Delta R.T.: 0.000 min
Response: 2087371243
Conc: 72.86 ng/ml

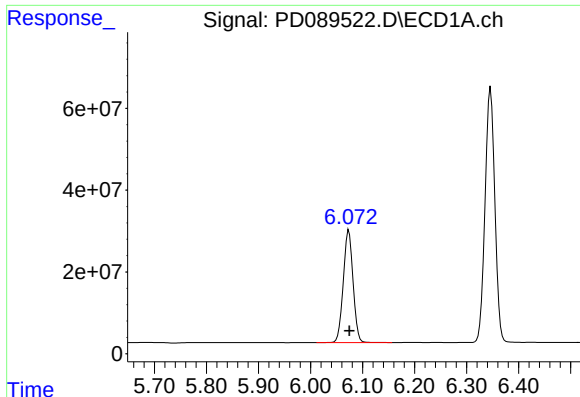

#9 Endosulfan I


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 358952053
Conc: 80.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

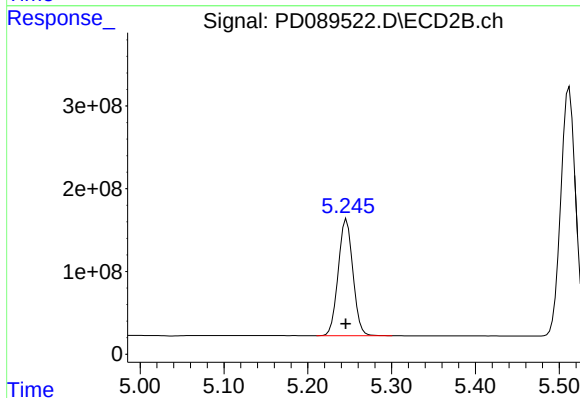


#9 Endosulfan I

R.T.: 5.246 min
Delta R.T.: 0.000 min
Response: 1715171555
Conc: 72.11 ng/ml

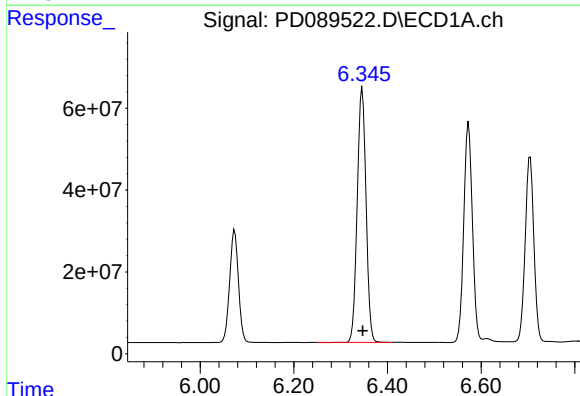


#13 Dieldrin

R.T.: 6.346 min
Delta R.T.: -0.001 min
Response: 815317554
Conc: 170.28 ng/ml

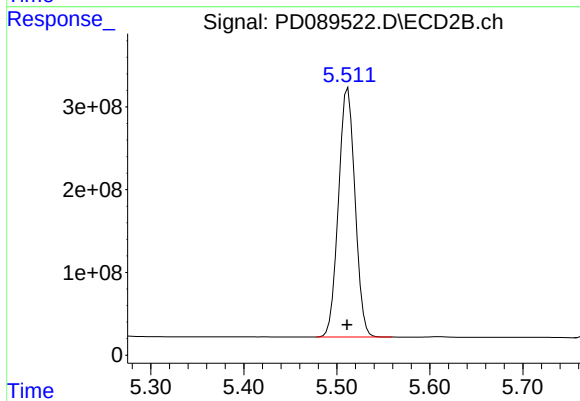

#13 Dieldrin


R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 3716989153
Conc: 144.92 ng/ml

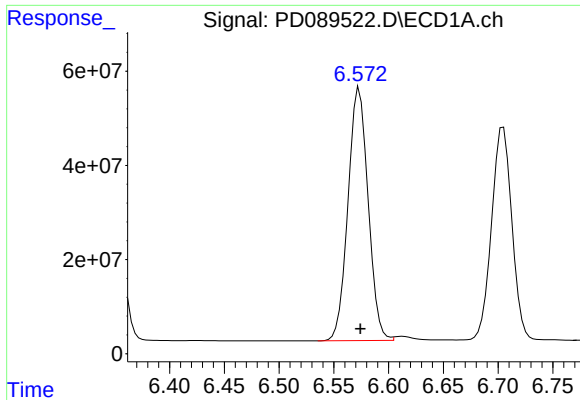

#14 Endrin


R.T.: 6.573 min
Delta R.T.: 0.000 min
Response: 686878898
Conc: 170.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

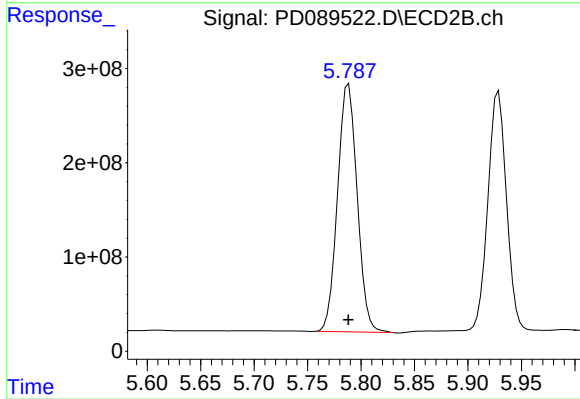


#14 Endrin

R.T.: 5.788 min
Delta R.T.: 0.000 min
Response: 3361706885
Conc: 143.41 ng/ml

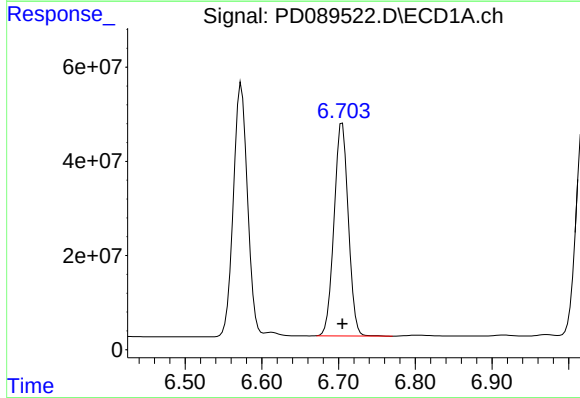


#16 4,4'-DDD

R.T.: 6.705 min
Delta R.T.: 0.000 min
Response: 583603455
Conc: 172.24 ng/ml

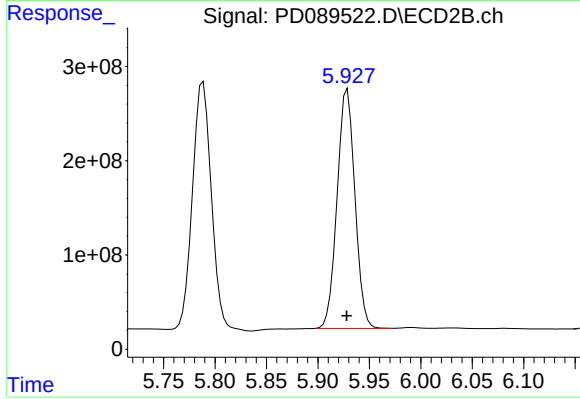

#16 4,4'-DDD


R.T.: 5.929 min
Delta R.T.: 0.000 min
Response: 3059554422
Conc: 145.78 ng/ml

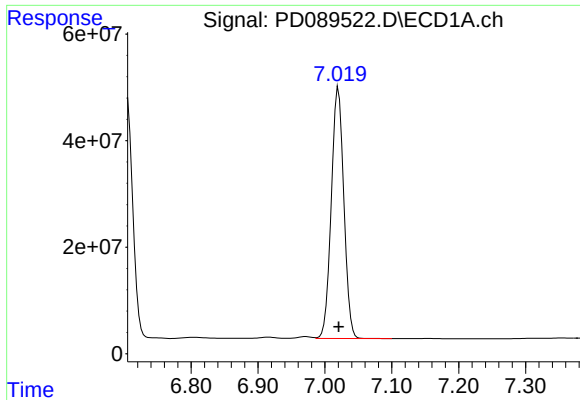

#17 4,4'-DDT


R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 611500604
Conc: 172.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

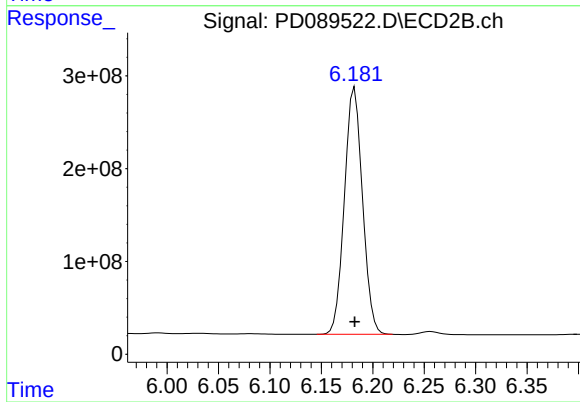


#17 4,4'-DDT

R.T.: 6.182 min
Delta R.T.: 0.000 min
Response: 3261899005
Conc: 148.85 ng/ml

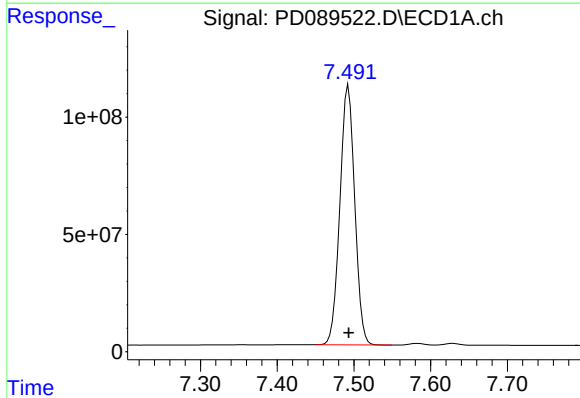


#20 Methoxychlor

R.T.: 7.493 min
Delta R.T.: 0.000 min
Response: 1486379086
Conc: 783.73 ng/ml

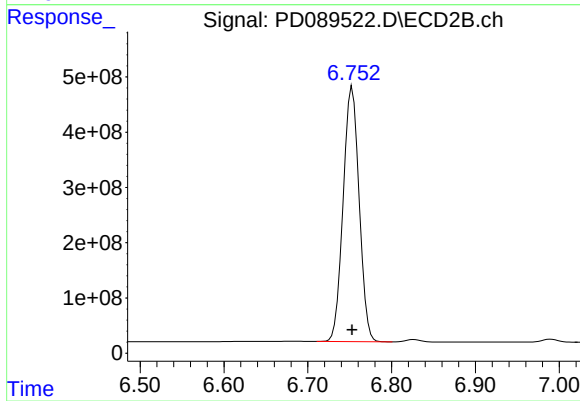

#20 Methoxychlor


R.T.: 6.753 min
Delta R.T.: 0.000 min
Response: 6124900577
Conc: 618.45 ng/ml

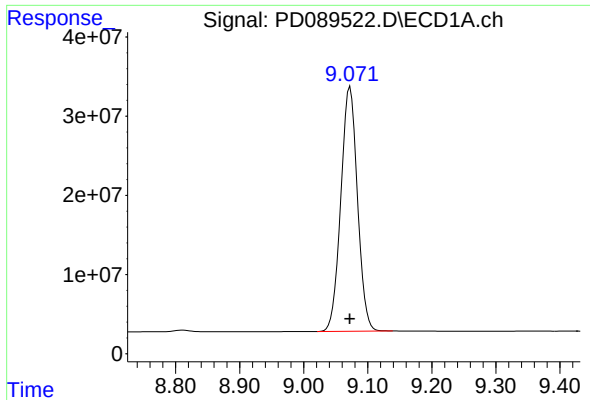

#27 Decachlorobiphenyl

R.T.: 9.072 min
Delta R.T.: 0.000 min
Response: 556159578
Conc: 148.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

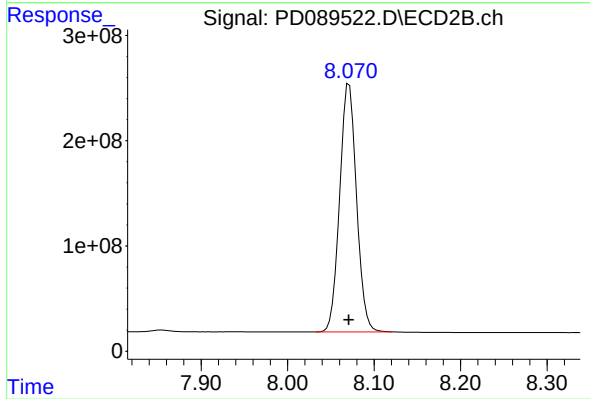

#27 Decachlorobiphenyl

R.T.: 8.071 min
Delta R.T.: 0.000 min
Response: 3180120471
Conc: 148.65 ng/ml