

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071822\
 Data File : PD070959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2022 10:36
 Operator : AR\AJ
 Sample : PB146258BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS258

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/20/2022
 Supervised By :Ankita Jodhani 07/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 09:24:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.482	4.126	46325020	496.6E6	19.253	21.160
27)	SA Decachlor...	8.255	9.325	101.3E6	401.4E6	39.890	43.460
Target Compounds							
2)	A alpha-BHC	3.924	4.530	14088125	179.6E6	3.755	5.952 #
3)	MA gamma-BHC...	4.208	4.823	15952643	152.2E6	4.382	5.883m#
4)	MA Heptachlor	4.507	5.340	16270014	119.6E6	4.669m	5.968 #
5)	MB Aldrin	4.756	5.654	16869568	102.9E6	4.668m	5.912 #
6)	B beta-BHC	4.457	5.000	7358119	66108768	4.697m	4.943
7)	B delta-BHC	4.664	5.224	11729695	102.4E6	3.367	4.513 #
8)	B Heptachlo...	5.203	6.049	15963828	86751410	4.795	5.842
9)	A Endosulfan I	5.543	6.413	15006750	78255191	4.978	5.901
10)	B trans-Chl...	5.430	6.286	16483652	87713883	4.736	5.825
11)	B cis-Chlor...	5.489	6.359	16467798	80243065	4.818	5.556
12)	B 4,4'-DDE	5.655	6.514	29636147	158.6E6	9.211	11.563 #
13)	MA Dieldrin	5.787	6.675	31119749	170.5E6	9.293	12.312 #
14)	MA Endrin	6.046	6.898	25699451	121.2E6	9.270	11.603 #
15)	B Endosulfa...	6.320	7.112	26619423	147.2E6	9.707	12.782 #
16)	A 4,4'-DDD	6.173	7.013	24912869	138.1E6	9.566	12.627m#
17)	MA 4,4'-DDT	6.415	7.315	23498495	124.8E6	8.783	11.151 #
18)	B Endrin al...	6.490	7.239	23283362	116.1E6	10.164	11.938
19)	B Endosulfa...	6.703	7.463	24493055	117.8E6	8.744	10.387
20)	A Methoxychlor	6.966	7.775	65875210	300.7E6	47.639	57.472
21)	B Endrin ke...	7.197	7.944	32452501	152.4E6	10.469	12.346

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071822\
Data File : PD070959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2022 10:36
Operator : AR\AJ
Sample : PB146258BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 09:24:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

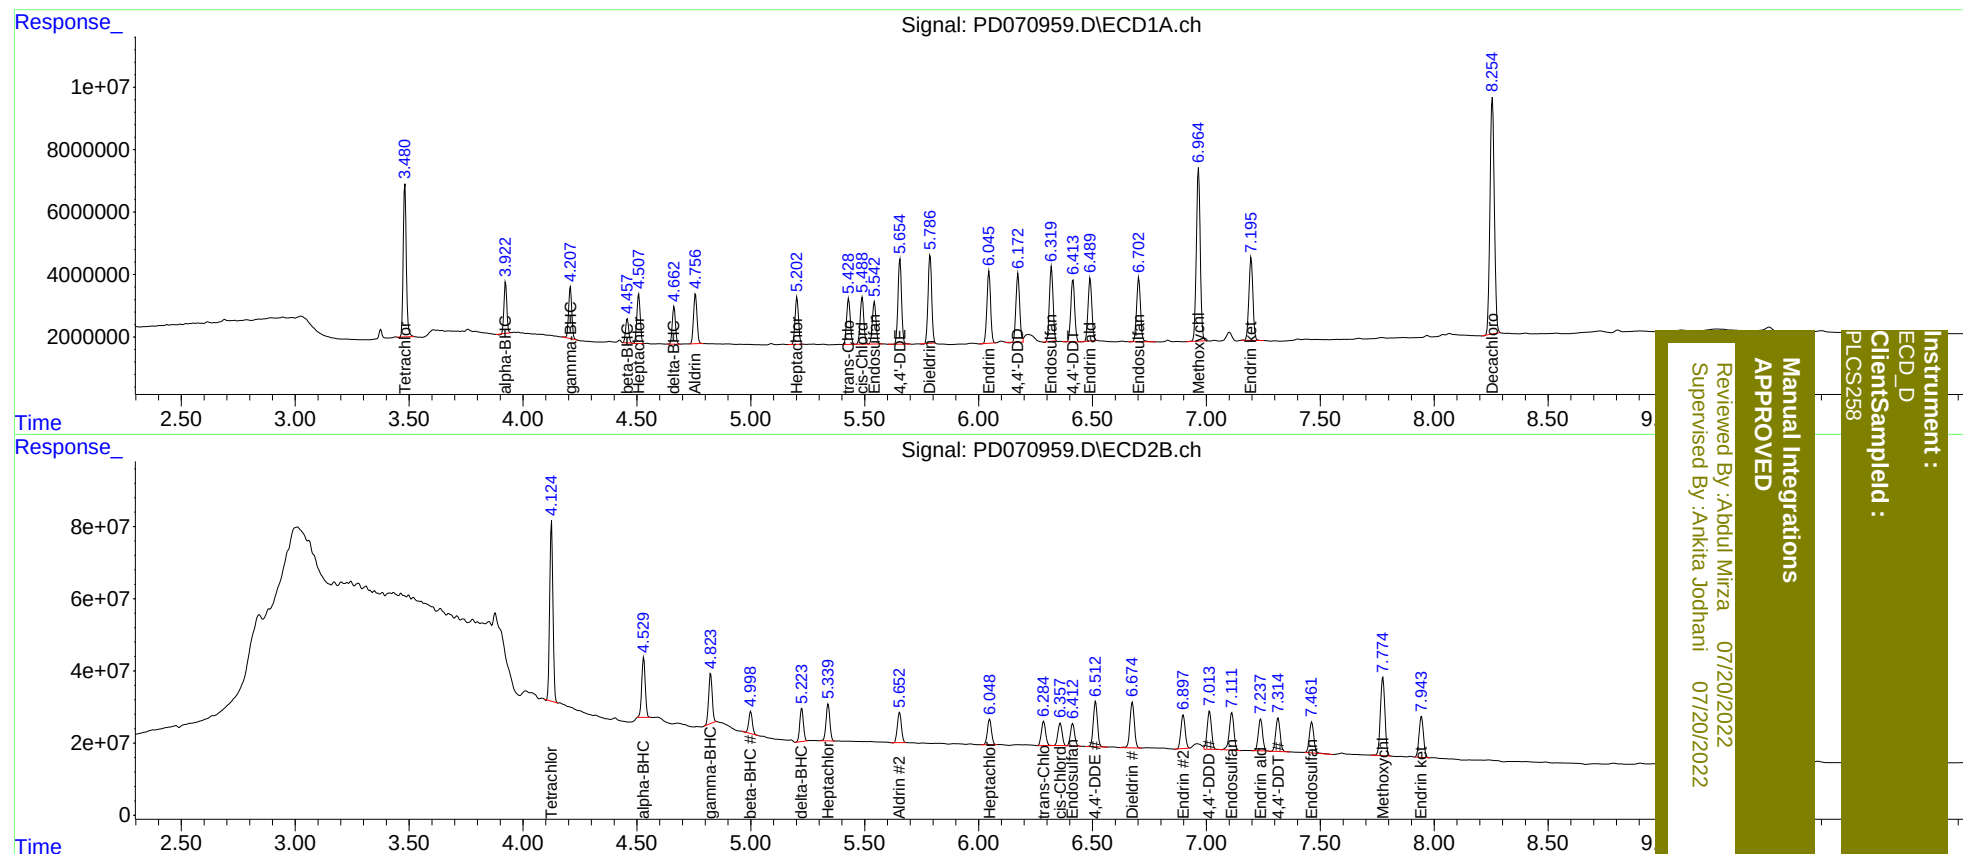

Reviewed By: Abdul Mirza 07/20/2022
Supervised By: Ankita Jodhani 07/20/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
PLCS258