

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071822\
 Data File : PD070970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2022 17:58
 Operator : AR\AJ
 Sample : N3710-08MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 H0B06MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:05:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.124	43800359	463.6E6	18.204	19.754
27)	SA Decachlor...	8.243	9.320	70619677	274.3E6	27.816	29.703
Target Compounds							
2)	A alpha-BHC	3.915	4.529	165.8E6	1264.8E6	44.198	41.904
3)	MA gamma-BHC...	4.199	4.823	151.7E6	1082.0E6	41.679	41.811
4)	MA Heptachlor	4.499	5.339	139.8E6	750.0E6	40.119	37.421
5)	MB Aldrin	4.748	5.652	142.6E6	638.9E6	39.451	36.709
6)	B beta-BHC	4.448	4.999	58278434	440.4E6	37.199	32.933
7)	B delta-BHC	4.654	5.223	144.5E6	874.3E6	41.467	38.548
8)	B Heptachlo...	5.192	6.047	135.7E6	558.1E6	40.744	37.578
9)	A Endosulfan I	5.532	6.411	127.5E6	515.5E6	42.294	38.871
10)	B trans-Chl...	5.419	6.283	136.7E6	547.9E6	39.279	36.389
11)	B cis-Chlor...	5.478	6.356	136.7E6	532.0E6	39.995	36.836
12)	B 4,4'-DDE	5.644	6.511	252.4E6	1057.8E6	78.447	77.121
13)	MA Dieldrin	5.776	6.672	290.3E6	1125.0E6	86.679	81.243
14)	MA Endrin	6.034	6.896	265.9E6	942.2E6	95.912	90.242
15)	B Endosulfa...	6.308	7.110	234.5E6	922.5E6	85.492	80.087
16)	A 4,4'-DDD	6.161	7.011	205.8E6	894.9E6	79.031	81.821
17)	MA 4,4'-DDT	6.402	7.312	229.7E6	921.1E6	85.846	82.301
18)	B Endrin al...	6.478	7.236	177.0E6	721.5E6	77.274	74.213
19)	B Endosulfa...	6.691	7.460	220.5E6	858.9E6	78.717	75.759
20)	A Methoxychlor	6.953	7.772	585.6E6	2160.3E6	423.482	412.905
21)	B Endrin ke...	7.185	7.941	261.4E6	996.7E6	84.309	80.718

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071822\
Data File : PD070970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2022 17:58
Operator : AR\AJ
Sample : N3710-08MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:05:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

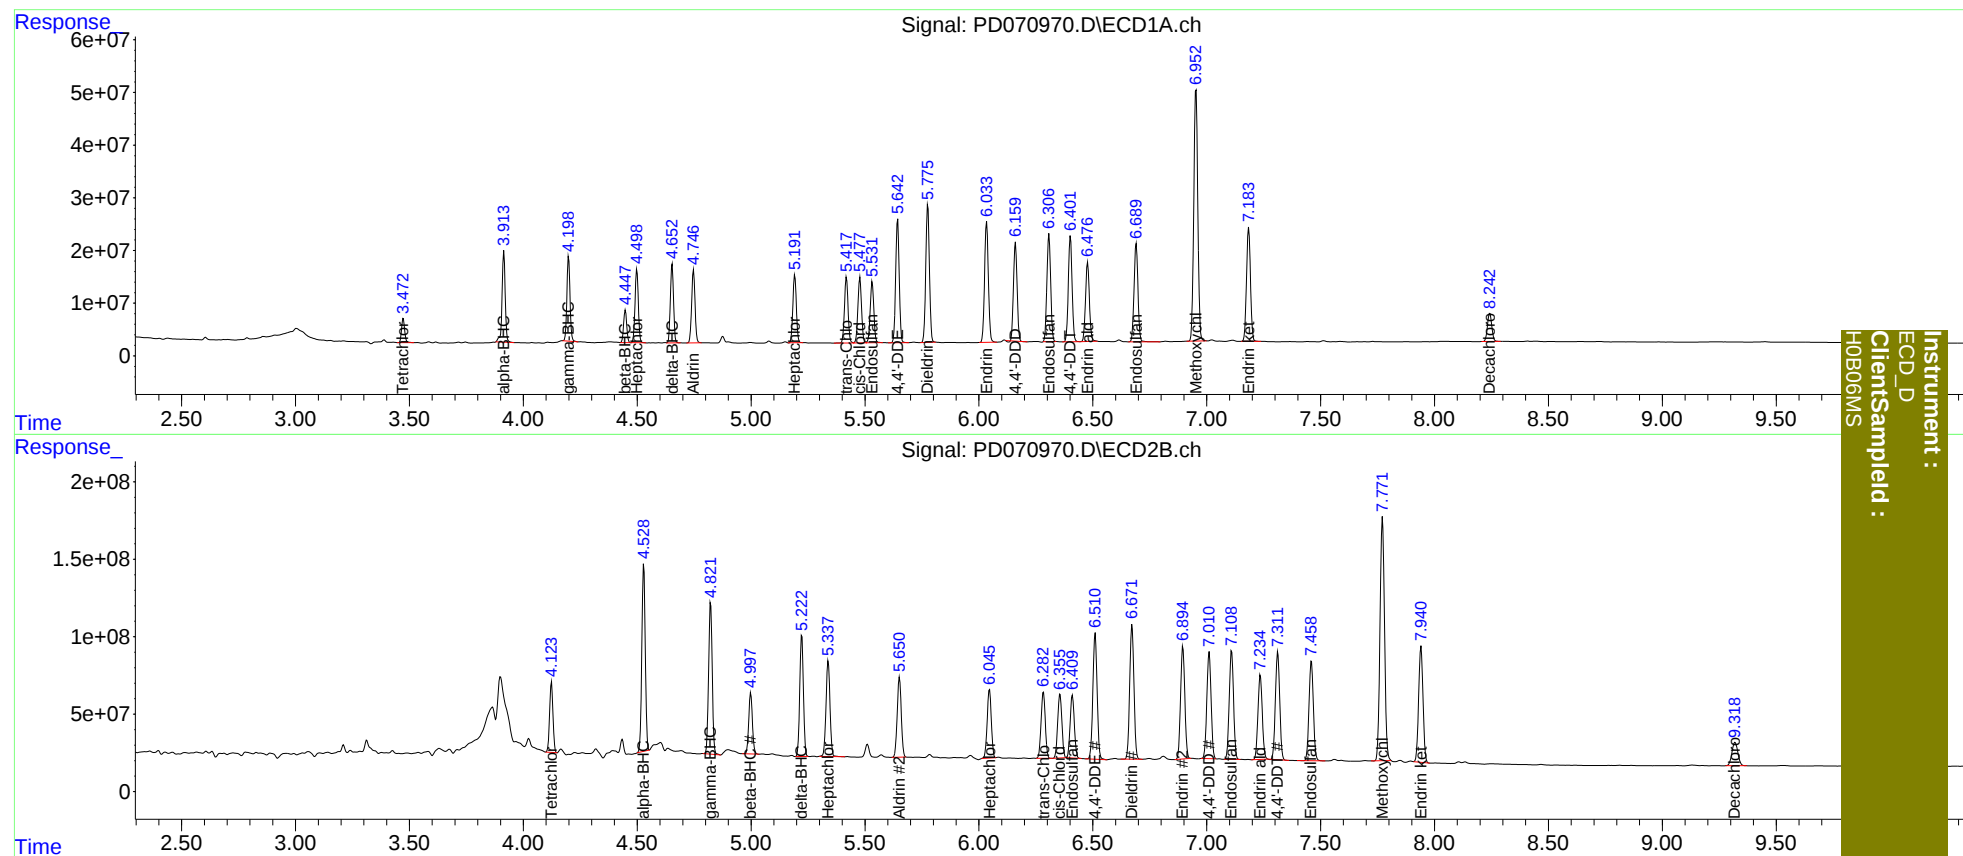

Instrument :
ECD_D
ClientSampled :
HOB06MS