

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071822\
 Data File : PD070971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2022 18:13
 Operator : AR\AJ
 Sample : N3710-09MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 H0B06MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/19/2022
 Supervised By : Ankita Jodhani 07/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:05:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.124	51516257	534.5E6	21.410	22.775
27)	SA Decachlor...	8.243	9.319	83194796	319.6E6	32.769	34.603
Target Compounds							
2)	A alpha-BHC	3.915	4.529	195.1E6	1461.1E6	52.020	48.409
3)	MA gamma-BHC...	4.199	4.823	178.6E6	1246.8E6	49.069	48.181
4)	MA Heptachlor	4.499	5.339	166.9E6	861.7E6	47.912	42.994
5)	MB Aldrin	4.747	5.652	169.1E6	742.7E6	46.800	42.674
6)	B beta-BHC	4.448	4.999	68104153	498.3E6	43.470	37.262
7)	B delta-BHC	4.653	5.223	172.3E6	1012.1E6	49.471	44.622
8)	B Heptachlo...	5.192	6.046	161.5E6	643.1E6	48.493	43.303
9)	A Endosulfan I	5.531	6.411	151.0E6	596.2E6	50.092	44.961
10)	B trans-Chl...	5.419	6.283	162.2E6	633.5E6	46.608	42.070
11)	B cis-Chlor...	5.478	6.356	161.8E6	613.4E6	47.352	42.472
12)	B 4,4'-DDE	5.644	6.511	300.3E6	1232.1E6	93.327	89.835
13)	MA Dieldrin	5.777	6.672	344.9E6	1309.8E6	103.004	94.591
14)	MA Endrin	6.035	6.896	316.8E6	1097.2E6	114.277	105.086
15)	B Endosulfa...	6.308	7.110	279.4E6	1072.2E6	101.881	93.087
16)	A 4,4'-DDD	6.160	7.011	255.8E6	1036.2E6	98.235m	94.748
17)	MA 4,4'-DDT	6.403	7.312	274.1E6	1078.3E6	102.459	96.351
18)	B Endrin al...	6.478	7.235	208.5E6	838.3E6	91.024	86.225
19)	B Endosulfa...	6.691	7.460	261.0E6	1005.0E6	93.166	88.646
20)	A Methoxychlor	6.954	7.772	693.9E6	2527.2E6	501.820	483.017
21)	B Endrin ke...	7.185	7.941	310.4E6	1162.7E6	100.135	94.156

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071822\
Data File : PD070971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2022 18:13
Operator : AR\AJ
Sample : N3710-09MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:05:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

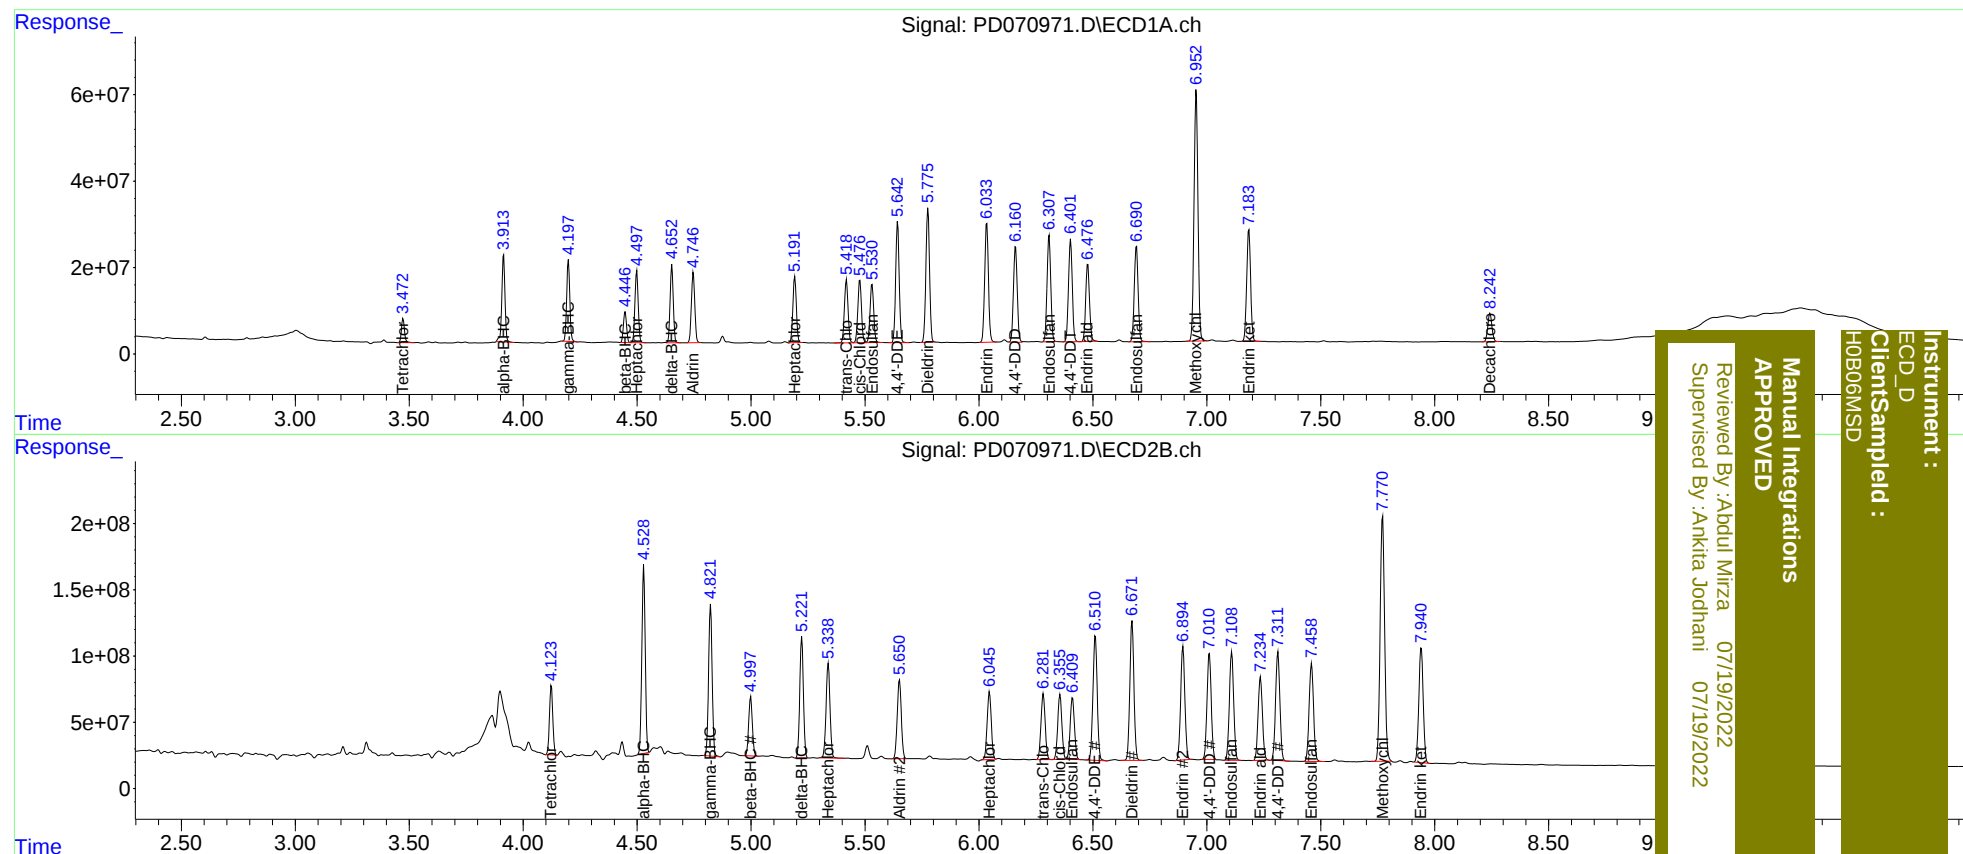

Instrument :
ECD_D
ClientSampled :
H0B06MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 07/19/2022
Supervised By: Ankita Jodhani 07/19/2022