

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071823\
 Data File : PD076873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2023 08:46
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 07:24:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	0.000	7.948	0	144621	N.D.	0.135
Target Compounds							
17)	MA 4,4'-DDT	6.986f	0.000	353377	0	0.158	N.D. #
18)	B Endrin al...	6.986f	0.000	353377	0	0.189	N.D. #
20)	A Methoxychlor	0.000	6.562f	0	217275	N.D.	0.407
25)	Toxaphene-4	0.000	6.562	0	217275	N.D.	8.660


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071823\
Data File : PD076873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2023 08:46
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 07:24:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

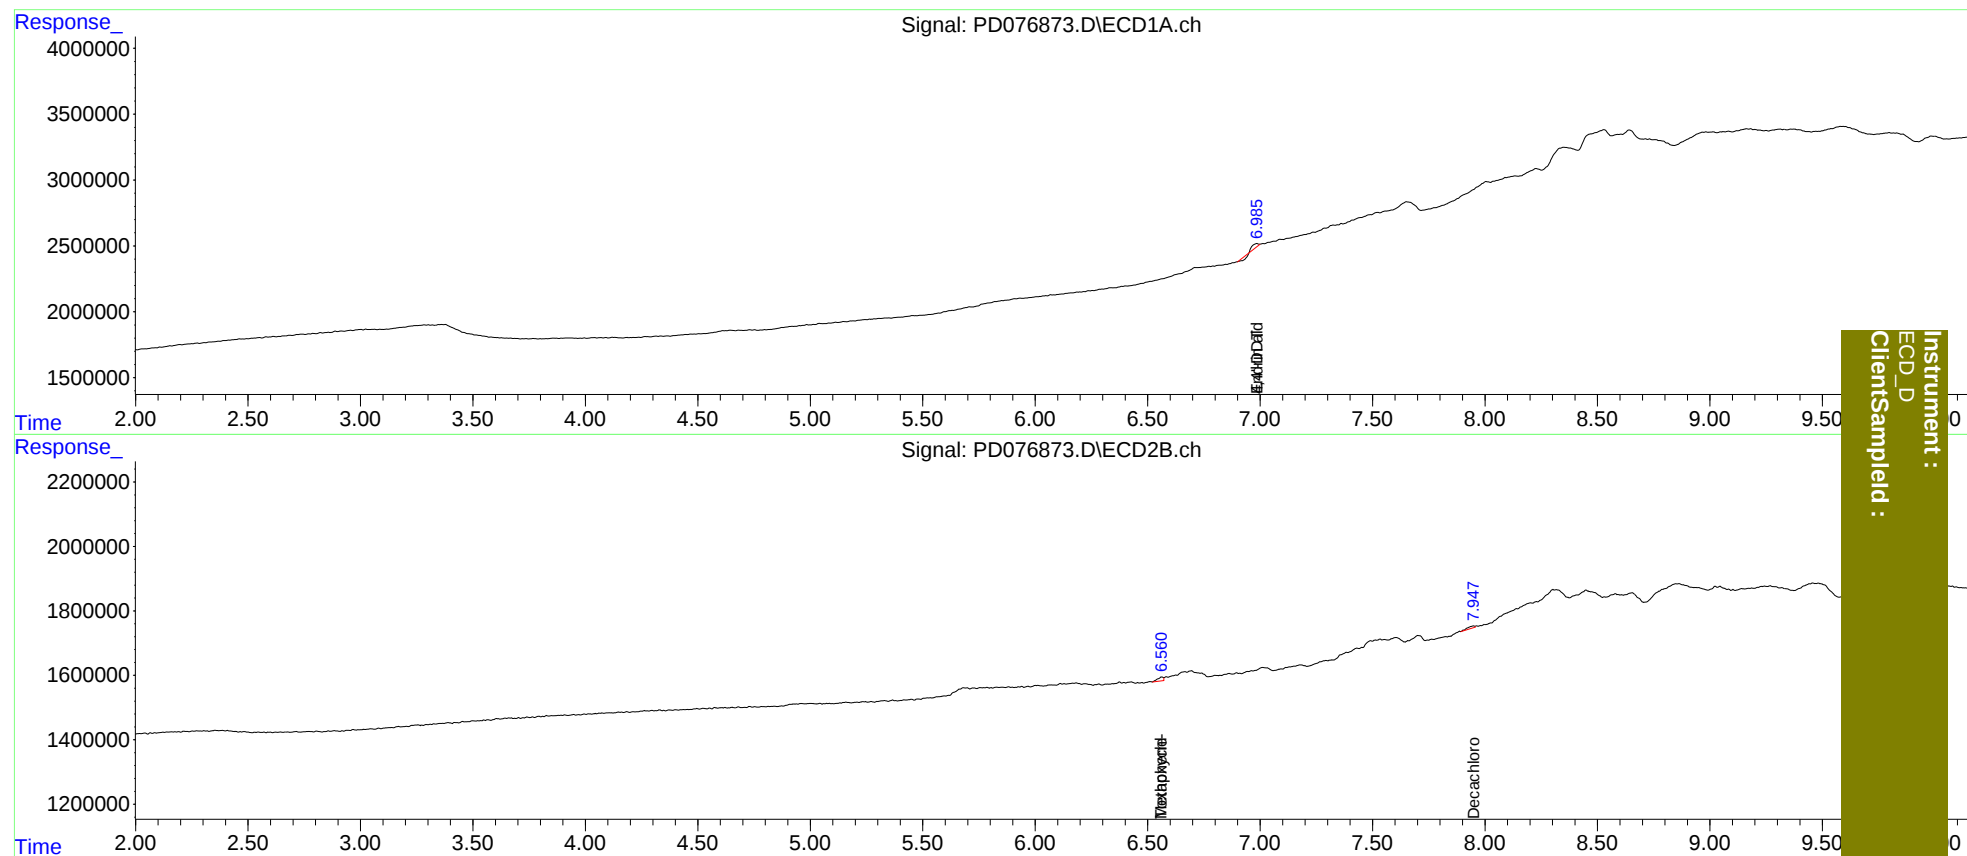


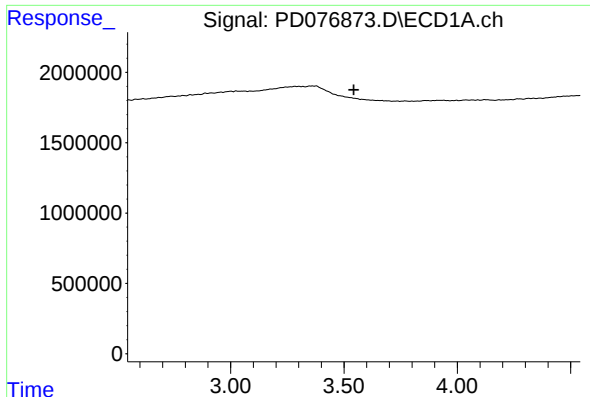

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

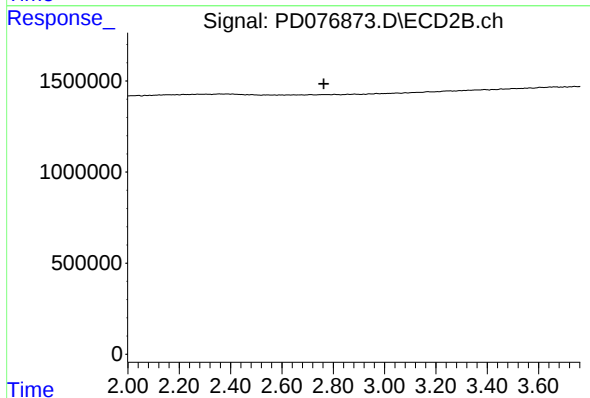


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.763 min
Response: 0
Conc: N.D.

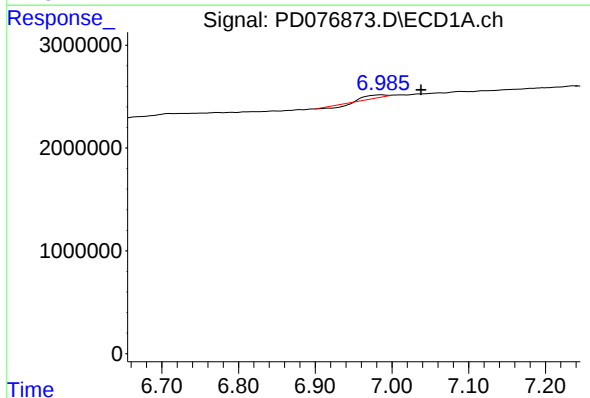


#17 4,4'-DDT

R.T.: 6.986 min
Delta R.T.: -0.052 min
Response: 353377
Conc: 0.16 ng/ml

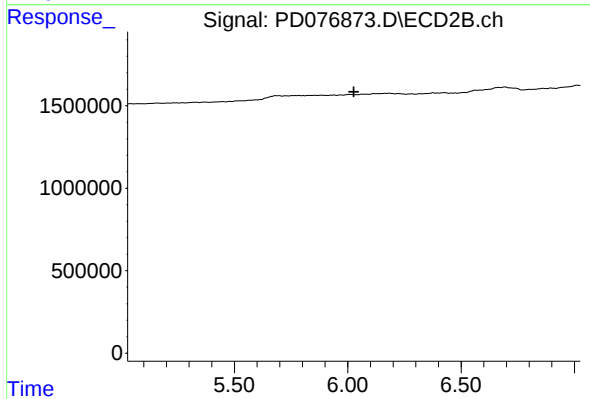

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

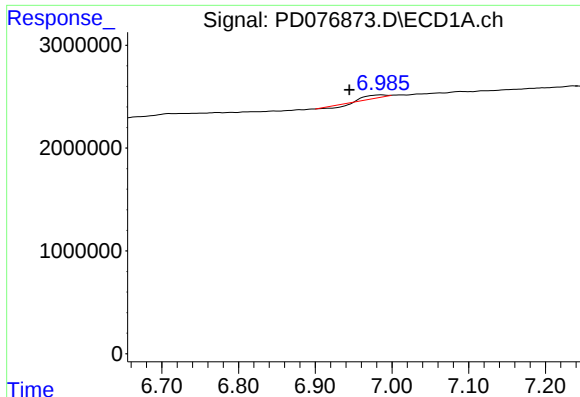

#18 Endrin aldehyde


R.T.: 6.986 min
Delta R.T.: 0.041 min
Response: 353377
Conc: 0.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

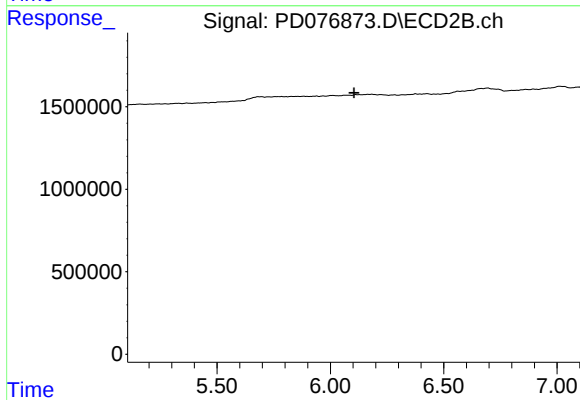


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.104 min
Response: 0
Conc: N.D.

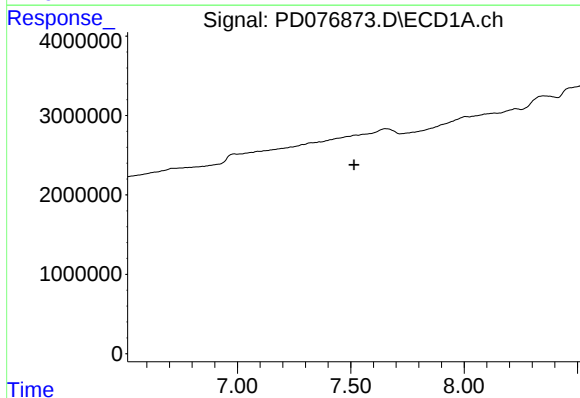


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

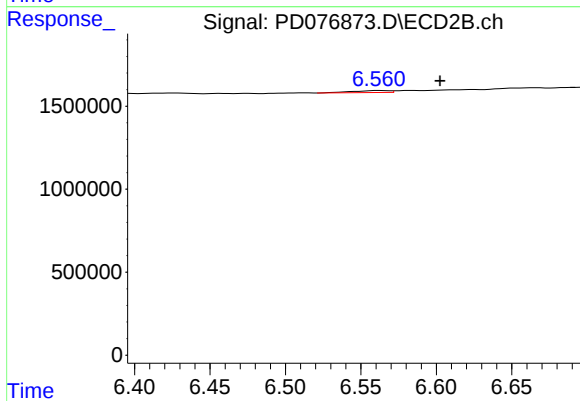

#20 Methoxychlor


R.T.: 6.562 min
Delta R.T.: -0.041 min
Response: 217275
Conc: 0.41 ng/ml

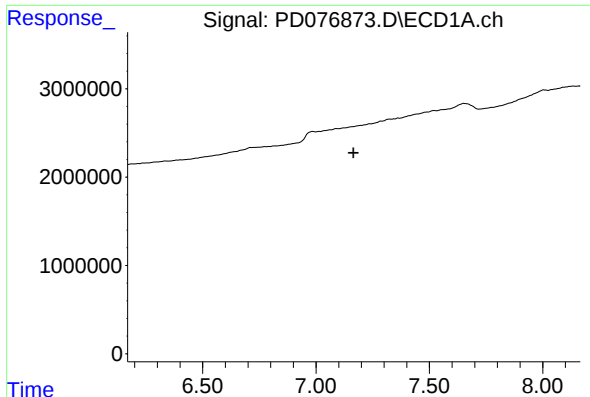

#25 Toxaphene-4


R.T.: 0.000 min
Exp R.T.: 7.165 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

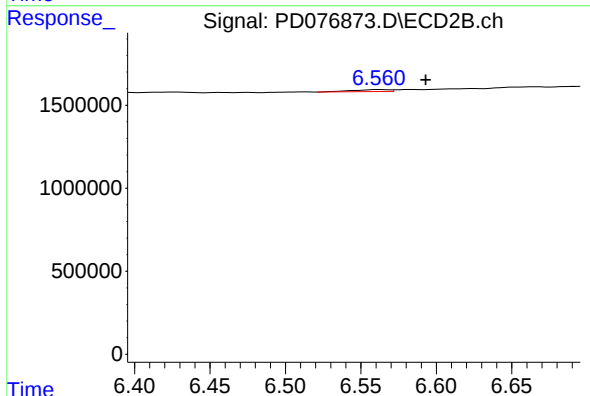


#25 Toxaphene-4

R.T.: 6.562 min
Delta R.T.: -0.031 min
Response: 217275
Conc: 8.66 ng/ml

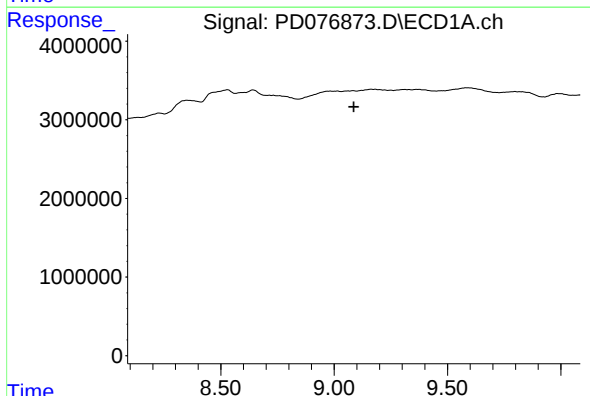

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.086 min
Response: 0
Conc: N.D.

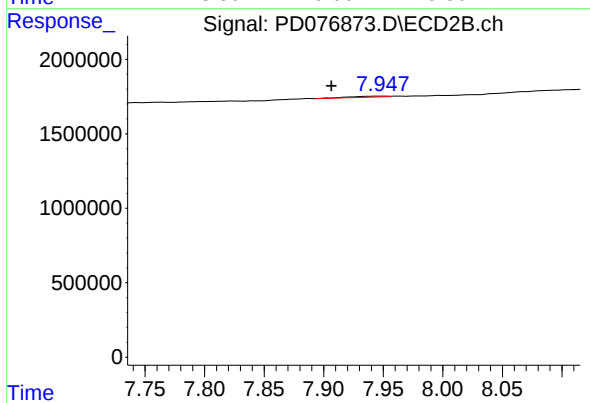

#27 Decachlorobiphenyl

R.T.: 7.948 min
Delta R.T.: 0.042 min
Response: 144621
Conc: 0.13 ng/ml