

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071823\
 Data File : PD076886.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2023 12:39
 Operator : AR\AJ
 Sample : 03624-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 07:28:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


6) B	beta-BHC	0.000	3.850f	0	190268	N.D.	0.266
20) A	Methoxychlor	7.444f	0.000	2456922	0	1.856	N.D. #
21) B	Endrin ke...	0.000	6.869	0	117738	N.D.	<MDL
26)	Toxaphene-5	0.000	6.747	0	2535	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071823\
Data File : PD076886.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2023 12:39
Operator : AR\AJ
Sample : 03624-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 07:28:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

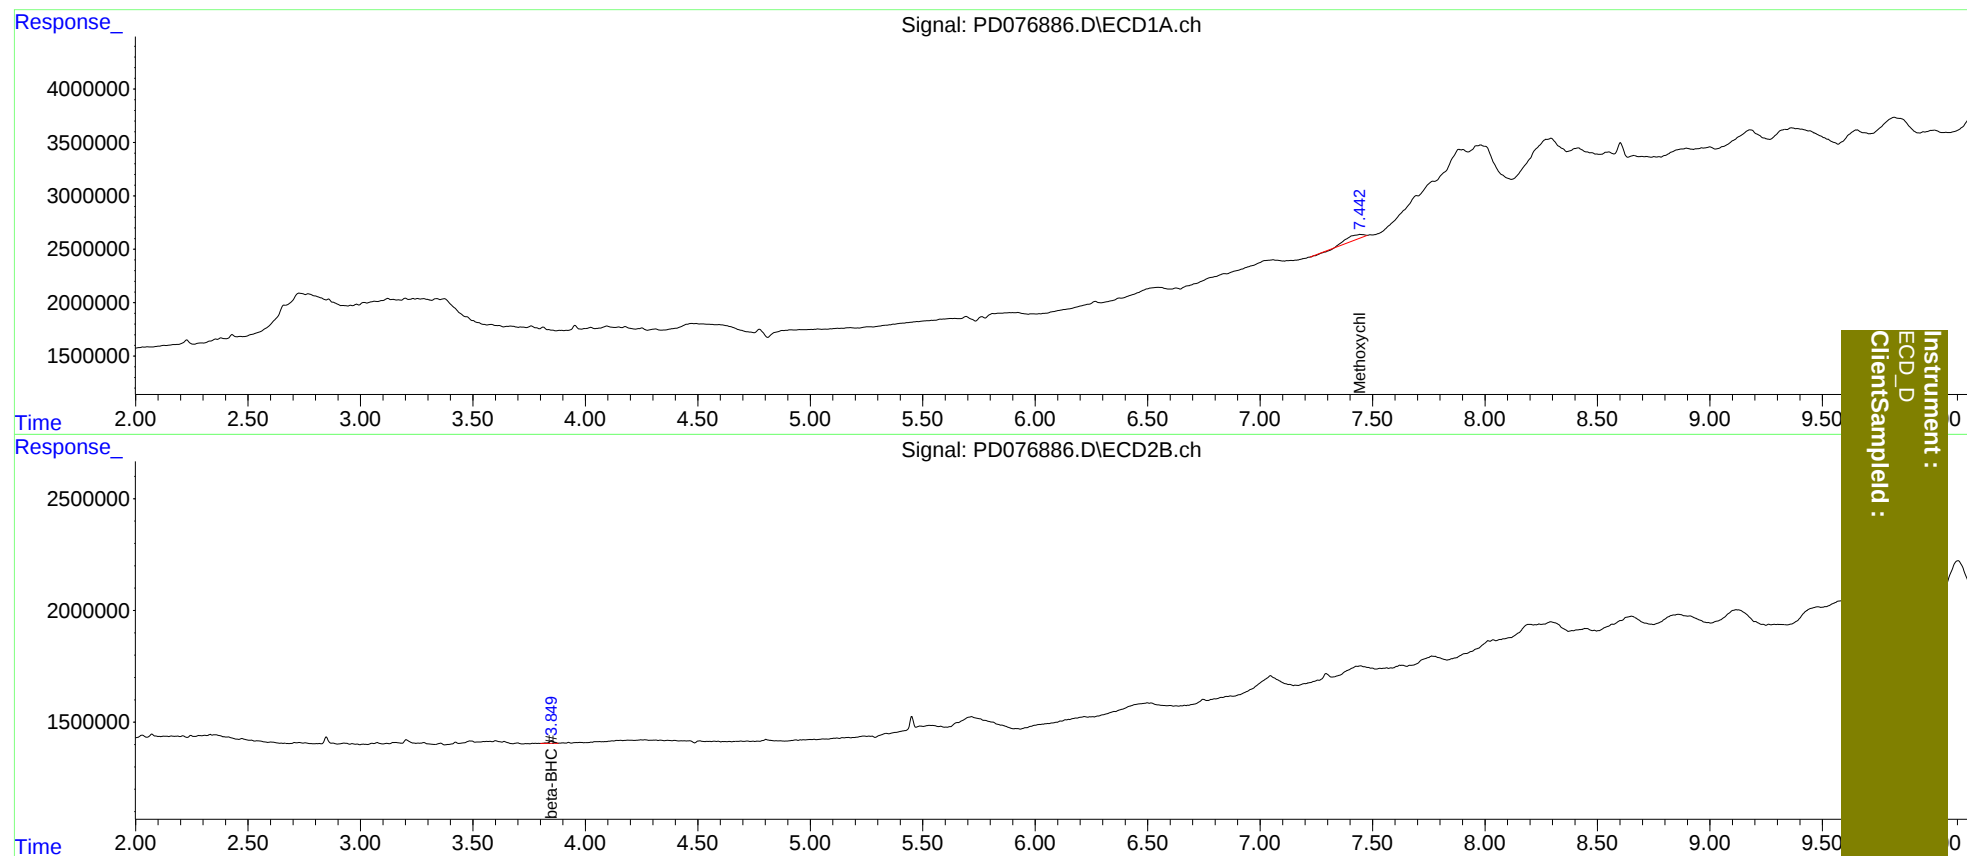

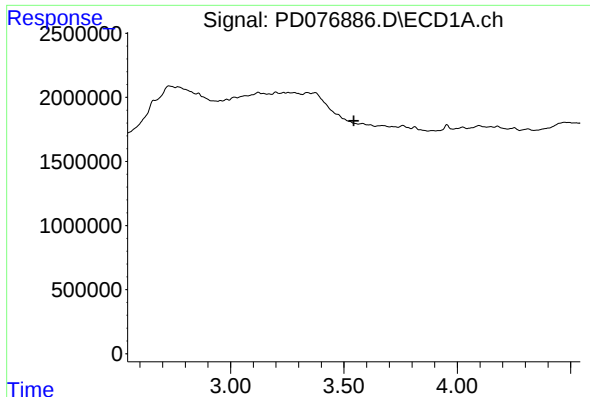

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 2.763 min
Response: 0
Conc: N.D.

#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.537 min
Response: 0
Conc: N.D.

#6 beta-BHC


R.T.: 3.850 min
Delta R.T.: -0.044 min
Response: 190268
Conc: 0.27 ng/ml

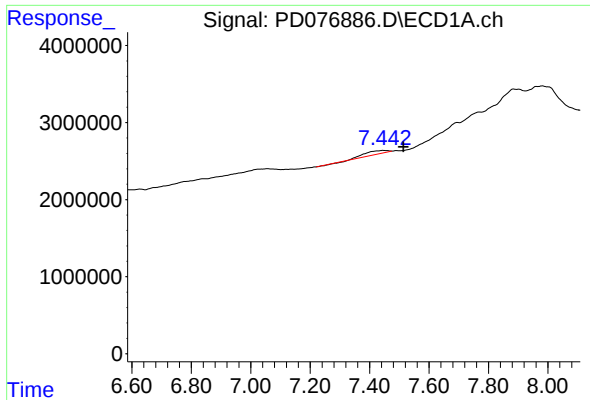

#20 Methoxychlor


R.T.: 7.444 min
Delta R.T.: -0.070 min
Response: 2456922
Conc: 1.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

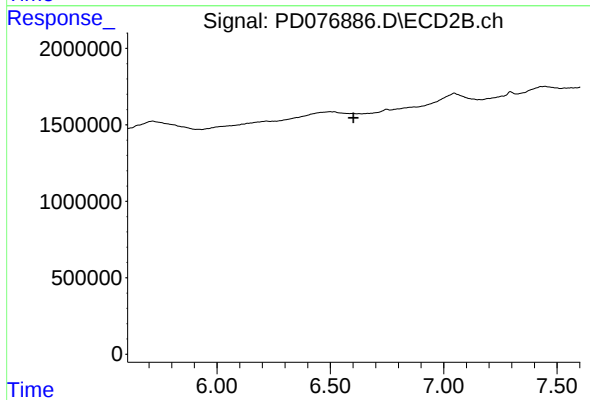


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.602 min
Response: 0
Conc: N.D.

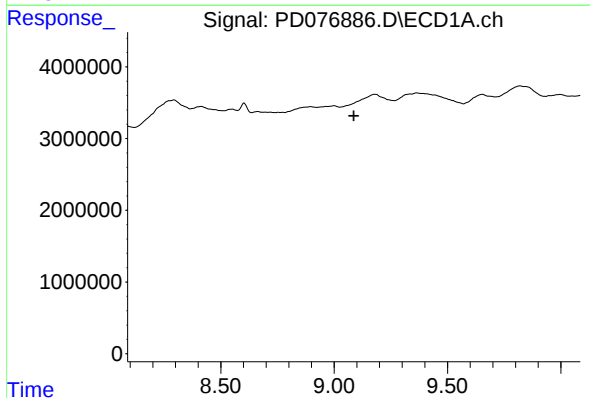

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.086 min
Response: 0
Conc: N.D.

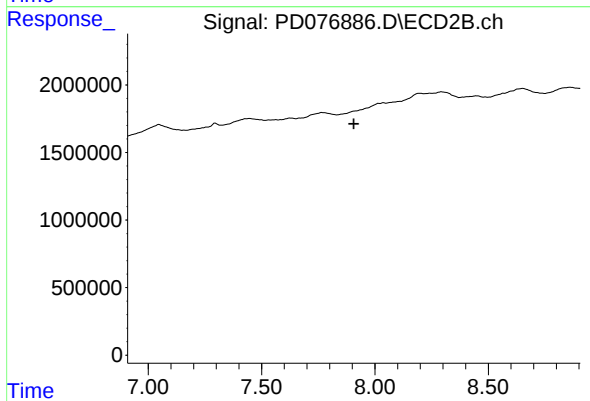

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.907 min
Response: 0
Conc: N.D.