

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071823\
 Data File : PD076878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2023 10:34
 Operator : AR\AJ
 Sample : 03472-34DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46S4DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/19/2023
 Supervised By :Ankita Jodhani 07/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 07:25:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.763	9203150	1761806	4.326	1.651 #
2) SA Decachlor...	9.087	7.905	7807052	3673648	3.213	3.427
Target Compounds						
3) MA gamma-BHC...	4.338	3.572	113.3E6	12662927	34.163m	8.452m#
7) B delta-BHC	4.798	4.130	246.1E6	96065249	73.391m	62.940
17) MA 4,4'-DDT	7.010	6.020	16433441	9542850	7.360m	10.187 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071823\
Data File : PD076878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2023 10:34
Operator : AR\AJ
Sample : 03472-34DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 07:25:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

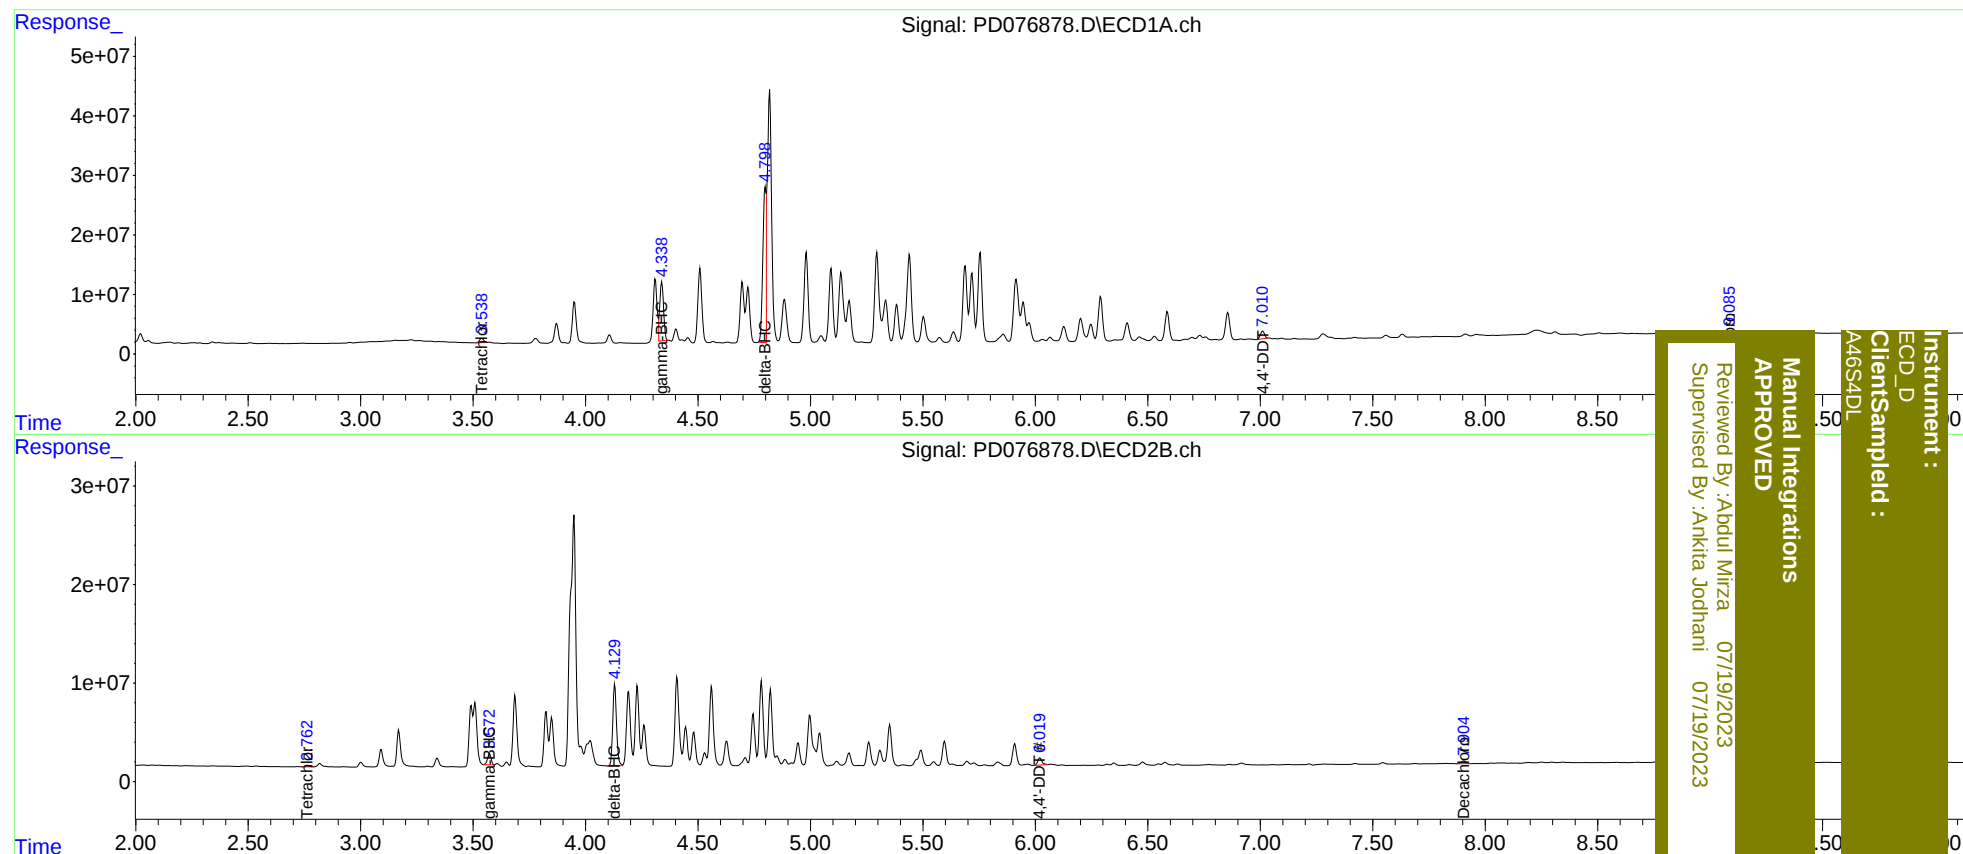

Instrument :
ECD_D
ClientSampled :
A46S4DL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/19/2023
Supervised By :Ankita Jodhani 07/19/2023