

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071824\
 Data File : PD084000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2024 04:53
 Operator : AR\AJ
 Sample : P3287-07DL3 15X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 XB506DL3

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/22/2024
 Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 06:06:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.560	2.771	1696210	8891466	1.671	1.641
2) SA Decachlor...	9.116	7.895	2942967	9148444	1.381	1.369
Target Compounds						
2) A alpha-BHC	4.019	3.270	140.0E6	650.3E6	74.001	72.134
3) MA gamma-BHC...	4.352	3.597	111.2E6	508.1E6	60.274	59.358m
4) MA Heptachlor	4.944	3.936	15271825	73402009	7.618	8.717
5) MB Aldrin	5.288	4.216	153.8E6	623.0E6	75.711	73.842
6) B beta-BHC	4.550	3.896	76878060	349.6E6	91.526	92.214
7) B delta-BHC	4.798	4.125	61559695	274.0E6	29.041	30.013
8) B Heptachlo...	5.715	4.716	37722754	154.4E6	19.376	19.662
9) A Endosulfan I	6.102	5.086	98833920	368.1E6	53.362m	52.968
10) B trans-Chl...	5.973	4.966	105.2E6	409.6E6	55.274	53.006
11) B cis-Chlor...	6.051	5.030	98931188	382.7E6	50.541m	48.626
12) B 4,4'-DDE	6.223	5.217	125.0E6	469.4E6	63.084	62.697
13) MA Dieldrin	6.379	5.350	99150537	378.4E6	49.516	48.875
14) MA Endrin	6.609	5.625	228.4E6	809.5E6	138.100	122.228
15) B Endosulfa...	6.830	5.918	113.2E6	396.8E6	62.111	59.471
16) A 4,4'-DDD	6.743	5.772	46920627	196.1E6	32.522	32.921
17) MA 4,4'-DDT	7.057	6.022	32549970	122.3E6	21.525	20.920
18) B Endrin al...	6.960	6.096	152.9E6	523.8E6	111.797	104.436m
19) B Endosulfa...	7.195	6.320	86371880	308.6E6	48.735	47.501
20) A Methoxychlor	7.534	6.596	20781679	71316445	23.358	24.136
21) B Endrin ke...	7.682	6.826	241.4E6	808.9E6	123.637	115.154

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071824\
Data File : PD084000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2024 04:53
Operator : AR\AJ
Sample : P3287-07DL3 15X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 06:06:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

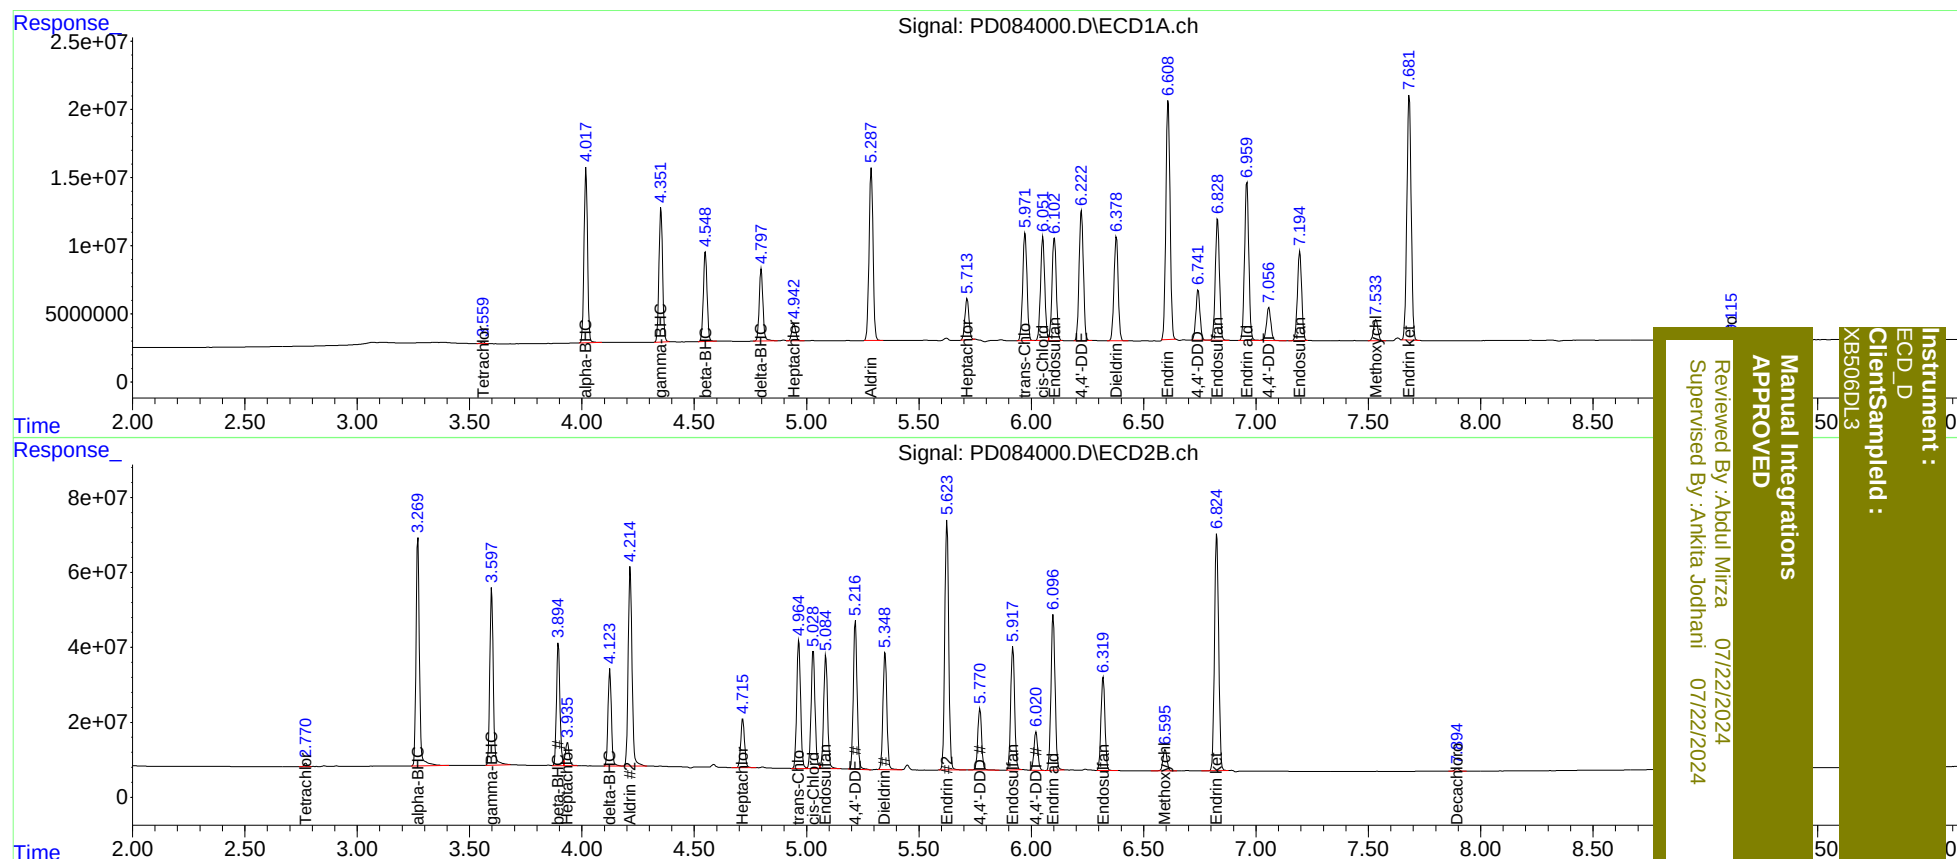

Instrument :
ECD_D
Client Sampled :
XB506DL3

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 07/22/2024
Supervised By: Ankita Jodhani 07/22/2024