

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071919\
 Data File : PD053985.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2019 18:10
 Operator : SM\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:50:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 03:49:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.983	67873605	93250871	97.530	96.478
28)	SA Decachlor...	8.008	9.024	64402232	84760042	96.070	94.098
Target Compounds							
23)	Chlordane-1	4.160	4.973	20835075	36546216	1006.173	975.371
24)	Chlordane-2	4.652	5.438	25793154	42442469	951.685	959.391
25)	Chlordane-3	5.210	6.081	82013844	173.8E6	993.089	984.774
26)	Chlordane-4	5.267	6.155	70341396	206.5E6	986.740	971.765
27)	Chlordane-5	6.093	6.956	28137064	37631541	986.246	989.147



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071919\
Data File : PD053985.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2019 18:10
Operator : SM\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:50:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 03:49:14 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

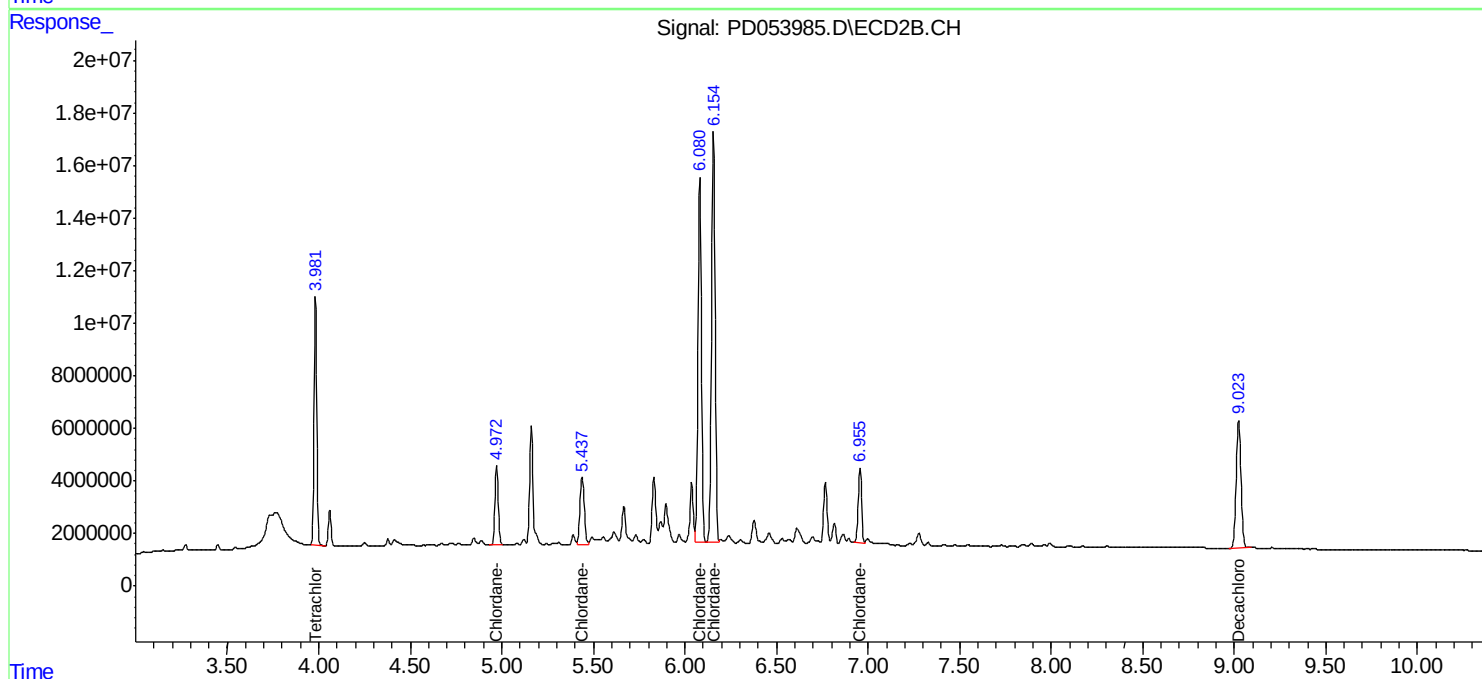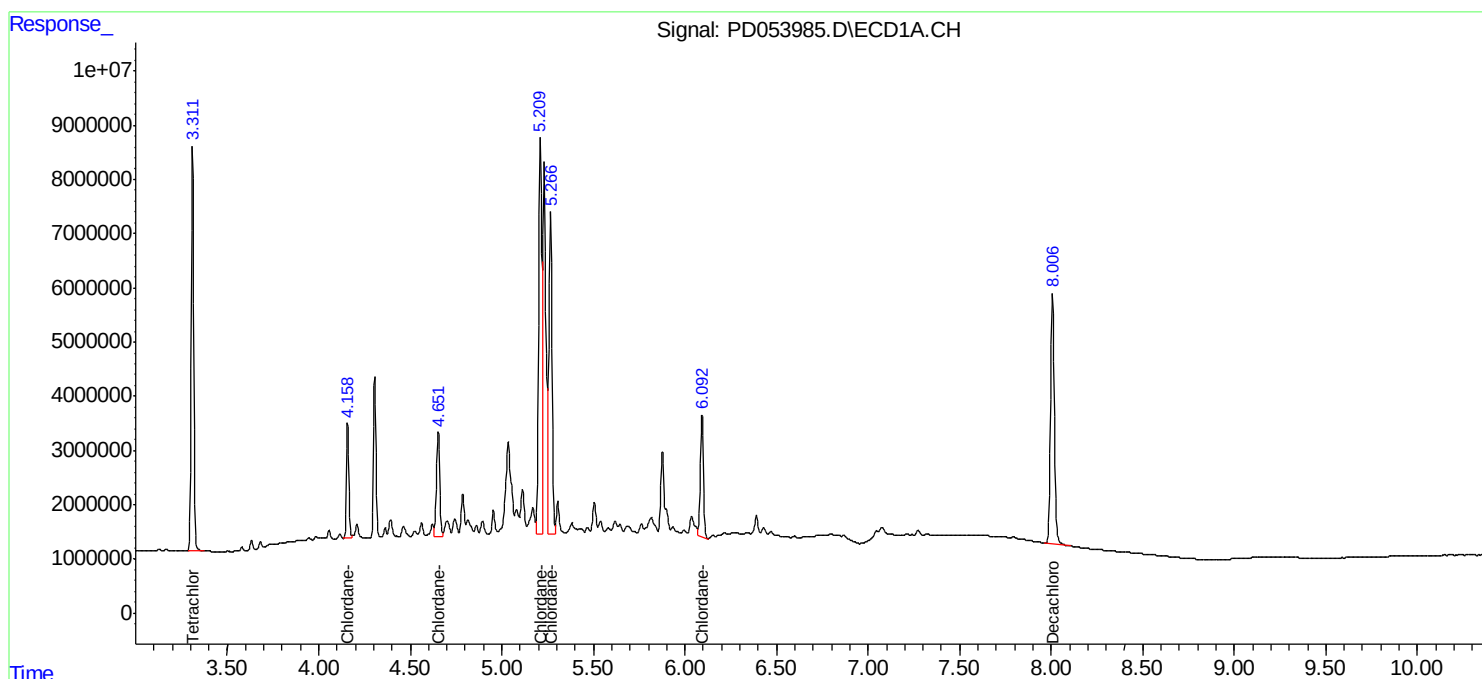


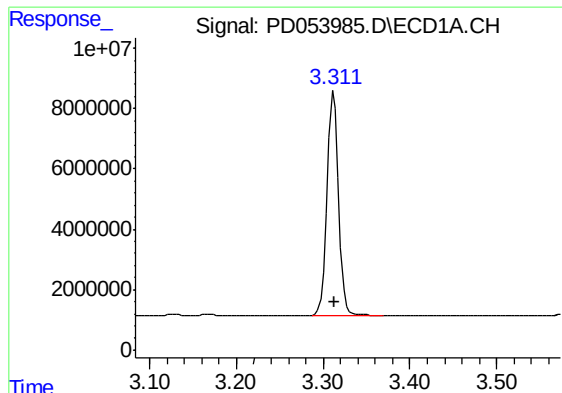

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 67873605
Conc: 97.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

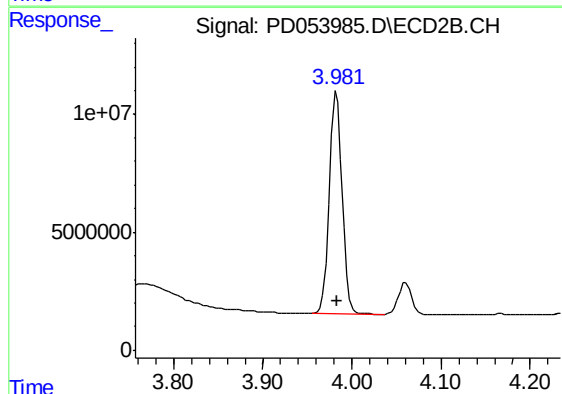


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 93250871
Conc: 96.48 ng/ml

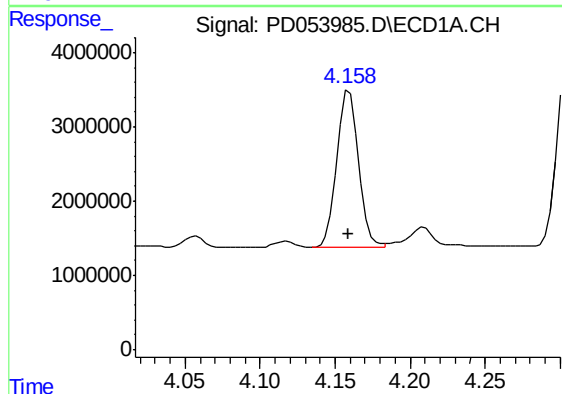


#23 Chlordane-1

R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 20835075
Conc: 1006.17 ng/ml

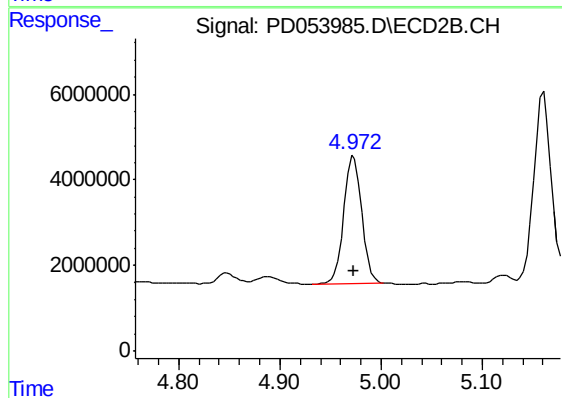

#23 Chlordane-1


R.T.: 4.973 min
Delta R.T.: 0.000 min
Response: 36546216
Conc: 975.37 ng/ml

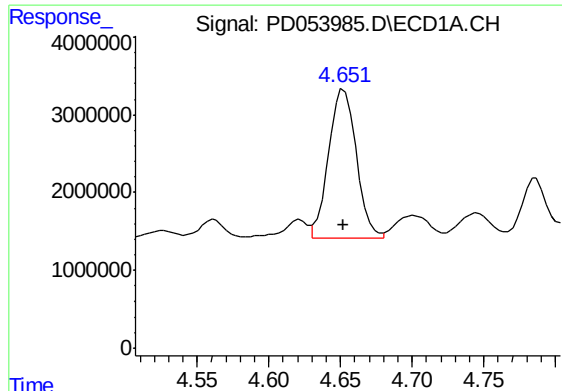

#24 Chlordane-2


R.T.: 4.652 min
Delta R.T.: 0.000 min
Response: 25793154
Conc: 951.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

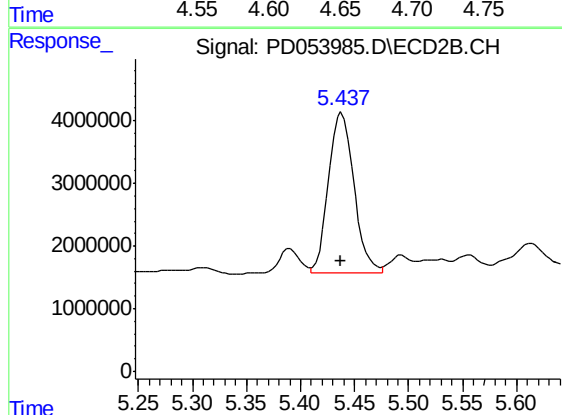


#24 Chlordane-2

R.T.: 5.438 min
Delta R.T.: 0.000 min
Response: 42442469
Conc: 959.39 ng/ml

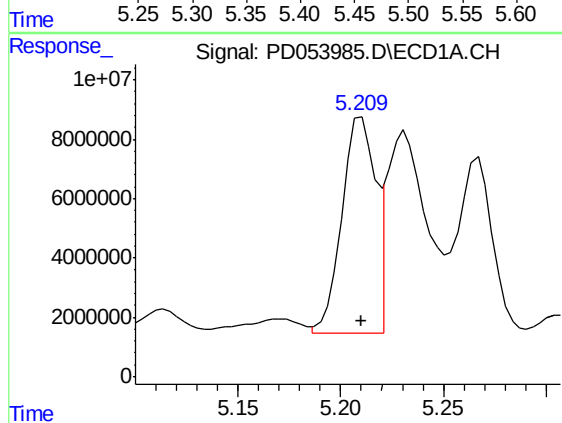


#25 Chlordane-3

R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 82013844
Conc: 993.09 ng/ml

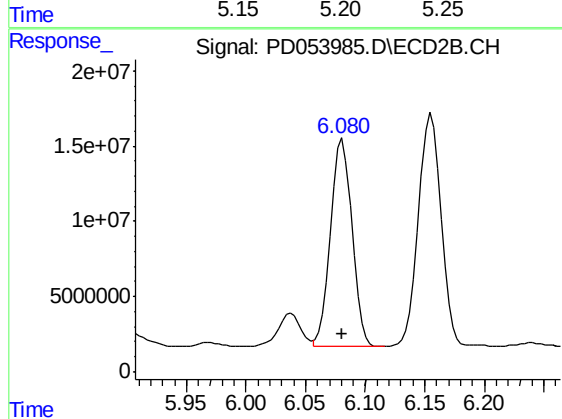

#25 Chlordane-3


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 173835970
Conc: 984.77 ng/ml

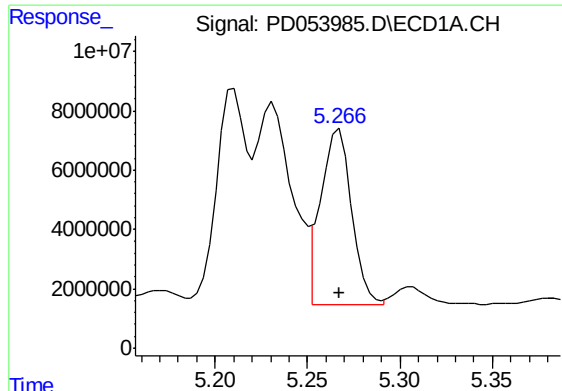

#26 Chlordane-4


R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 70341396
Conc: 986.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

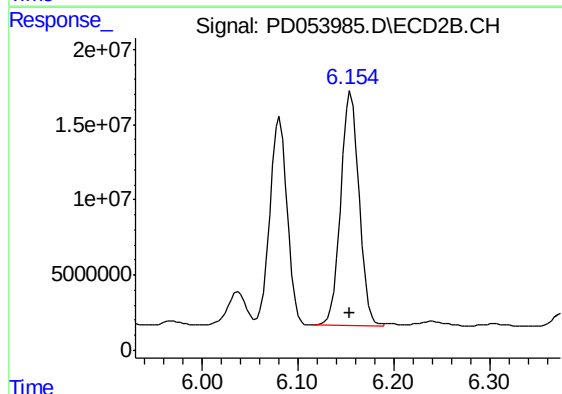


#26 Chlordane-4

R.T.: 6.155 min
Delta R.T.: 0.000 min
Response: 206478461
Conc: 971.76 ng/ml

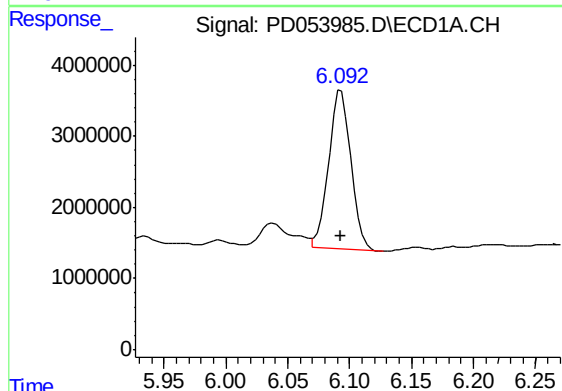


#27 Chlordane-5

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 28137064
Conc: 986.25 ng/ml

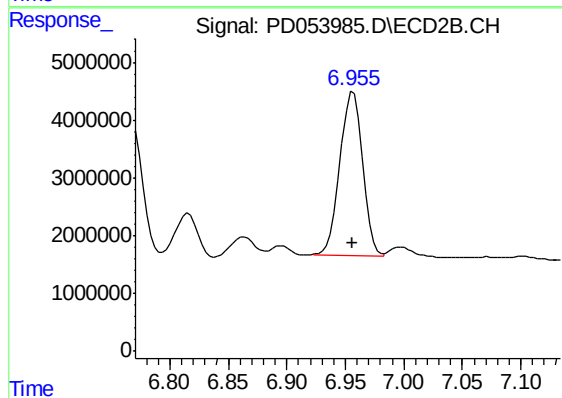

#27 Chlordane-5


R.T.: 6.956 min
Delta R.T.: 0.000 min
Response: 37631541
Conc: 989.15 ng/ml

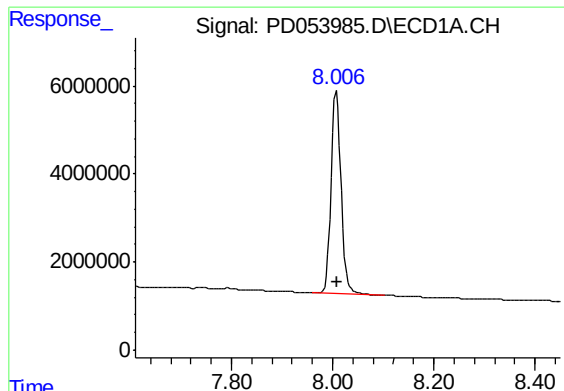

#28 Decachlorobiphenyl

R.T.: 8.008 min
Delta R.T.: 0.000 min
Response: 64402232
Conc: 96.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

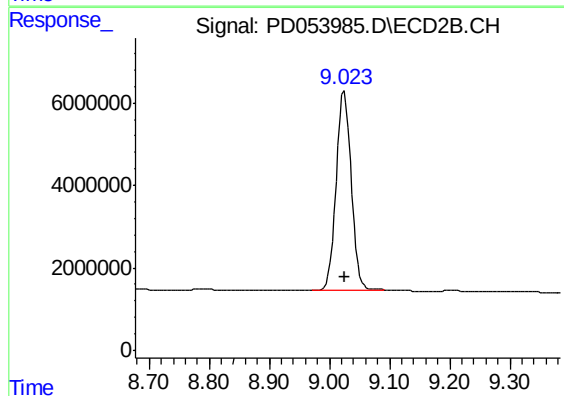

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 84760042
Conc: 94.10 ng/ml