

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071919\
 Data File : PD053988.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2019 18:52
 Operator : SM\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:51:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 03:49:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.983	17531078	24658561	25.191	25.512
28)	SA Decachlor...	8.008	9.025	17181778	23336115	25.630	25.907
Target Compounds							
23)	Chlordane-1	4.160	4.972	5256564	9940972	253.851	265.312
24)	Chlordane-2	4.653	5.437	6943975	11477337	256.210	259.440
25)	Chlordane-3	5.210	6.080	20075882	43806043	243.095	248.159
26)	Chlordane-4	5.268	6.154	17091000	52821088	239.750	248.596
27)	Chlordane-5	6.093	6.955	7043138	9652725	246.873	253.722



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071919\
Data File : PD053988.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2019 18:52
Operator : SM\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:51:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 03:49:14 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

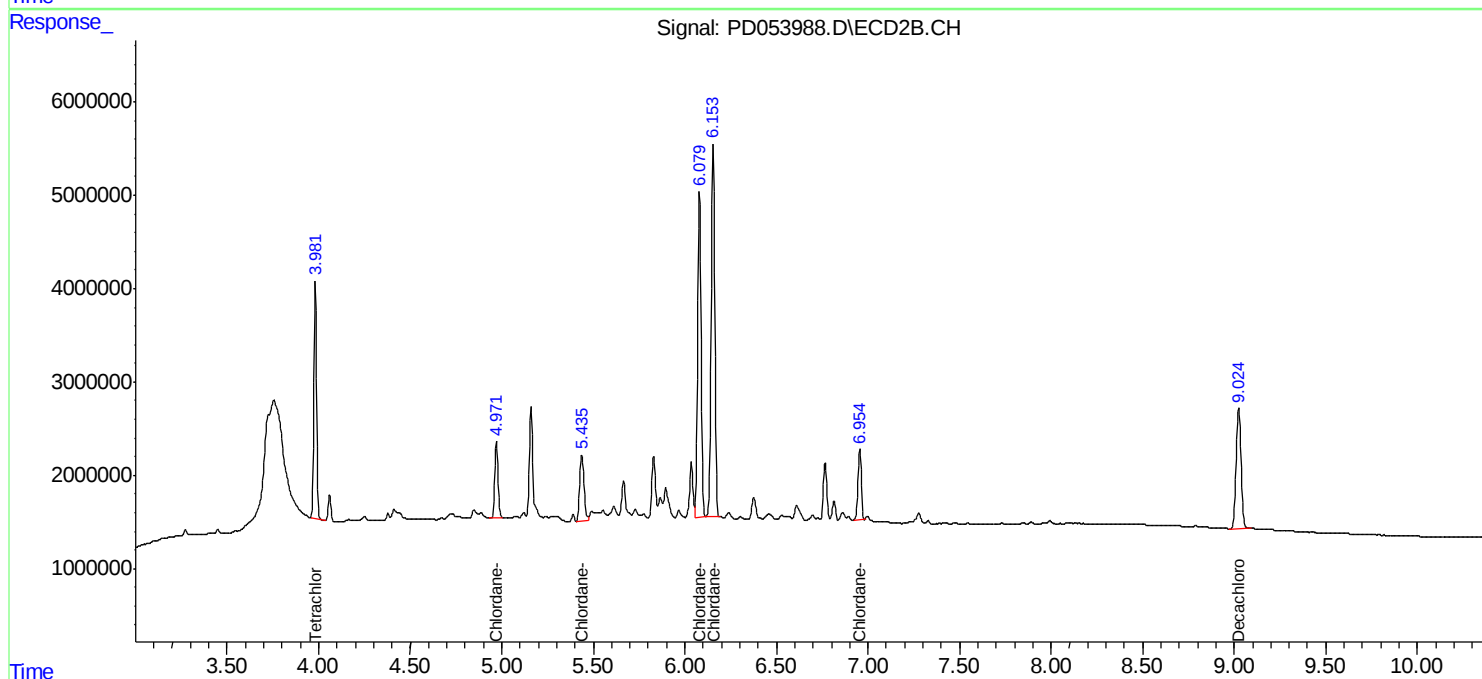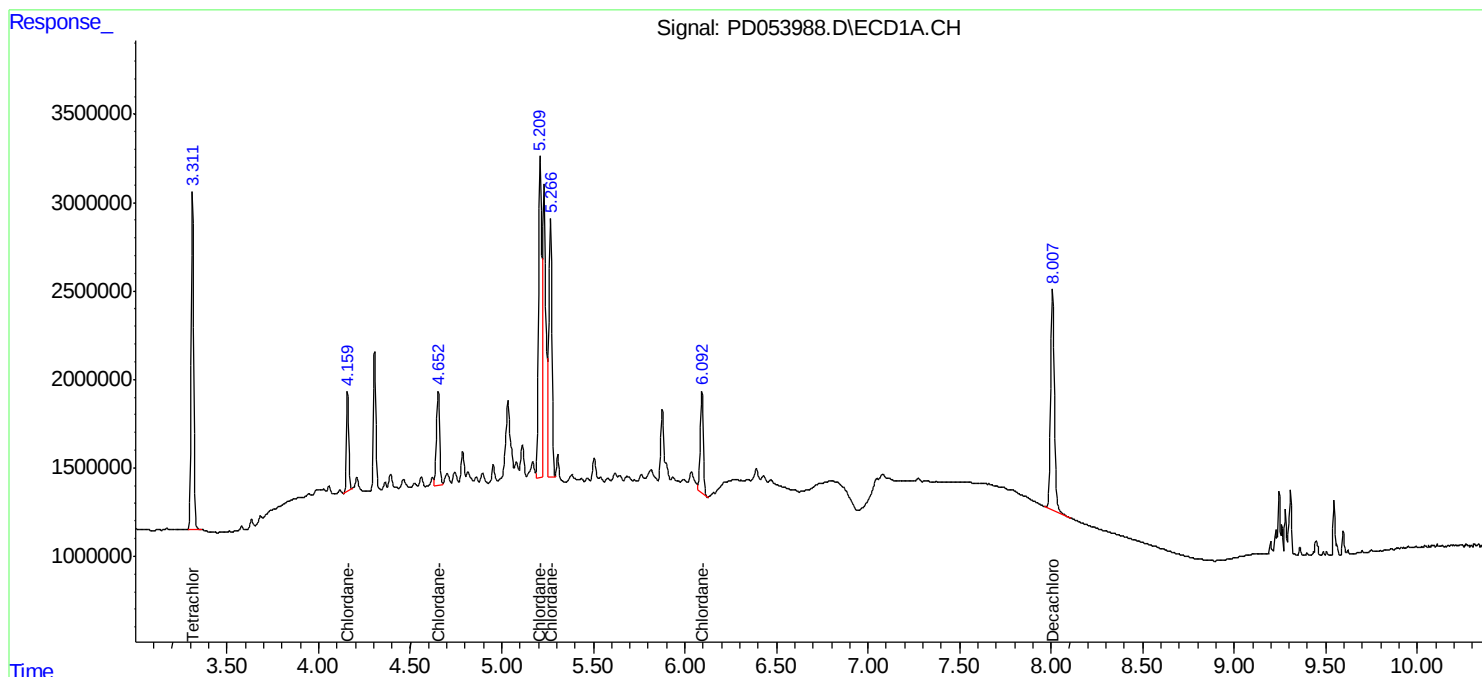


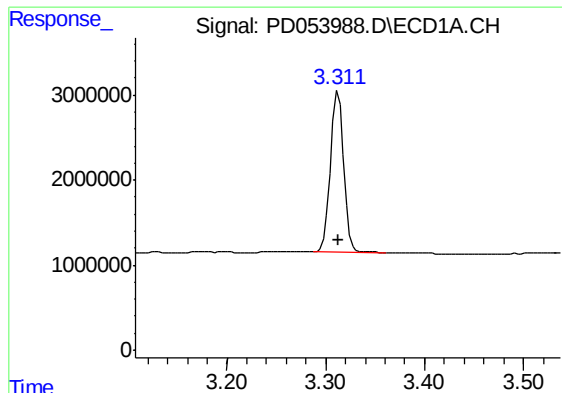

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: 0.000 min
Response: 17531078
Conc: 25.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

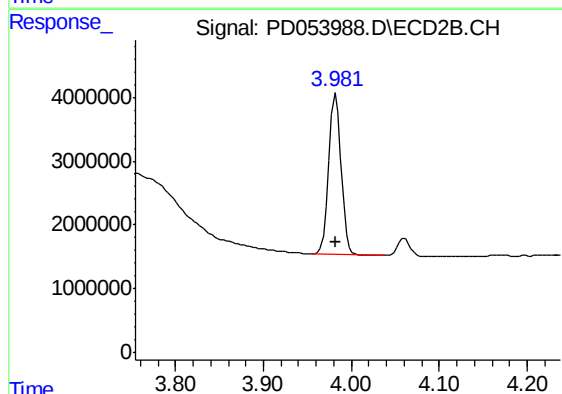


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 24658561
Conc: 25.51 ng/ml

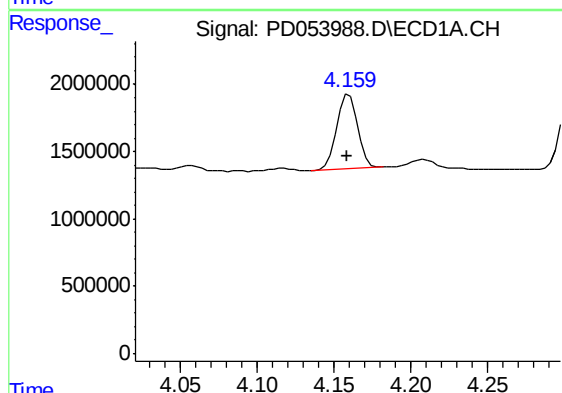


#23 Chlordane-1

R.T.: 4.160 min
Delta R.T.: 0.000 min
Response: 5256564
Conc: 253.85 ng/ml

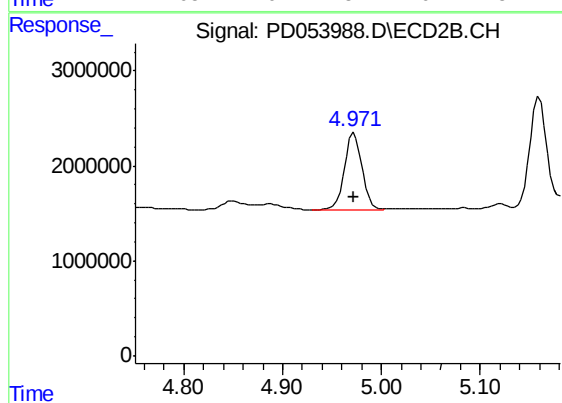

#23 Chlordane-1


R.T.: 4.972 min
Delta R.T.: 0.000 min
Response: 9940972
Conc: 265.31 ng/ml

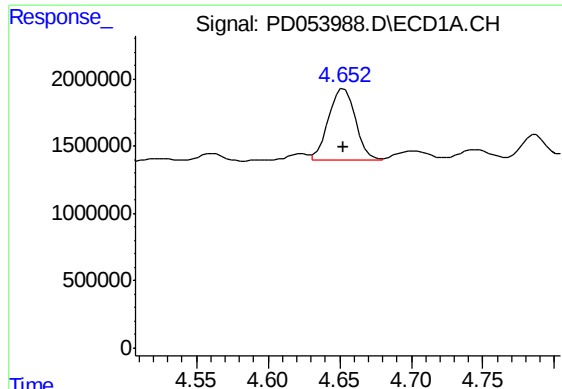

#24 Chlordane-2


R.T.: 4.653 min
Delta R.T.: 0.000 min
Response: 6943975
Conc: 256.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

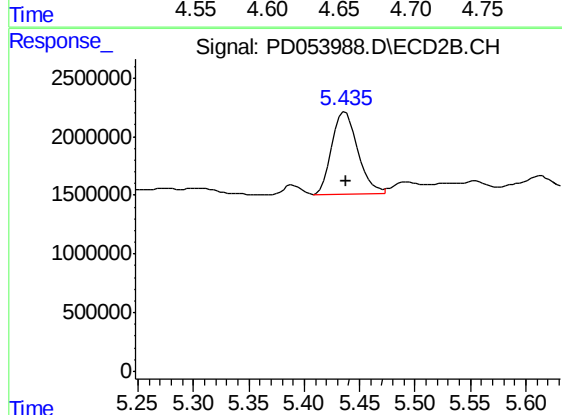


#24 Chlordane-2

R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 11477337
Conc: 259.44 ng/ml

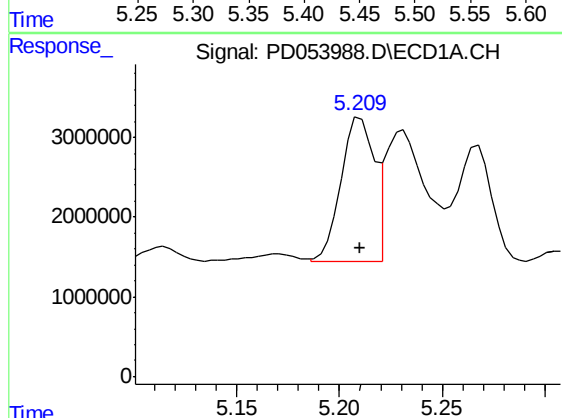


#25 Chlordane-3

R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 20075882
Conc: 243.09 ng/ml

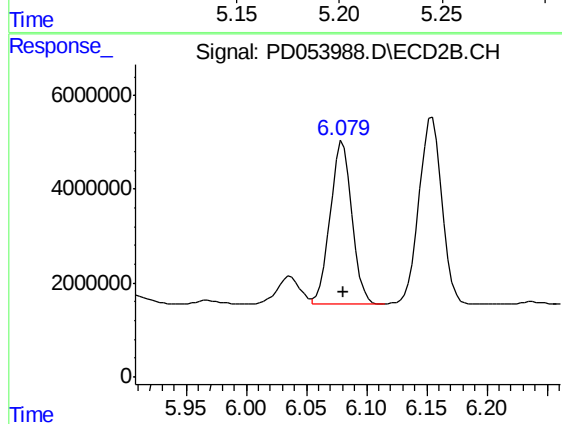

#25 Chlordane-3


R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 43806043
Conc: 248.16 ng/ml

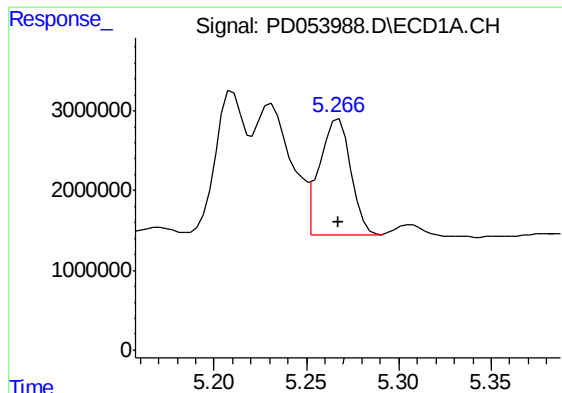

#26 Chlordane-4


R.T.: 5.268 min
Delta R.T.: 0.000 min
Response: 17091000
Conc: 239.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

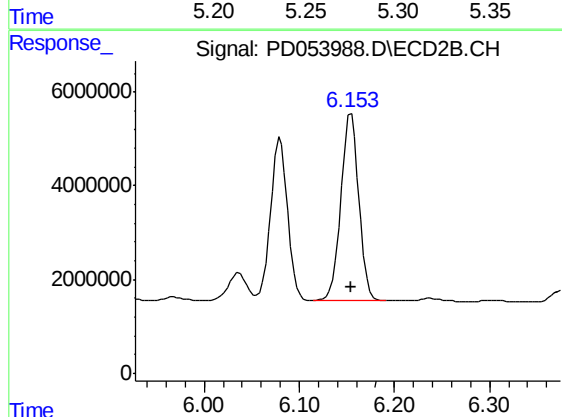


#26 Chlordane-4

R.T.: 6.154 min
Delta R.T.: 0.000 min
Response: 52821088
Conc: 248.60 ng/ml

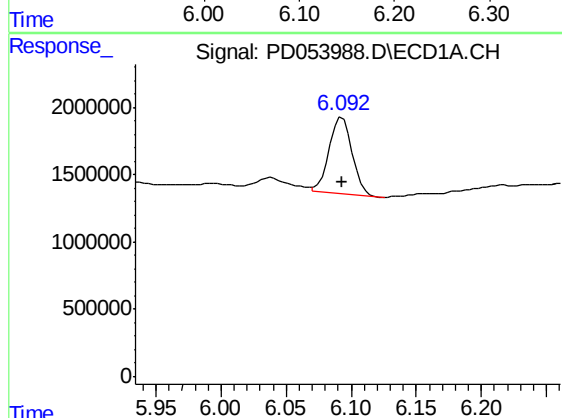


#27 Chlordane-5

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 7043138
Conc: 246.87 ng/ml

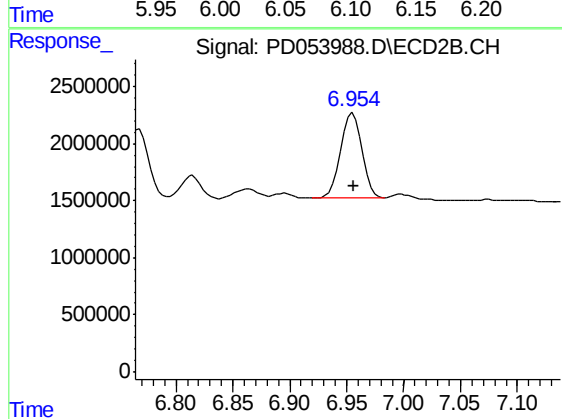

#27 Chlordane-5


R.T.: 6.955 min
Delta R.T.: 0.000 min
Response: 9652725
Conc: 253.72 ng/ml

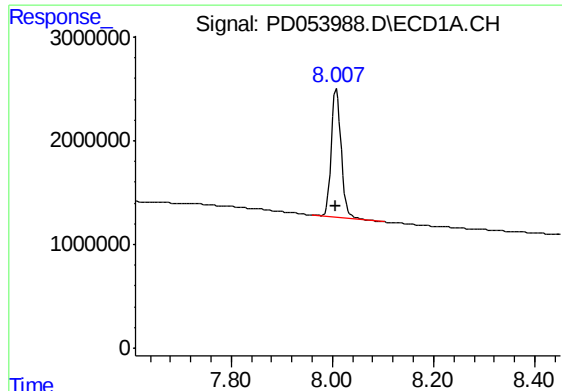

#28 Decachlorobiphenyl

R.T.: 8.008 min
Delta R.T.: 0.000 min
Response: 17181778
Conc: 25.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

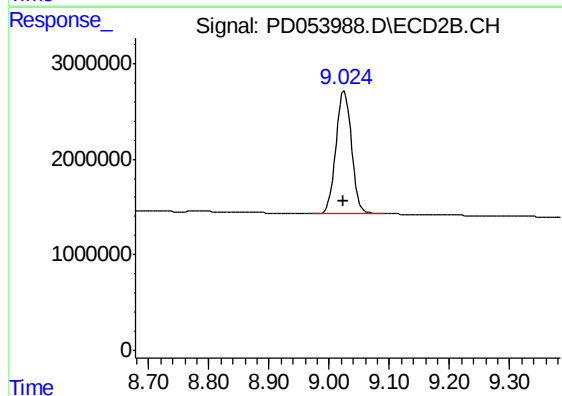

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 23336115
Conc: 25.91 ng/ml