

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071919\
 Data File : PD053986.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2019 18:24
 Operator : SM\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 03:50:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 03:49:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.983	46956697	64324111	67.473	66.550
28)	SA Decachlor...	8.008	9.024	49231456	65531046	73.440	72.750
Target Compounds							
23)	Chlordane-1	4.159	4.973	14262153	25083703	688.752	669.452
24)	Chlordane-2	4.652	5.438	18147565	29712688	669.587	671.641
25)	Chlordane-3	5.210	6.081	57074319	122.3E6	691.101	692.561
26)	Chlordane-4	5.267	6.156	49538746	146.6E6	694.923	690.163
27)	Chlordane-5	6.093	6.957	20067938	26963117	703.411	708.727



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071919\
Data File : PD053986.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2019 18:24
Operator : SM\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 03:50:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 03:49:14 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

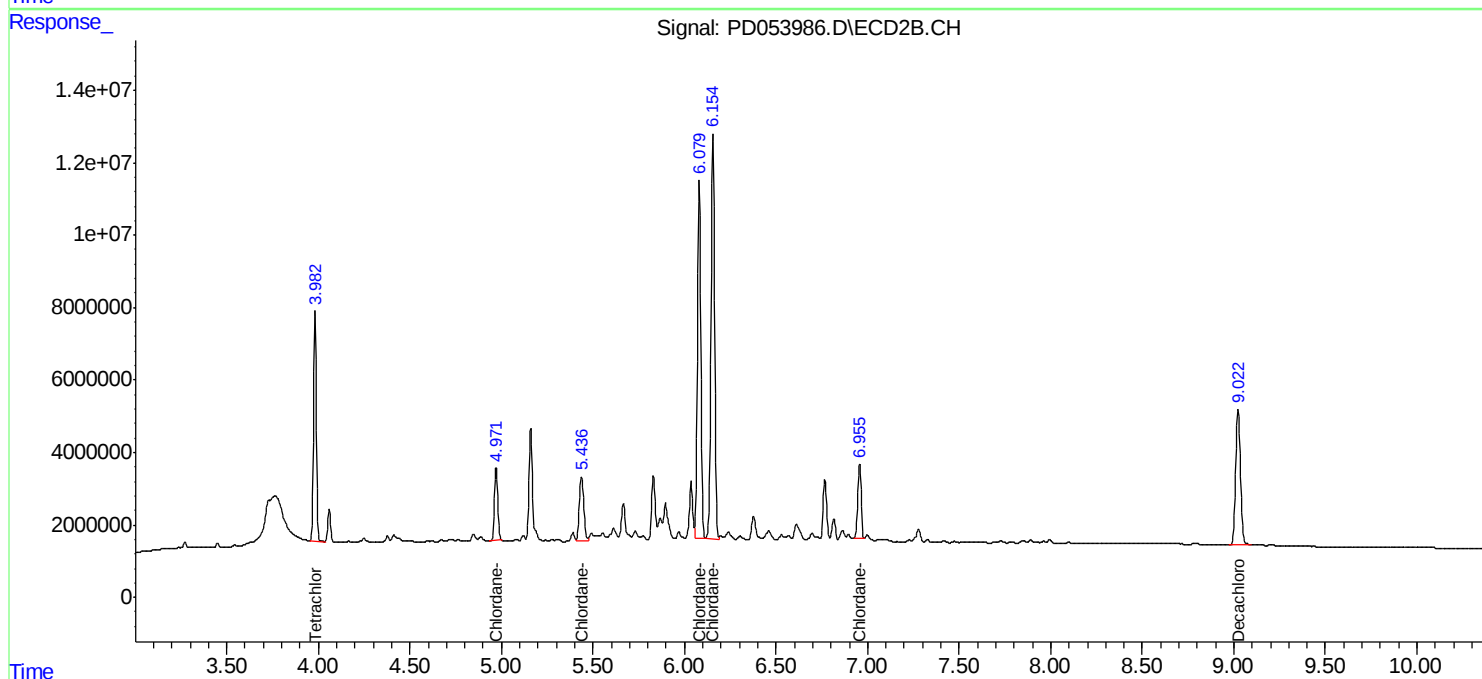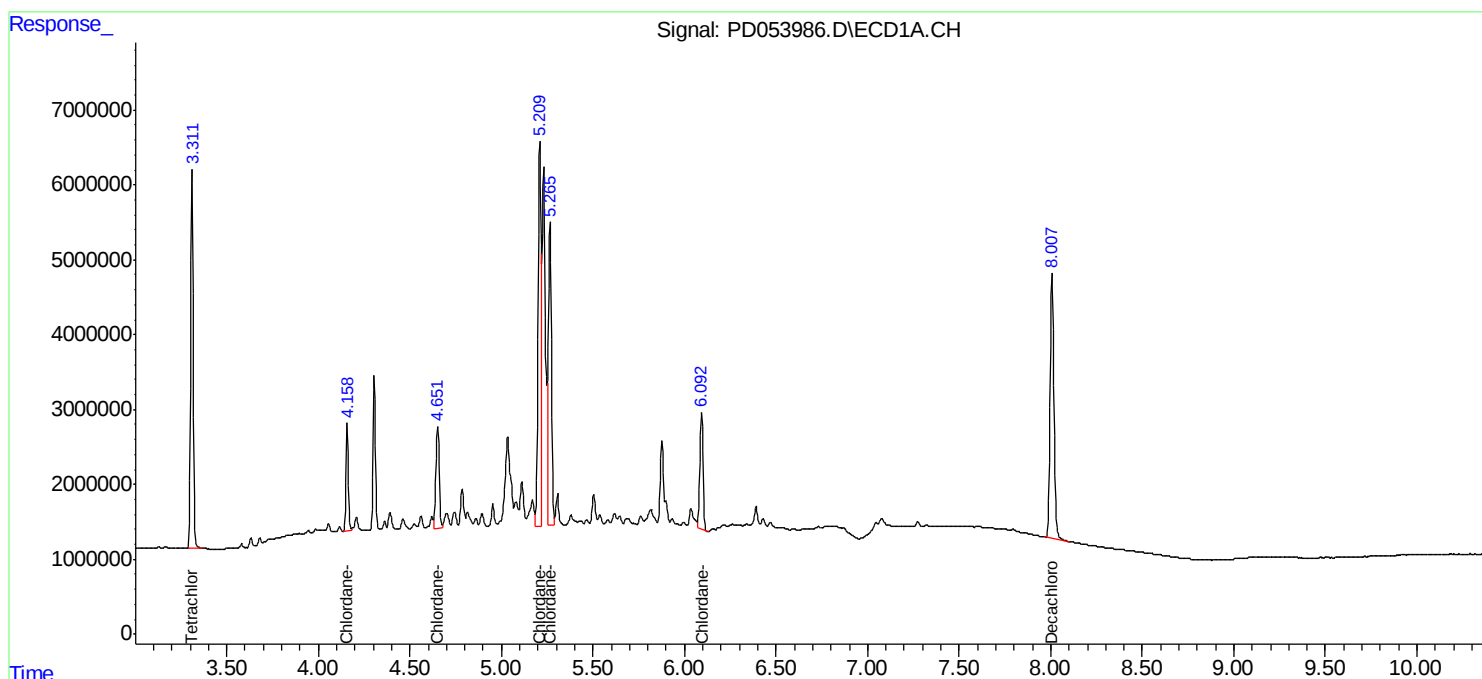


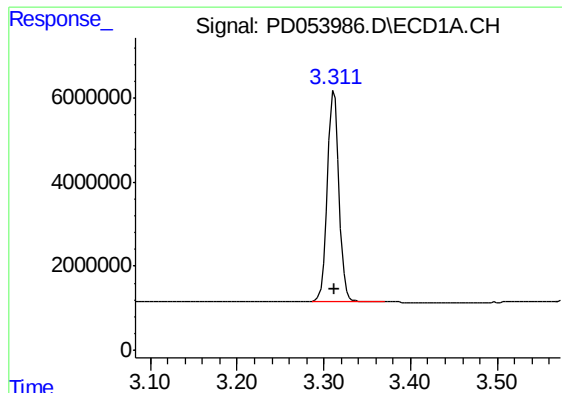

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 46956697
Conc: 67.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

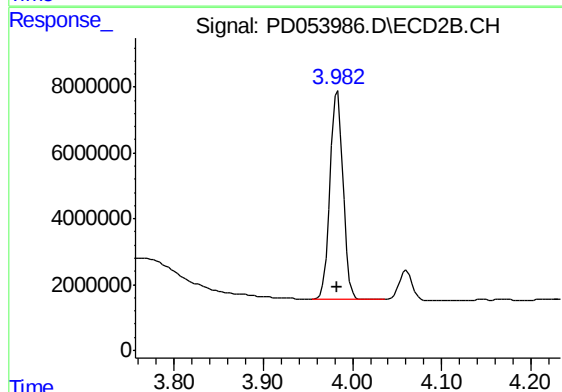


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 64324111
Conc: 66.55 ng/ml

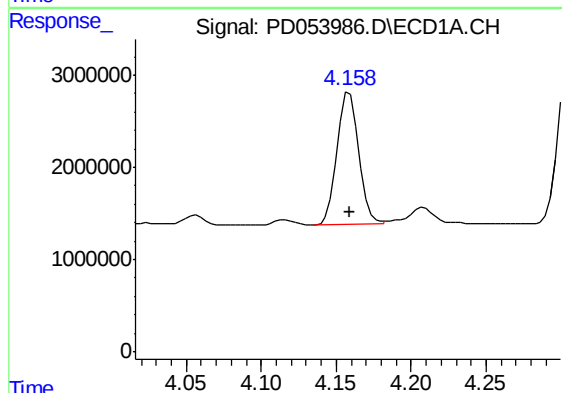


#23 Chlordane-1

R.T.: 4.159 min
Delta R.T.: 0.000 min
Response: 14262153
Conc: 688.75 ng/ml

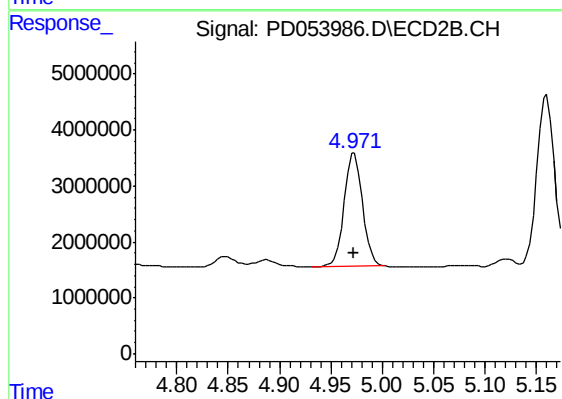

#23 Chlordane-1


R.T.: 4.973 min
Delta R.T.: 0.000 min
Response: 25083703
Conc: 669.45 ng/ml

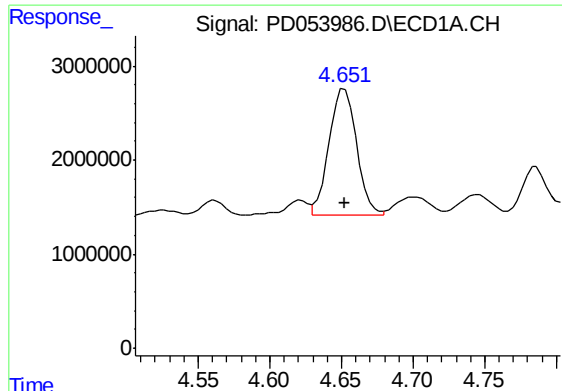

#24 Chlordane-2


R.T.: 4.652 min
Delta R.T.: 0.000 min
Response: 18147565
Conc: 669.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

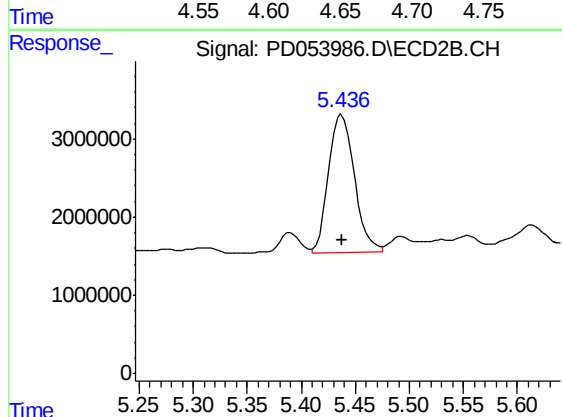


#24 Chlordane-2

R.T.: 5.438 min
Delta R.T.: 0.000 min
Response: 29712688
Conc: 671.64 ng/ml

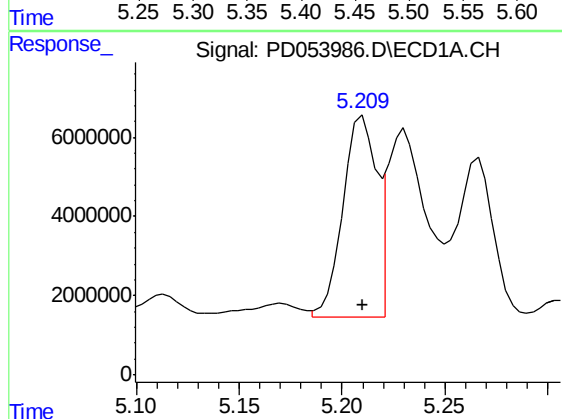


#25 Chlordane-3

R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 57074319
Conc: 691.10 ng/ml

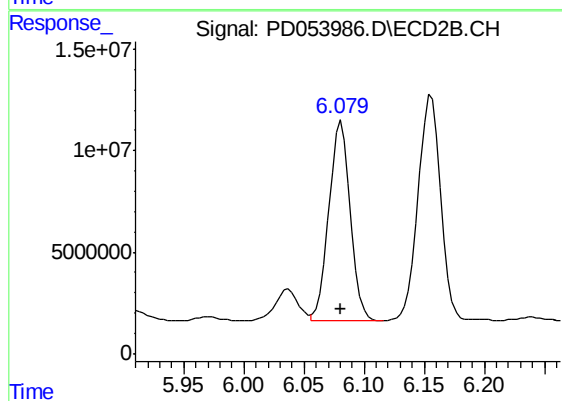

#25 Chlordane-3


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 122253577
Conc: 692.56 ng/ml

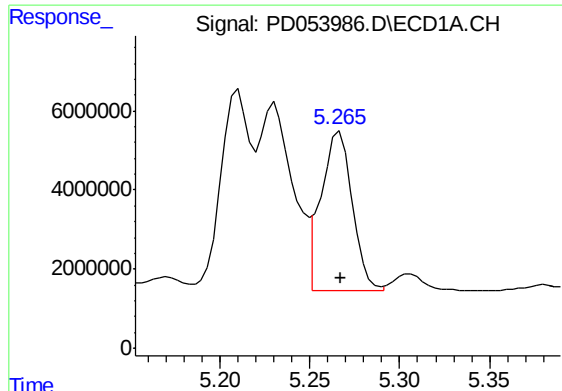

#26 Chlordane-4


R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 49538746
Conc: 694.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

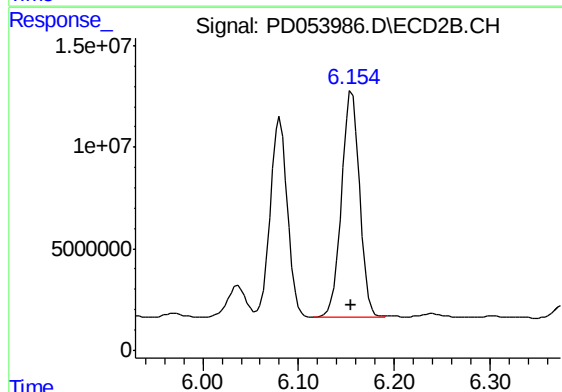


#26 Chlordane-4

R.T.: 6.156 min
Delta R.T.: 0.000 min
Response: 146644267
Conc: 690.16 ng/ml

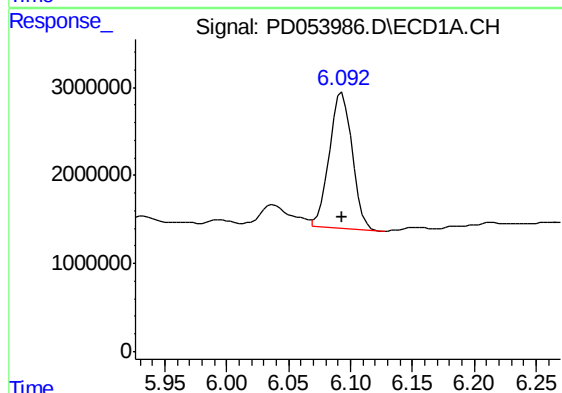


#27 Chlordane-5

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 20067938
Conc: 703.41 ng/ml

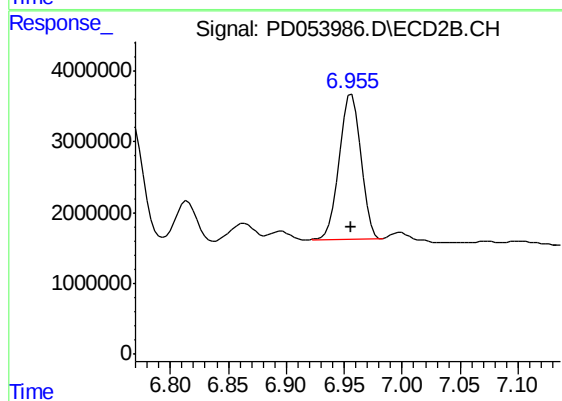

#27 Chlordane-5


R.T.: 6.957 min
Delta R.T.: 0.000 min
Response: 26963117
Conc: 708.73 ng/ml

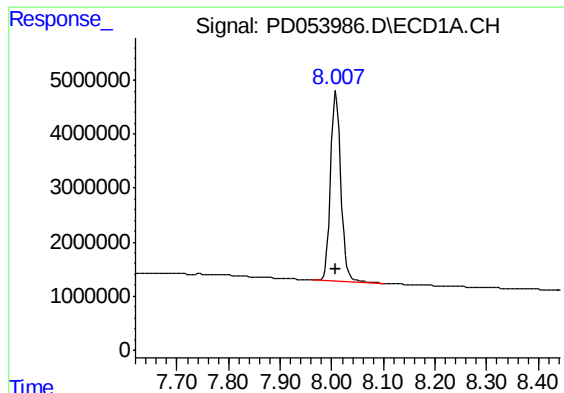

#28 Decachlorobiphenyl

R.T.: 8.008 min
Delta R.T.: 0.000 min
Response: 49231456
Conc: 73.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

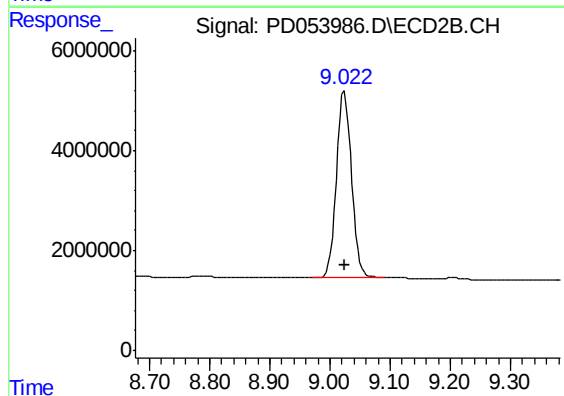

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 65531046
Conc: 72.75 ng/ml