

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071919\
 Data File : PD053996.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2019 20:43
 Operator : SM\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD071819CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 04:02:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 04:01:57 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.313	3.983	34008411	47115795	50.418	50.340
28)	SA Decachlor...	8.009	9.025	33076641	44927225	48.809	48.559
Target Compounds							
23)	Chlordane-1	4.159	4.973	10026936	18369675	506.752	490.344
24)	Chlordane-2	4.652	5.438	13297414	21769673	513.752	513.637
25)	Chlordane-3	5.210	6.081	39813603	85685201	500.602	489.304
26)	Chlordane-4	5.267	6.155	35173777	102.3E6	511.072	483.072
27)	Chlordane-5	6.093	6.957	13853707	18561154	518.666	493.701



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071919\
Data File : PD053996.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2019 20:43
Operator : SM\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD071819CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 04:02:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 04:01:57 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

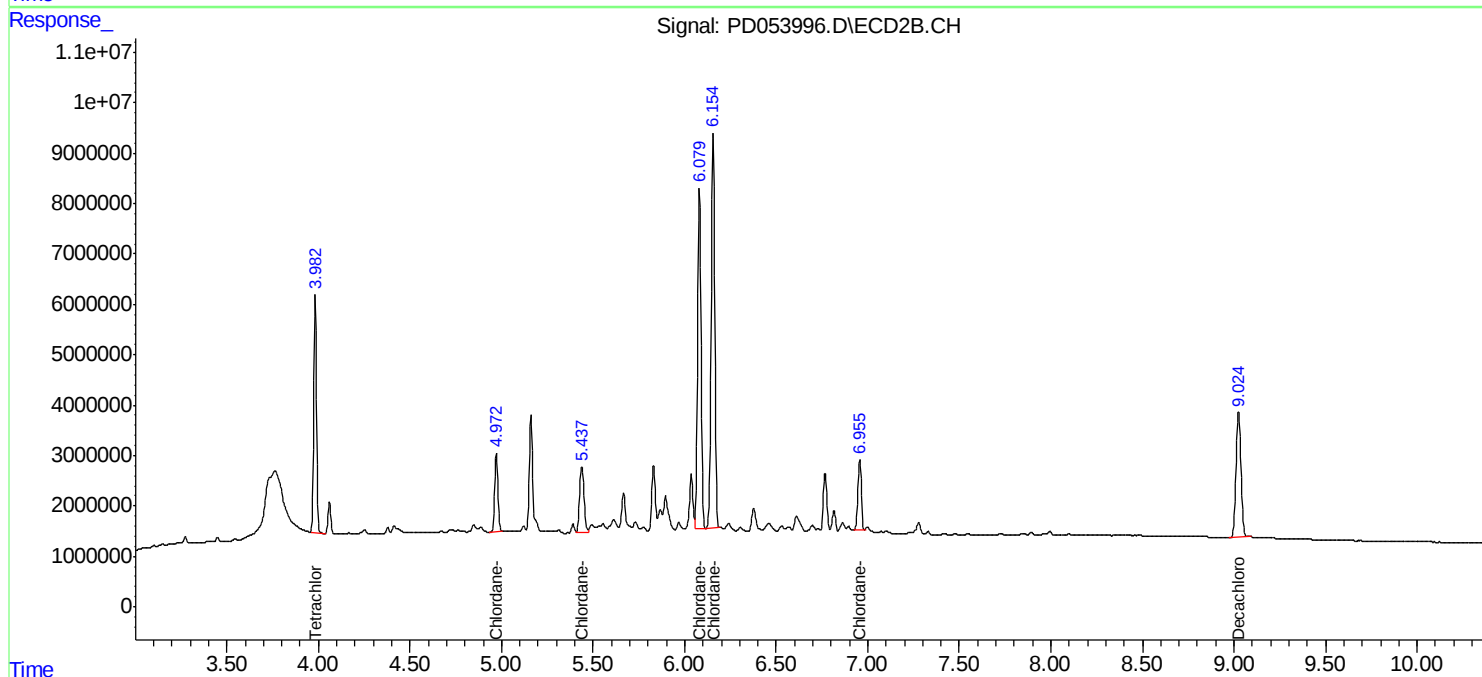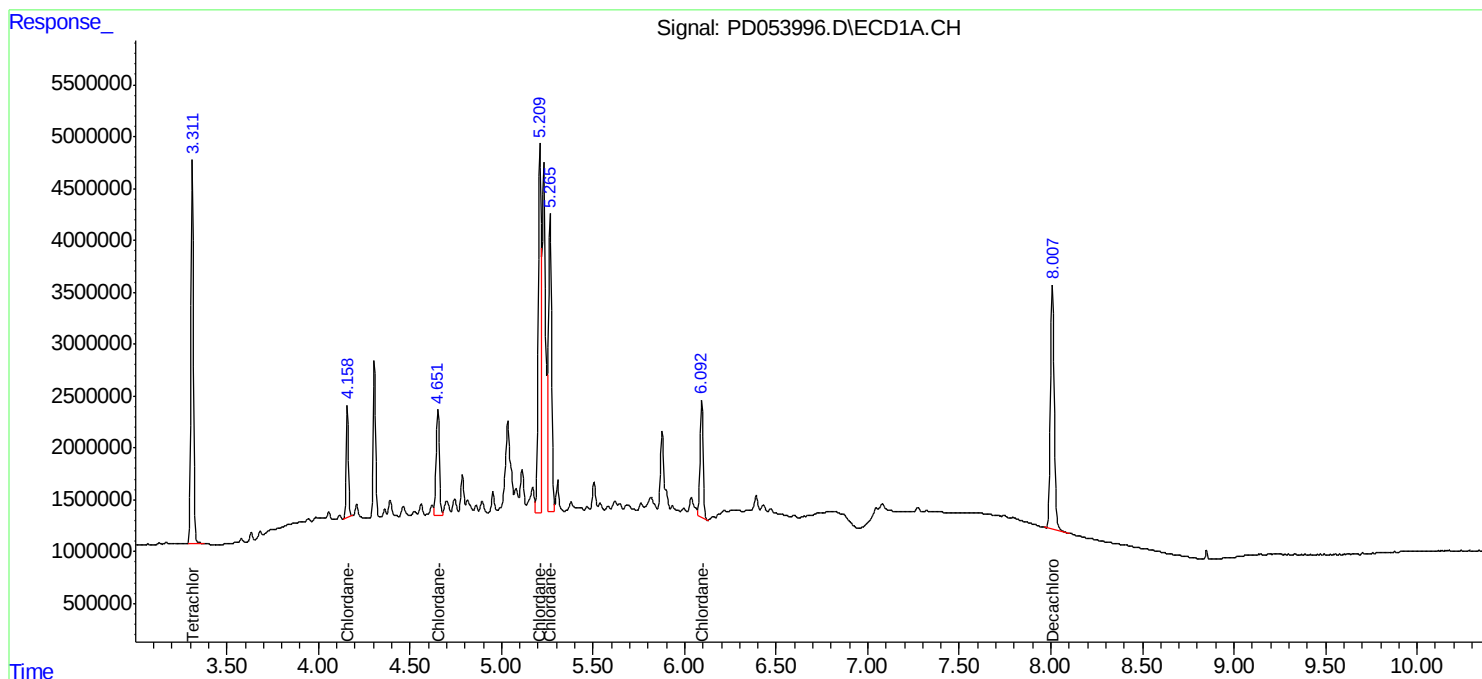


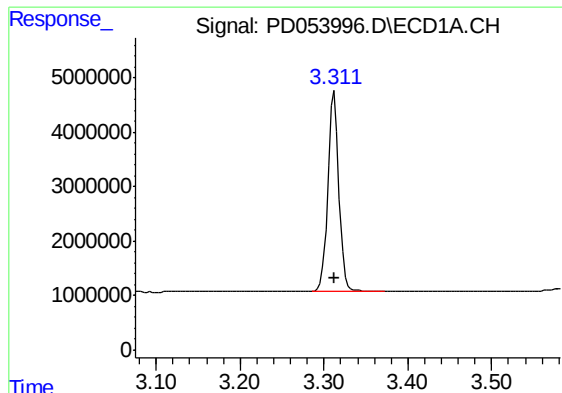

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: 0.000 min
Response: 34008411
Conc: 50.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071819CHLOR

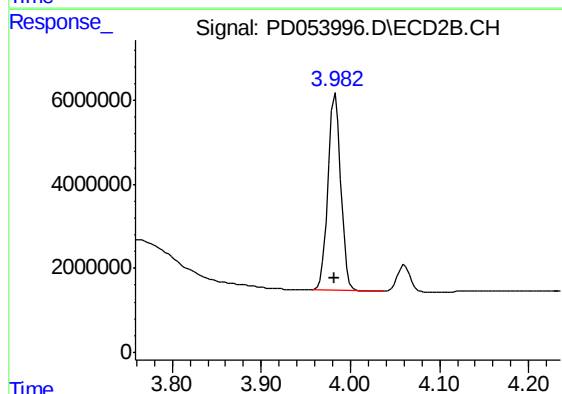


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 47115795
Conc: 50.34 ng/ml

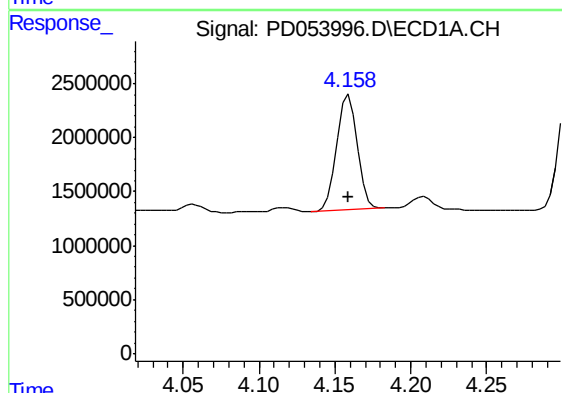


#23 Chlordane-1

R.T.: 4.159 min
Delta R.T.: 0.000 min
Response: 10026936
Conc: 506.75 ng/ml

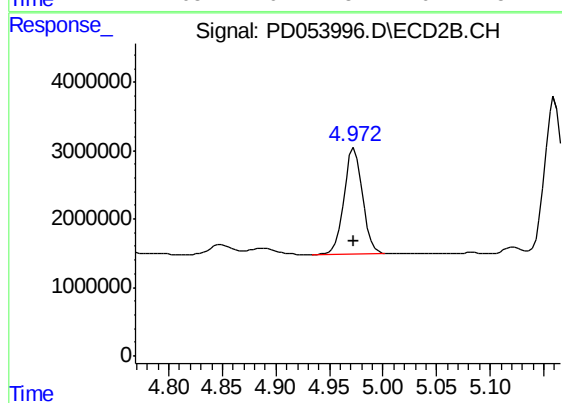

#23 Chlordane-1


R.T.: 4.973 min
Delta R.T.: 0.000 min
Response: 18369675
Conc: 490.34 ng/ml

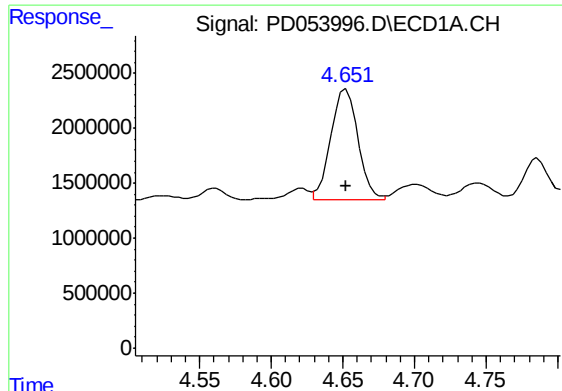

#24 Chlordane-2


R.T.: 4.652 min
Delta R.T.: 0.000 min
Response: 13297414
Conc: 513.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071819CHLOR

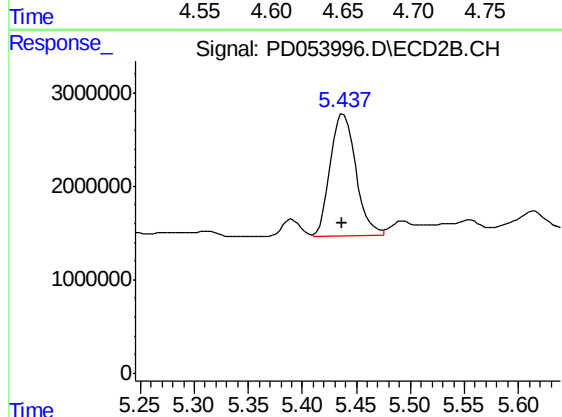


#24 Chlordane-2

R.T.: 5.438 min
Delta R.T.: 0.000 min
Response: 21769673
Conc: 513.64 ng/ml

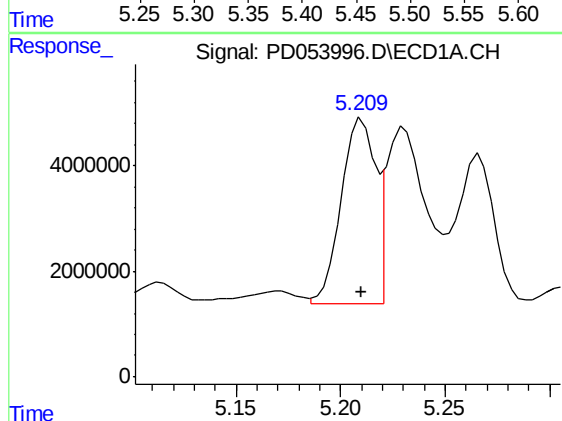


#25 Chlordane-3

R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 39813603
Conc: 500.60 ng/ml

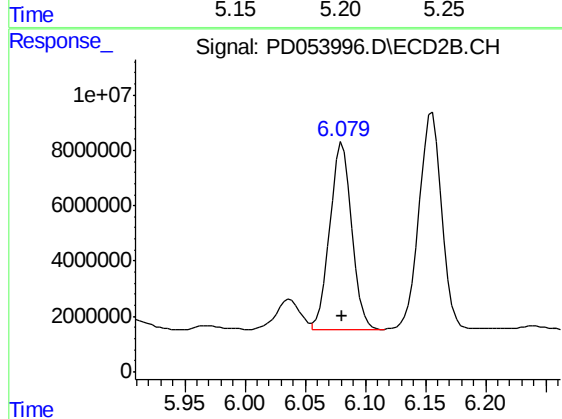

#25 Chlordane-3


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 85685201
Conc: 489.30 ng/ml

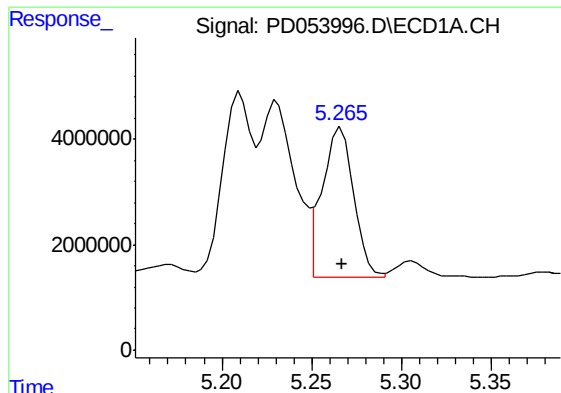

#26 Chlordane-4


R.T.: 5.267 min
Delta R.T.: 0.000 min
Response: 35173777
Conc: 511.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071819CHLOR

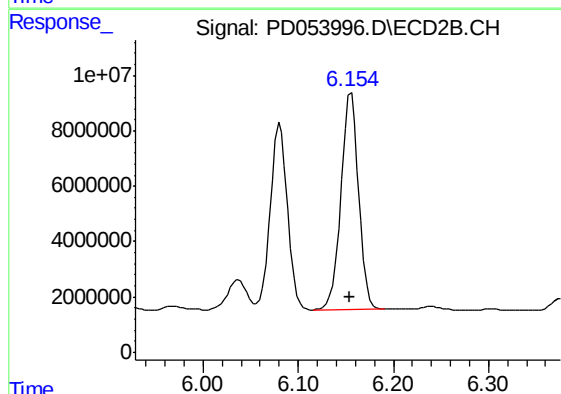


#26 Chlordane-4

R.T.: 6.155 min
Delta R.T.: 0.000 min
Response: 102254110
Conc: 483.07 ng/ml

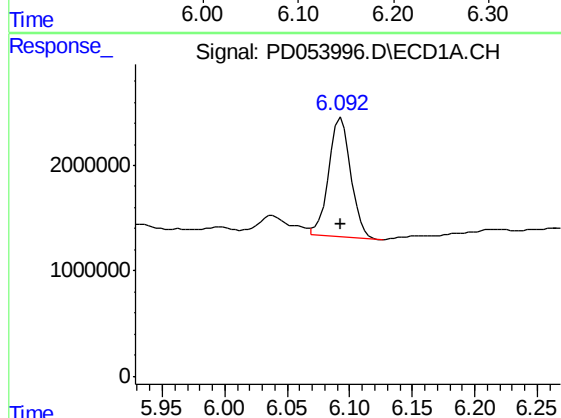


#27 Chlordane-5

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 13853707
Conc: 518.67 ng/ml

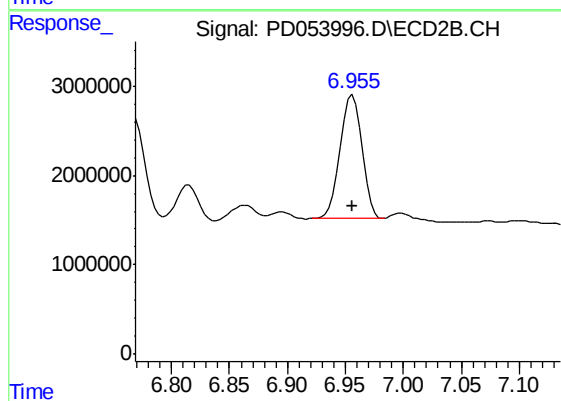

#27 Chlordane-5


R.T.: 6.957 min
Delta R.T.: 0.000 min
Response: 18561154
Conc: 493.70 ng/ml

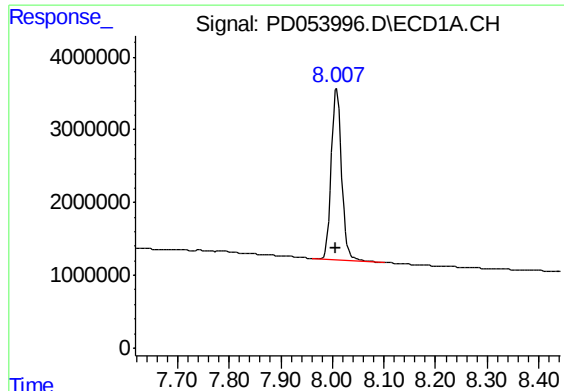

#28 Decachlorobiphenyl

R.T.: 8.009 min
Delta R.T.: 0.000 min
Response: 33076641
Conc: 48.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071819CHLOR

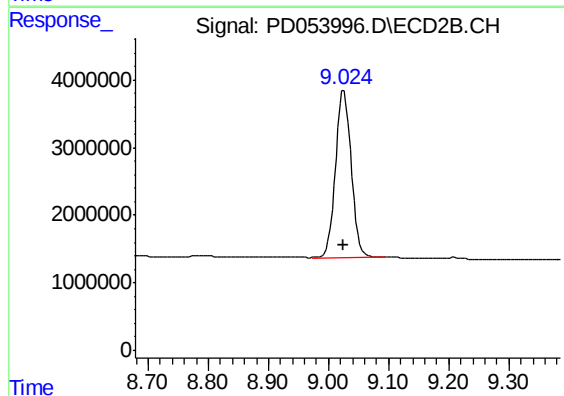

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 44927225
Conc: 48.56 ng/ml