

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071921\
 Data File : PD064328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2021 13:12
 Operator : AR\AJ
 Sample : M2995-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLX86MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 05:10:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 14 06:42:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.047	3.511	19881221	126.1E6	14.859	12.621
27)	SA Decachlor...	9.213	8.254	23353253	91278663	21.775	17.474
Target Compounds							
2)	A alpha-BHC	4.448	3.951	102.9E6	752.4E6	55.290	56.257
3)	MA gamma-BHC...	4.739	4.233	102.8E6	683.2E6	57.710	56.152
4)	MA Heptachlor	5.252	4.532	108.0E6	687.1E6	61.206	60.263
5)	MB Aldrin	5.561	4.780	102.0E6	647.9E6	63.997	62.547
6)	B beta-BHC	4.918	4.478	47228419	304.0E6	56.277	55.935
7)	B delta-BHC	5.138	4.684	33156948	229.6E6	19.413	20.883
8)	B Heptachlo...	5.957	5.221	96189003	554.3E6	63.100	60.669
9)	A Endosulfan I	6.319	5.560	89103582	475.3E6	64.488	56.210
10)	B trans-Chl...	6.193	5.446	96167231	558.3E6	60.843	60.013
11)	B cis-Chlor...	6.266	5.505	95840451	529.5E6	61.118	58.488
12)	B 4,4'-DDE	6.426	5.666	189.7E6	1035.8E6	136.906	123.601
13)	MA Dieldrin	6.580	5.803	201.6E6	1036.1E6	139.182	121.194
14)	MA Endrin	6.801	6.060	168.2E6	848.1E6	142.497	116.350
15)	B Endosulfa...	7.017	6.331	172.5E6	803.8E6	142.729	123.565
16)	A 4,4'-DDD	6.926	6.181	161.2E6	805.7E6	141.582	119.781
17)	MA 4,4'-DDT	7.226	6.422	172.4E6	825.6E6	149.368	117.923
18)	B Endrin al...	7.142	6.500	147.6E6	660.2E6	143.431	119.198
19)	B Endosulfa...	7.367	6.711	140.9E6	607.7E6	114.473	98.701
20)	A Methoxychlor	7.692	6.968	436.6E6	1608.3E6	680.494	521.200
21)	B Endrin ke...	7.846	7.206	197.3E6	828.1E6	148.461	122.214

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071921\
Data File : PD064328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2021 13:12
Operator : AR\AJ
Sample : M2995-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 05:10:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

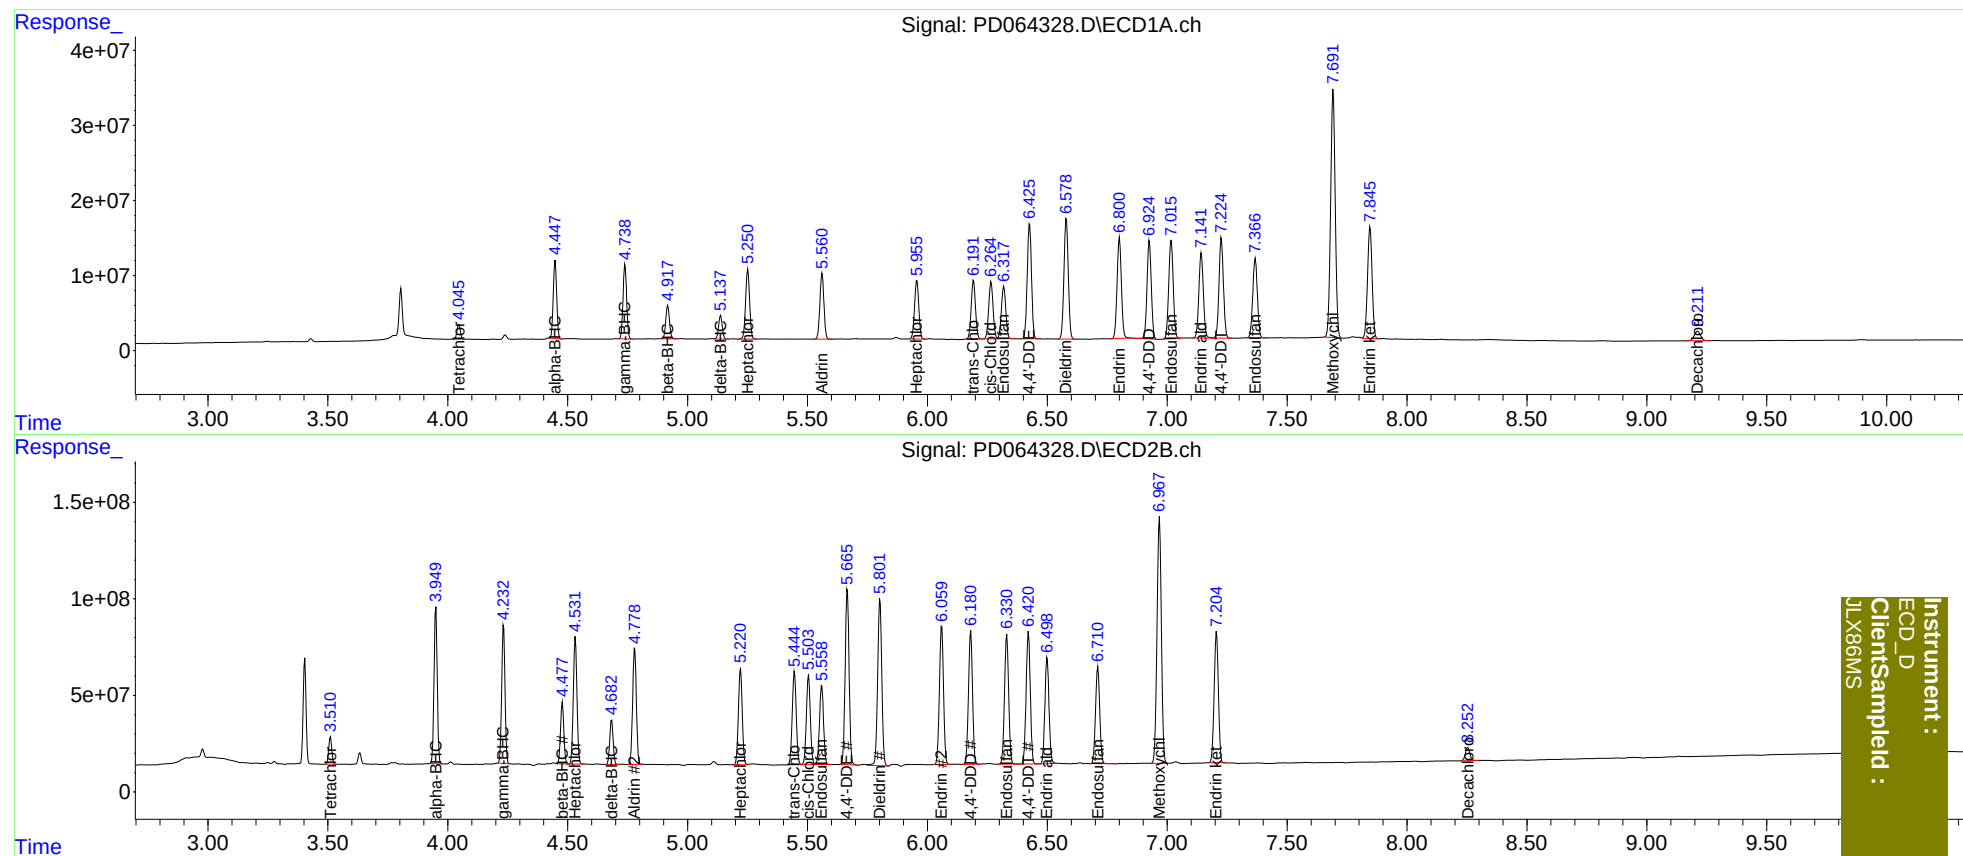

Instrument :
ECD_D
ClientSampled :
JLX86MS