

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071921\
 Data File : PD064326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2021 11:11
 Operator : AR\AJ
 Sample : PB137721BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS721

Manual Integrations
 APPROVED

Ankita
 7/20/2021 3:51:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 05:09:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 14 06:42:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.057	3.511	21799024	188.0E6	16.293	18.813
2)	SA Decachlor...	9.228	8.259	48331326	198.4E6	45.065	37.979
Target Compounds							
2)	A alpha-BHC	4.459	3.951	7171649	66342830	3.852	4.961 #
3)	MA gamma-BHC...	4.749	4.234	7133260	63529090	4.006m	5.222 #
4)	MA Heptachlor	5.264	4.533	8358375	62725178	4.738	5.501
5)	MB Aldrin	5.573	4.781	7339743	57292541	4.606	5.531
6)	B beta-BHC	4.928	4.480	4096724	27154708	4.882m	4.997
7)	B delta-BHC	5.150	4.685	3643177	30280843	2.133	2.754 #
8)	B Heptachlo...	5.969	5.223	7598226	49851843	4.984	5.456
9)	A Endosulfan I	6.331	5.562	6997559	45506459	5.064	5.382
10)	B trans-Chl...	6.205	5.449	7798059	49172205	4.934	5.286
11)	B cis-Chlor...	6.279	5.507	7638979	48531202	4.871	5.360
12)	B 4,4'-DDE	6.439	5.669	13053888	89161153	9.423	10.639
13)	MA Dieldrin	6.592	5.804	14307473	87074508	9.878m	10.186m
14)	MA Endrin	6.814	6.063	12177050	77001949	10.314	10.564
15)	B Endosulfa...	7.030	6.334	15327480	72074152	12.682	11.079
16)	A 4,4'-DDD	6.939	6.184	10613247	70724875	9.321	10.514
17)	MA 4,4'-DDT	7.240	6.424	12232099	68175837	10.596	9.738
18)	B Endrin al...	7.156	6.503	11851314	59201749	11.513	10.689
19)	B Endosulfa...	7.380	6.714	12575545	55185076	10.214	8.963
20)	A Methoxychlor	7.704	6.970	35661613	161.1E6	55.579m	52.200m
21)	B Endrin ke...	7.859	7.209	15658244	73995328	11.782	10.920

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071921\
Data File : PD064326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2021 11:11
Operator : AR\AJ
Sample : PB137721BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 05:09:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

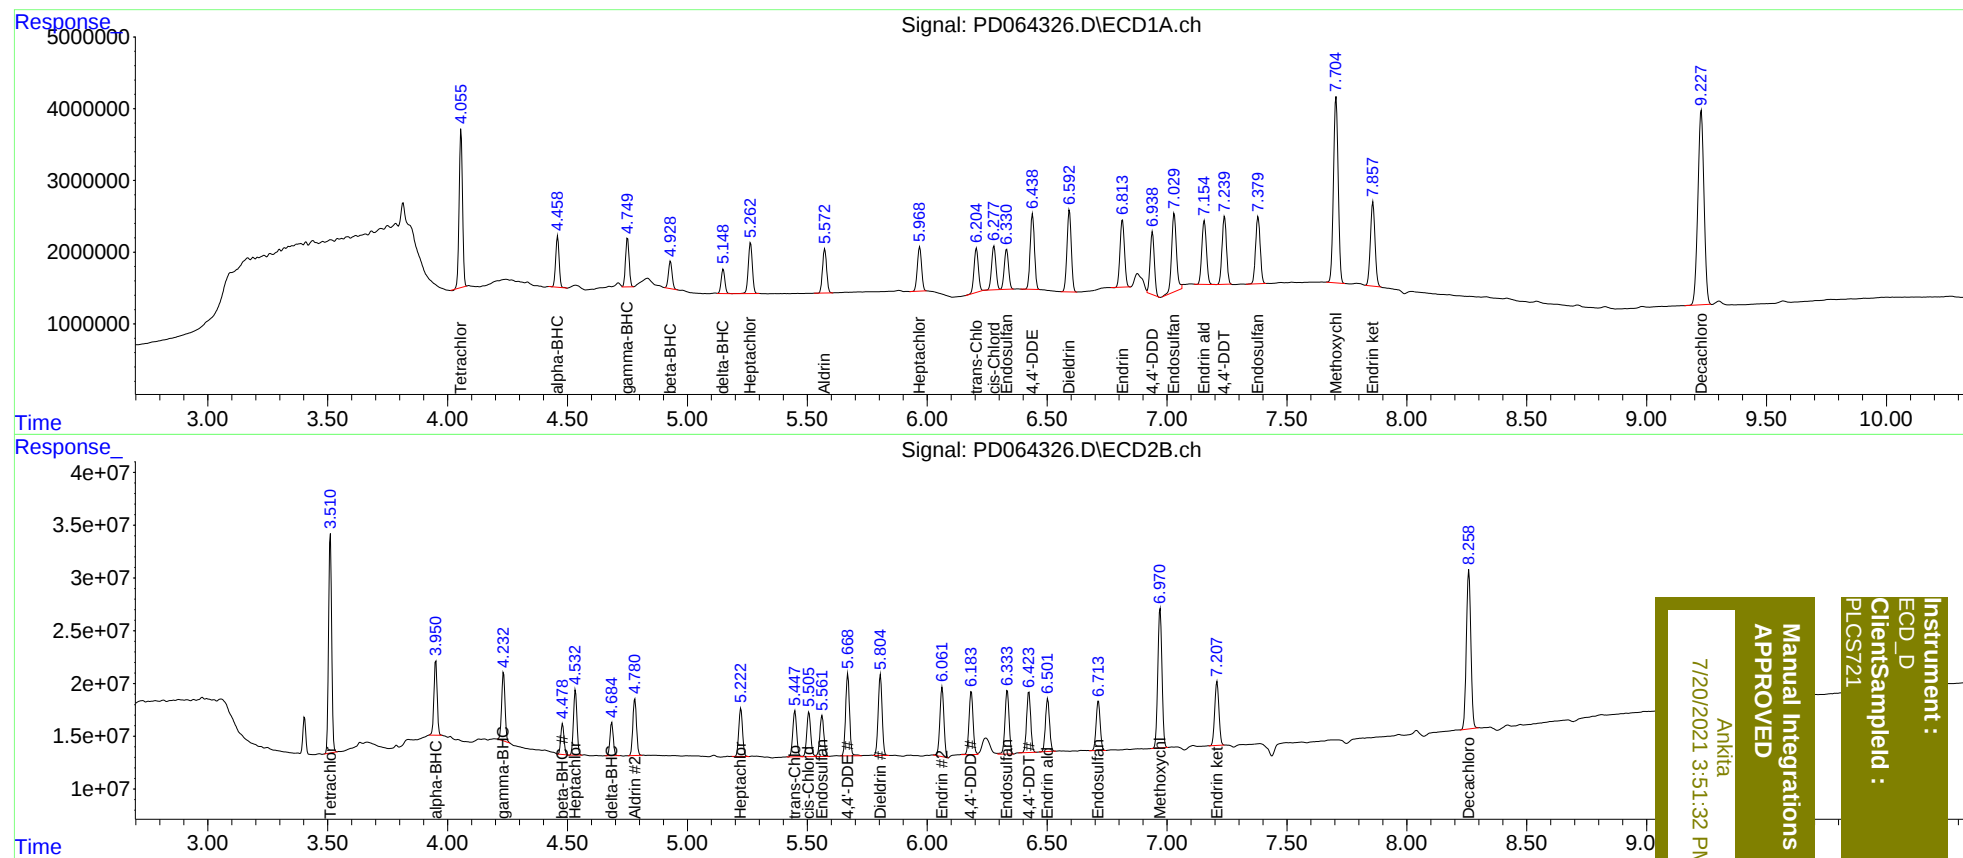

Manual Integrations
APPROVED

Ankita
7/20/2021 3:51:32 PM

Instrument :
ECD_D
ClientSampled :
PLC5721