

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071921\
 Data File : PD064329.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2021 13:45
 Operator : AR\AJ
 Sample : M2995-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLX86MSD

Manual Integrations
 APPROVED

mohammad
 7/22/2021 5:04:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 05:10:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 14 06:42:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.057	3.511	20413404	123.9E6	15.257	12.405
2)	SA Decachlor...	9.227	8.257	23391468	90028356	21.811	17.234
Target Compounds							
2)	A alpha-BHC	4.459	3.951	103.3E6	733.7E6	55.458	54.866
3)	MA gamma-BHC...	4.751	4.234	101.0E6	671.0E6	56.727	55.151
4)	MA Heptachlor	5.263	4.533	106.1E6	669.8E6	60.153	58.748
5)	MB Aldrin	5.573	4.781	100.4E6	631.0E6	62.981	60.922
6)	B beta-BHC	4.930	4.479	45926821	294.9E6	54.726	54.265
7)	B delta-BHC	5.150	4.685	32579542	223.5E6	19.075	20.328
8)	B Heptachlo...	5.969	5.223	94921364	538.6E6	62.269	58.951
9)	A Endosulfan I	6.331	5.562	86836946	462.7E6	62.848	54.725
10)	B trans-Chl...	6.204	5.448	96495355	541.6E6	61.050m	58.220
11)	B cis-Chlor...	6.277	5.506	95296180	517.1E6	60.771m	57.114
12)	B 4,4'-DDE	6.440	5.669	187.1E6	1010.3E6	135.050	120.552
13)	MA Dieldrin	6.592	5.804	197.8E6	1014.6E6	136.576m	118.687
14)	MA Endrin	6.813	6.062	161.5E6	830.7E6	136.798	113.961
15)	B Endosulfa...	7.029	6.333	169.7E6	786.2E6	140.428	120.855
16)	A 4,4'-DDD	6.939	6.183	155.5E6	789.9E6	136.561	117.432
17)	MA 4,4'-DDT	7.241	6.424	165.8E6	812.4E6	143.638	116.033
18)	B Endrin al...	7.156	6.502	142.8E6	651.6E6	138.758	117.653
19)	B Endosulfa...	7.380	6.714	138.6E6	596.3E6	112.580	96.845
20)	A Methoxychlor	7.702	6.970	432.3E6	1595.2E6	673.705m	516.950
21)	B Endrin ke...	7.858	7.208	192.8E6	820.1E6	145.048	121.034

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071921\
Data File : PD064329.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2021 13:45
Operator : AR\AJ
Sample : M2995-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 05:10:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070921CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 06:42:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

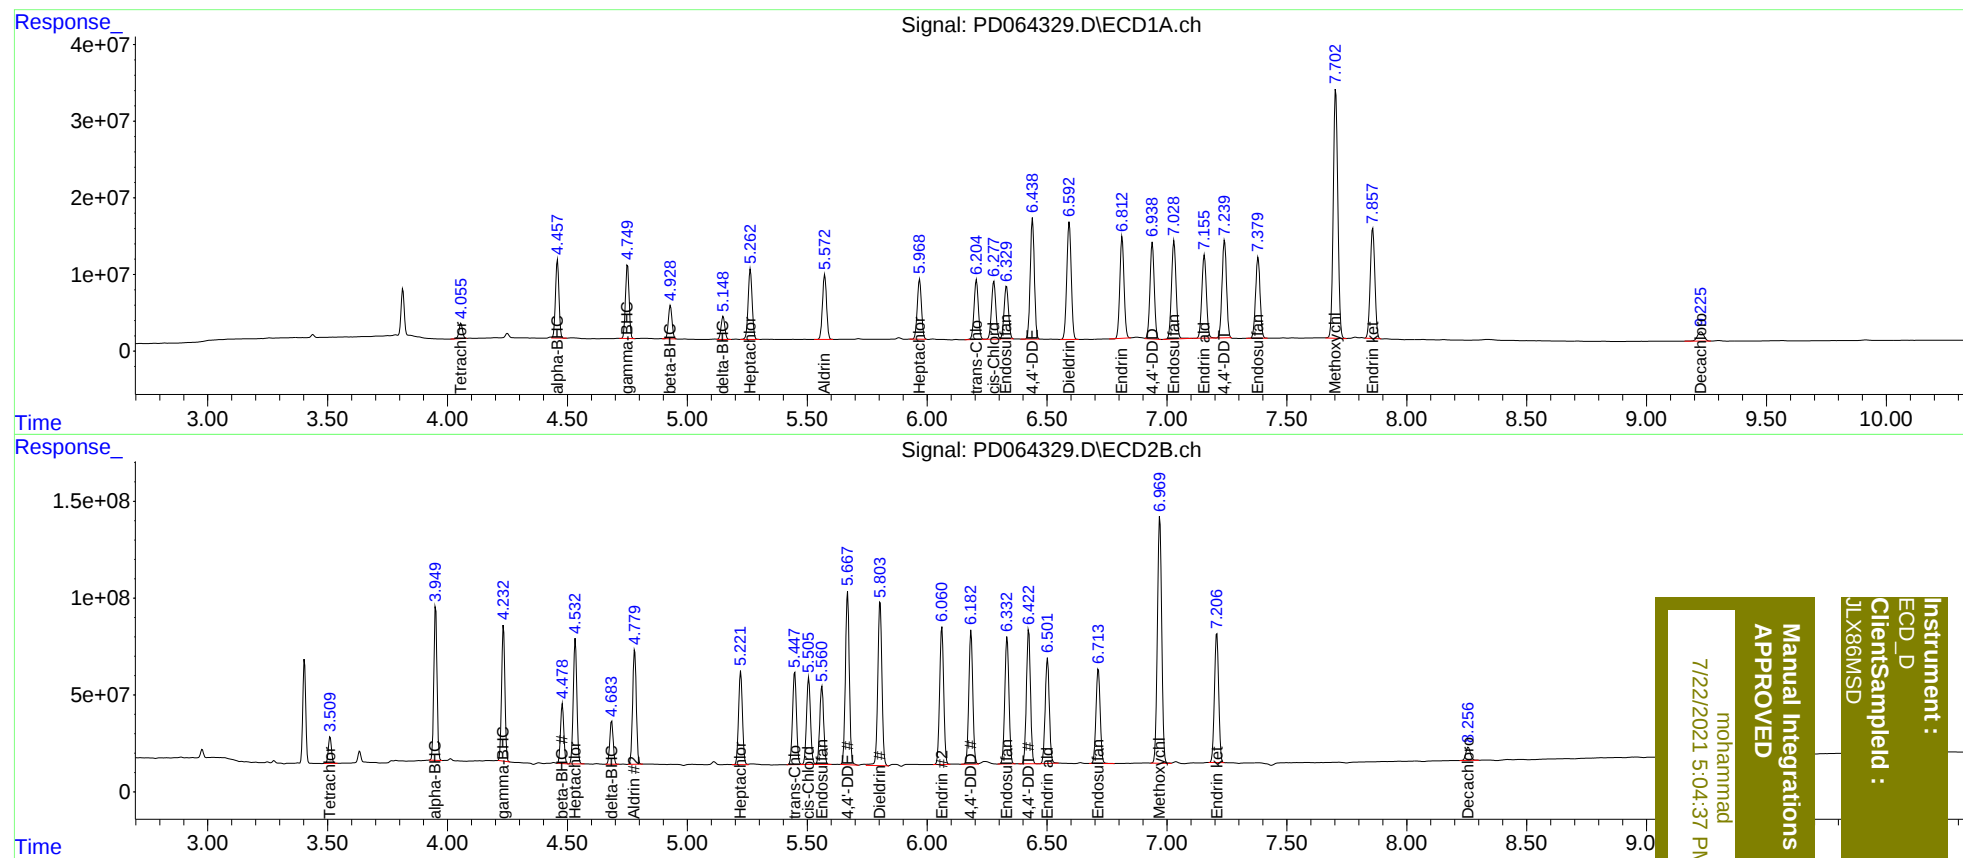

Manual Integrations
APPROVED

7/22/2021 5:04:37 PM
mohammad

Instrument :
ECD_D
ClientSampled :
JLX86MSD