

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
 Data File : PD071023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2022 06:25
 Operator : AR\AJ
 Sample : N3214-07
 Misc : TOX LOD 50PPB
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/20/2022
 Supervised By :Ankita Jodhani 07/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 08:41:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 05:25:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.474	4.125	48228307	522.2E6	19.114	20.841
7) SA Decachlor...	8.242	9.321	55800143	215.7E6	20.880	21.554
Target Compounds						
2) Toxaphene-1	5.737	6.156	1321949	2224704	57.736	59.396
3) Toxaphene-2	5.953	6.762	1759260	7412339	48.098	61.316 #
4) Toxaphene-3	6.341	7.441	2700679	11895814	49.808	53.305
5) Toxaphene-4	6.587	7.582	2879401	5375812	50.337	48.280
6) Toxaphene-5	7.073	7.865	3307181	8296980	54.974m	55.975

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
Data File : PD071023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2022 06:25
Operator : AR\AJ
Sample : N3214-07
Misc : TOX LOD 50PPB
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 08:41:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 05:25:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

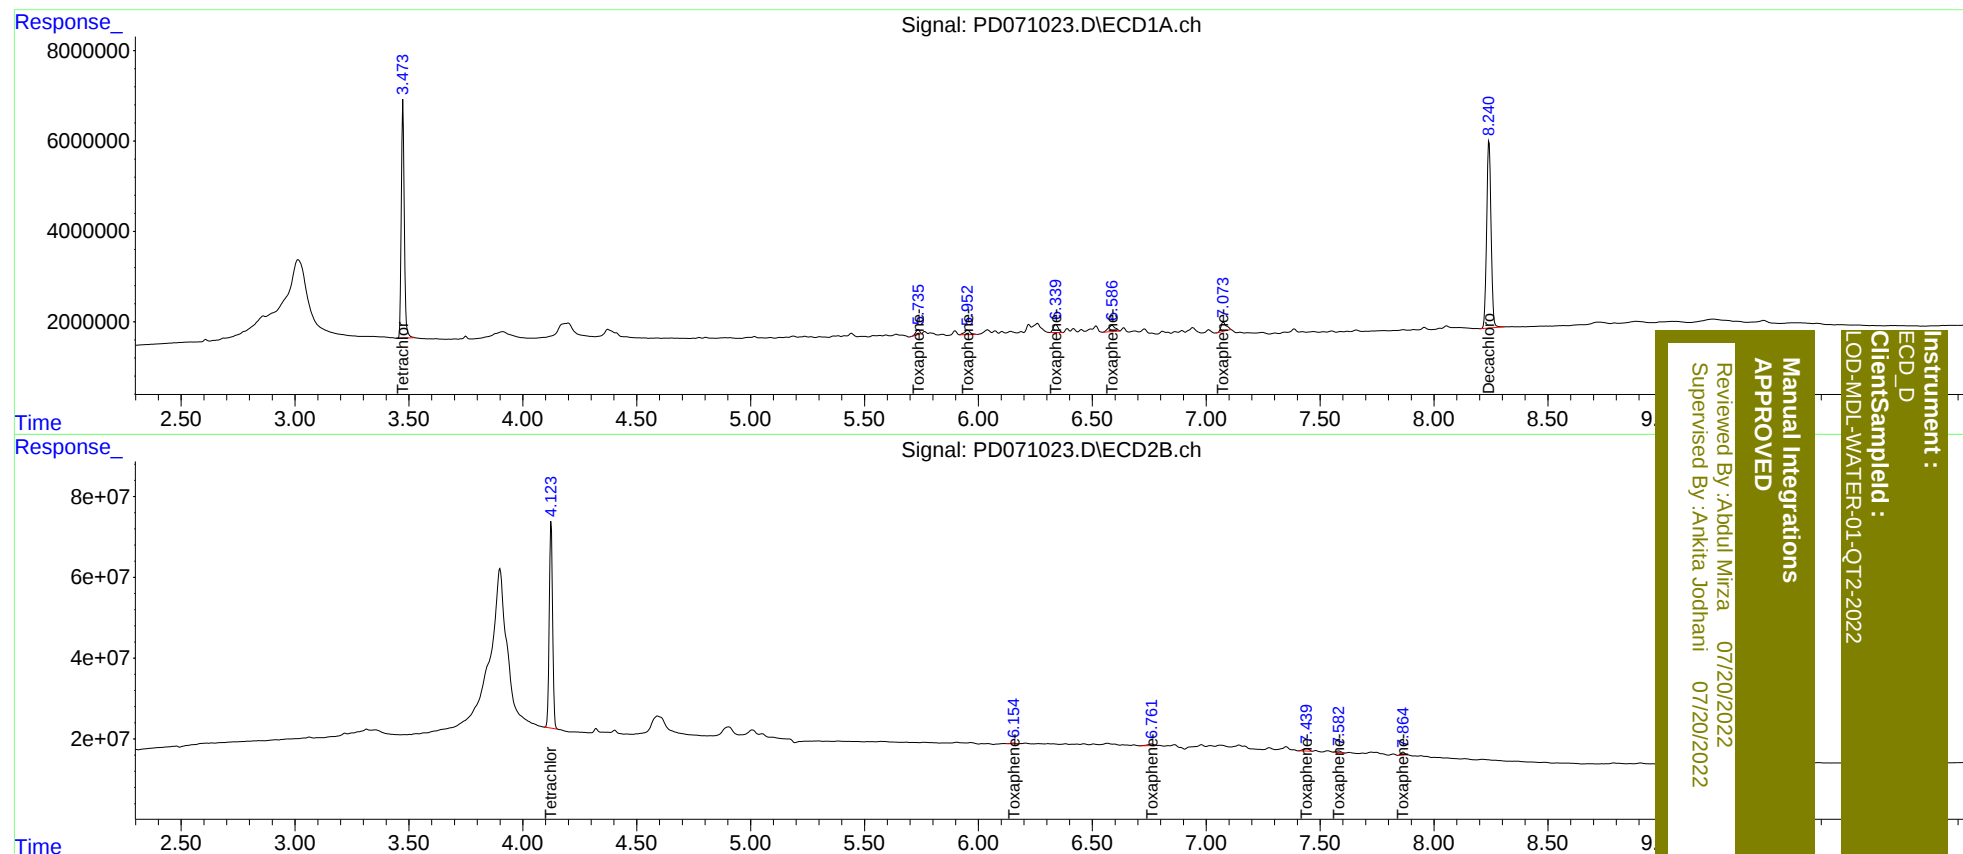

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 07/20/2022
Supervised By: Ankita Jodhani 07/20/2022

Instrument :
ECD_D
Client Sample :
LOD-MDL-WATER-01-QT2-2022