

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
 Data File : PD070989.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2022 21:13
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 04:16:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 04:16:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.125	328.3E6	2529.3E6	100.533	98.522
28)	SA Decachlor...	8.244	9.322	272.6E6	962.6E6	98.523	96.085
Target Compounds							
23)	Chlordane-1	4.348	5.147	107.1E6	738.9E6	995.829	941.001
24)	Chlordane-2	4.851	5.626	114.8E6	530.5E6	963.569	949.984
25)	Chlordane-3	5.420	6.284	372.7E6	1865.9E6	1005.003	976.184
26)	Chlordane-4	5.479	6.358	305.4E6	2149.5E6	1005.837	974.274
27)	Chlordane-5	6.318	7.181	124.5E6	456.7E6	1000.343	968.266



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
Data File : PD070989.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2022 21:13
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 04:16:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 04:16:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

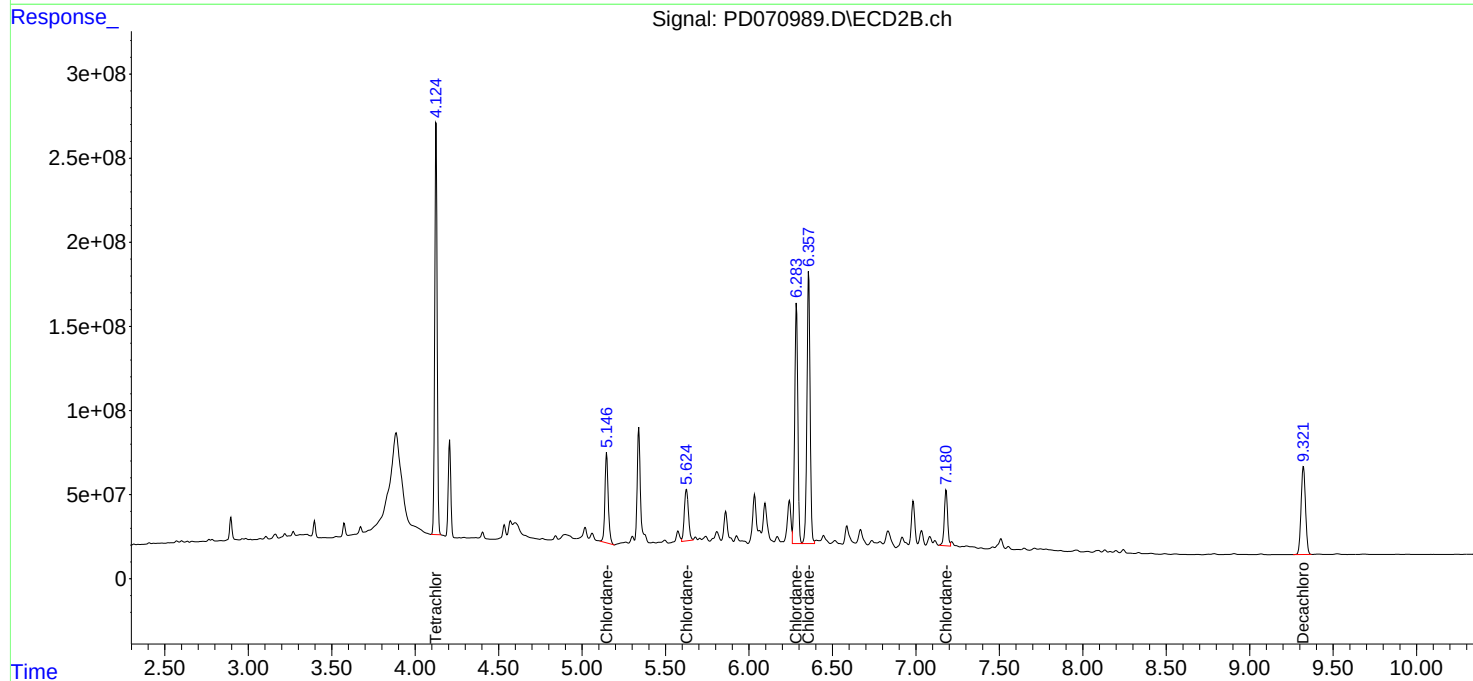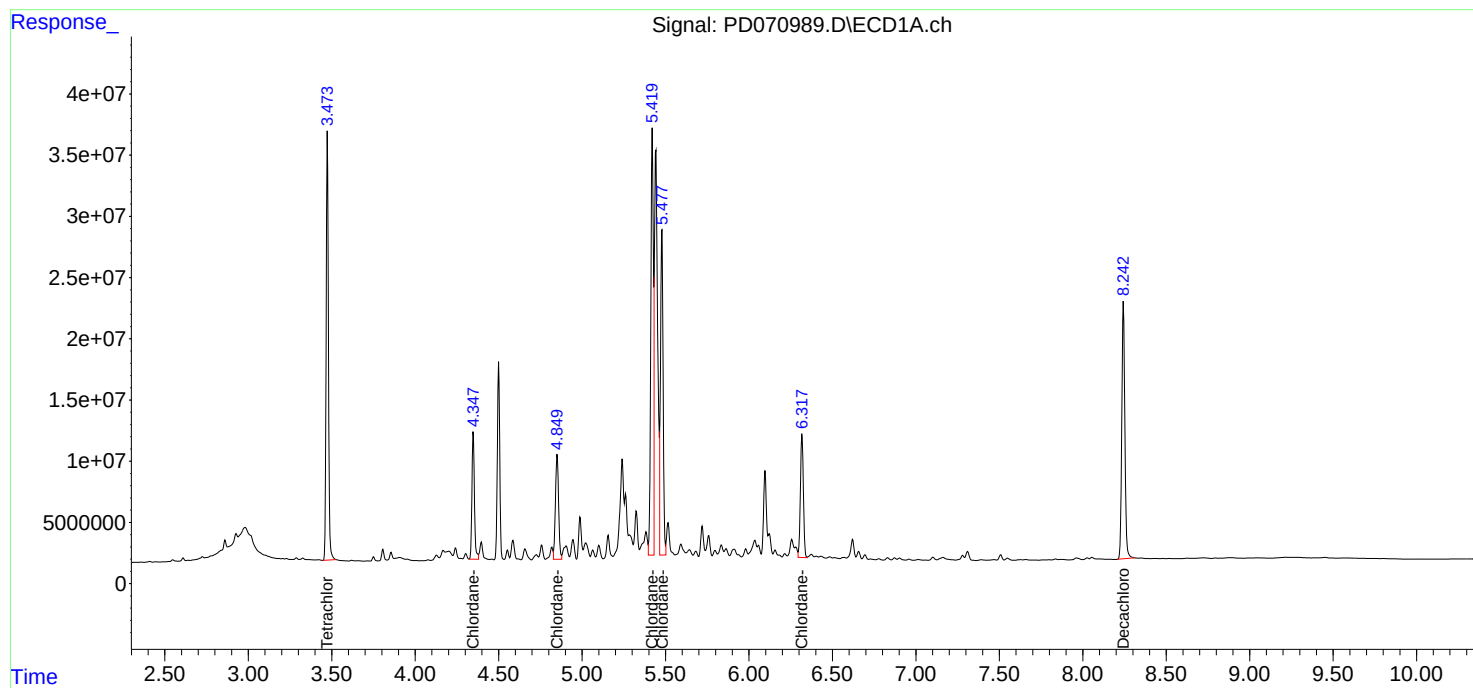


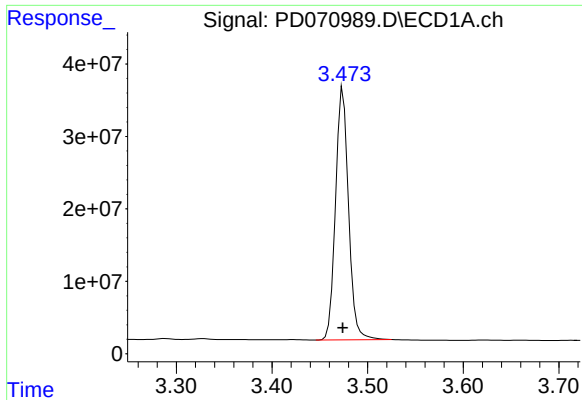

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 328348614
Conc: 100.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

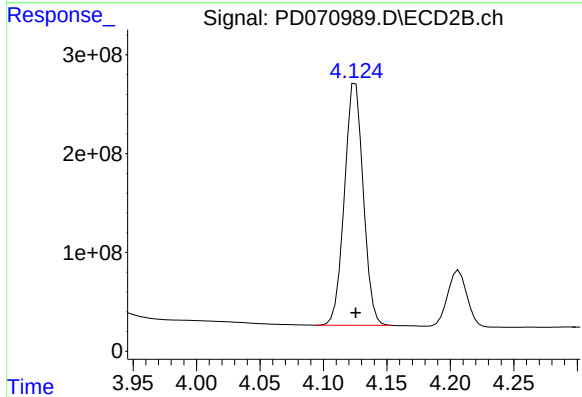


#1 Tetrachloro-m-xylene

R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 2529318759
Conc: 98.52 ng/ml

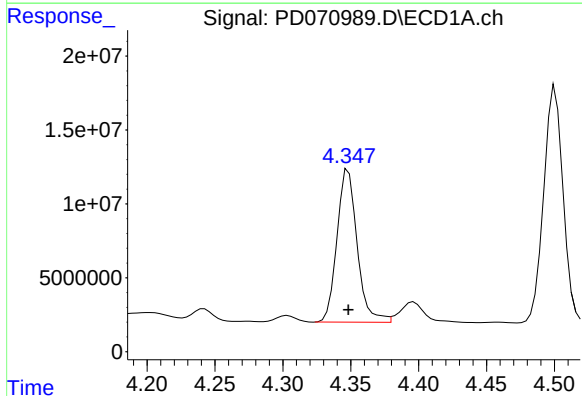


#23 Chlordane-1

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 107067212
Conc: 995.83 ng/ml

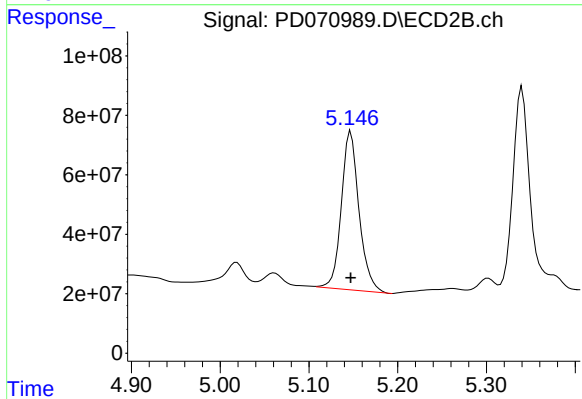

#23 Chlordane-1


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 738935631
Conc: 941.00 ng/ml

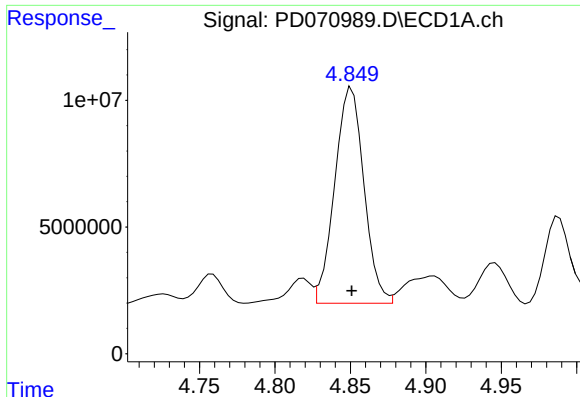

#24 Chlordane-2


R.T.: 4.851 min
Delta R.T.: 0.000 min
Response: 114815394
Conc: 963.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

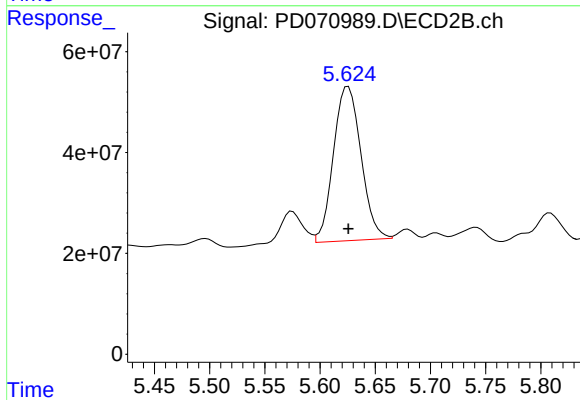


#24 Chlordane-2

R.T.: 5.626 min
Delta R.T.: 0.000 min
Response: 530538971
Conc: 949.98 ng/ml

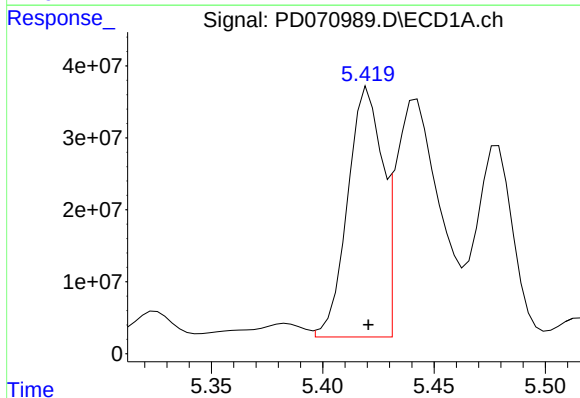


#25 Chlordane-3

R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 372690603
Conc: 1005.00 ng/ml

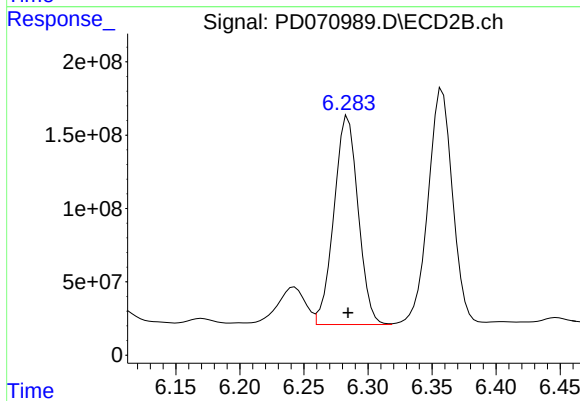

#25 Chlordane-3


R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 1865947239
Conc: 976.18 ng/ml

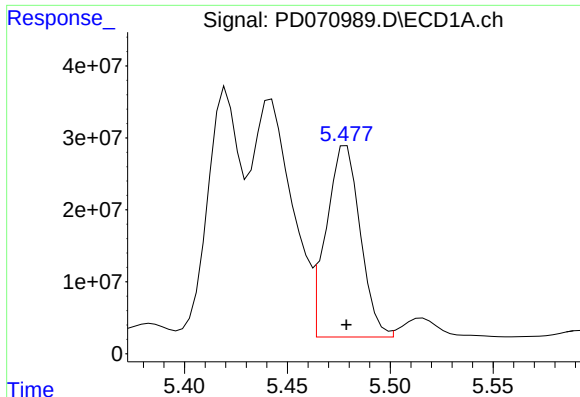

#26 Chlordane-4


R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 305412927
Conc: 1005.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

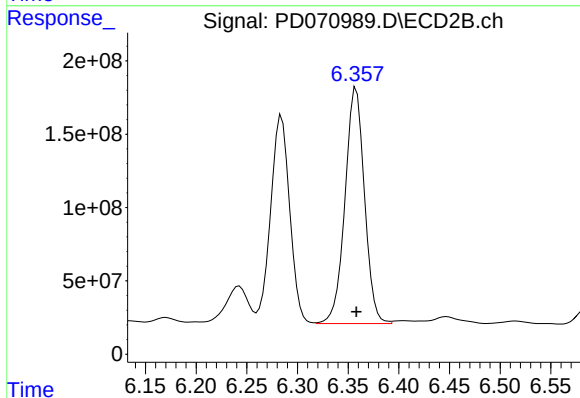


#26 Chlordane-4

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 2149479289
Conc: 974.27 ng/ml

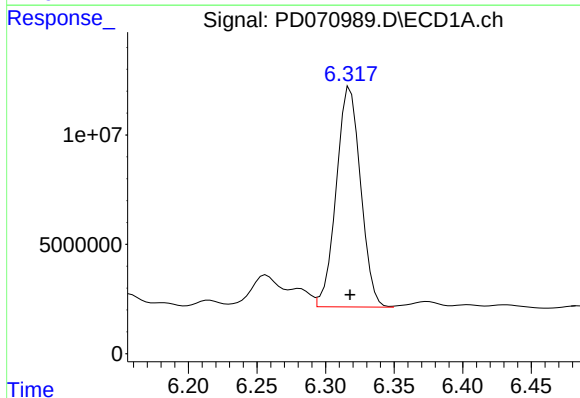


#27 Chlordane-5

R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 124468862
Conc: 1000.34 ng/ml

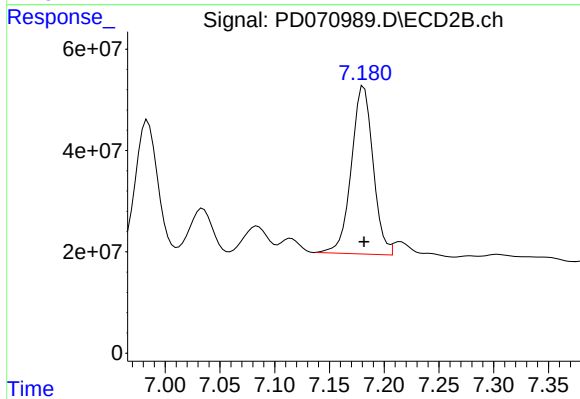

#27 Chlordane-5


R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 456723484
Conc: 968.27 ng/ml

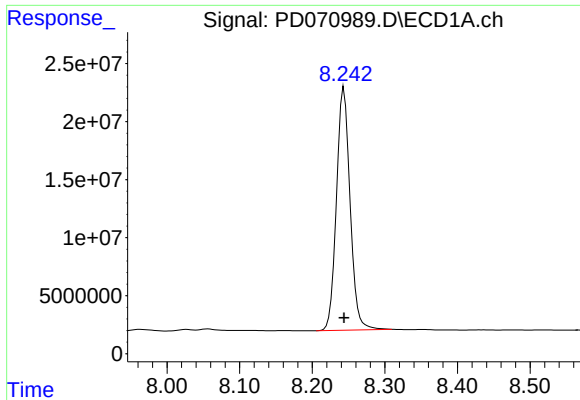

#28 Decachlorobiphenyl

R.T.: 8.244 min
Delta R.T.: 0.000 min
Response: 272550654
Conc: 98.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

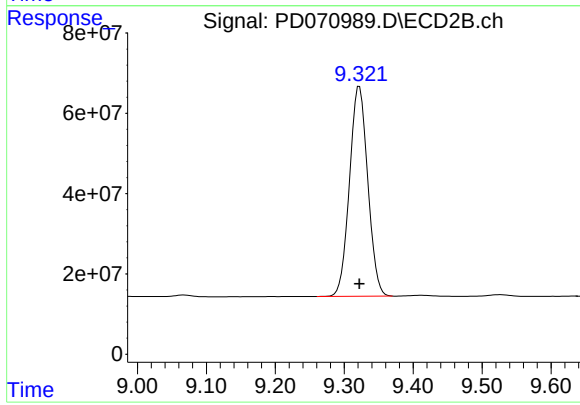

#28 Decachlorobiphenyl

R.T.: 9.322 min
Delta R.T.: 0.000 min
Response: 962569163
Conc: 96.09 ng/ml