

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
 Data File : PD070990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2022 21:28
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 04:18:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 04:18:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.125	238.8E6	1870.6E6	73.726	73.562
28)	SA Decachlor...	8.244	9.322	201.6E6	729.1E6	73.575	73.505
Target Compounds							
23)	Chlordane-1	4.348	5.147	77644286	558.6E6	731.212	723.797
24)	Chlordane-2	4.851	5.625	85264780	399.8E6	726.690	726.913
25)	Chlordane-3	5.421	6.284	272.7E6	1385.1E6	740.221	732.900
26)	Chlordane-4	5.479	6.358	221.9E6	1599.1E6	737.002	733.003
27)	Chlordane-5	6.318	7.181	90361625	342.4E6	733.982	733.806



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
Data File : PD070990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2022 21:28
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 04:18:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 04:18:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

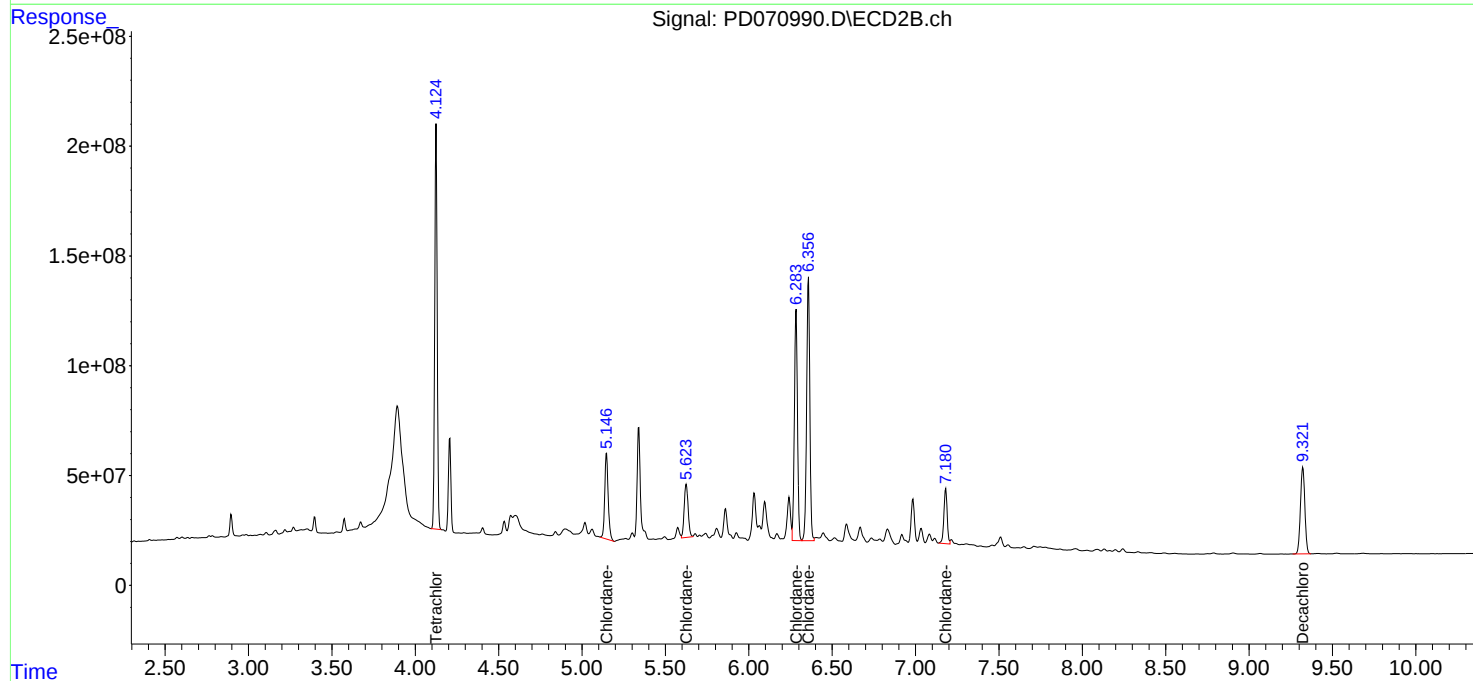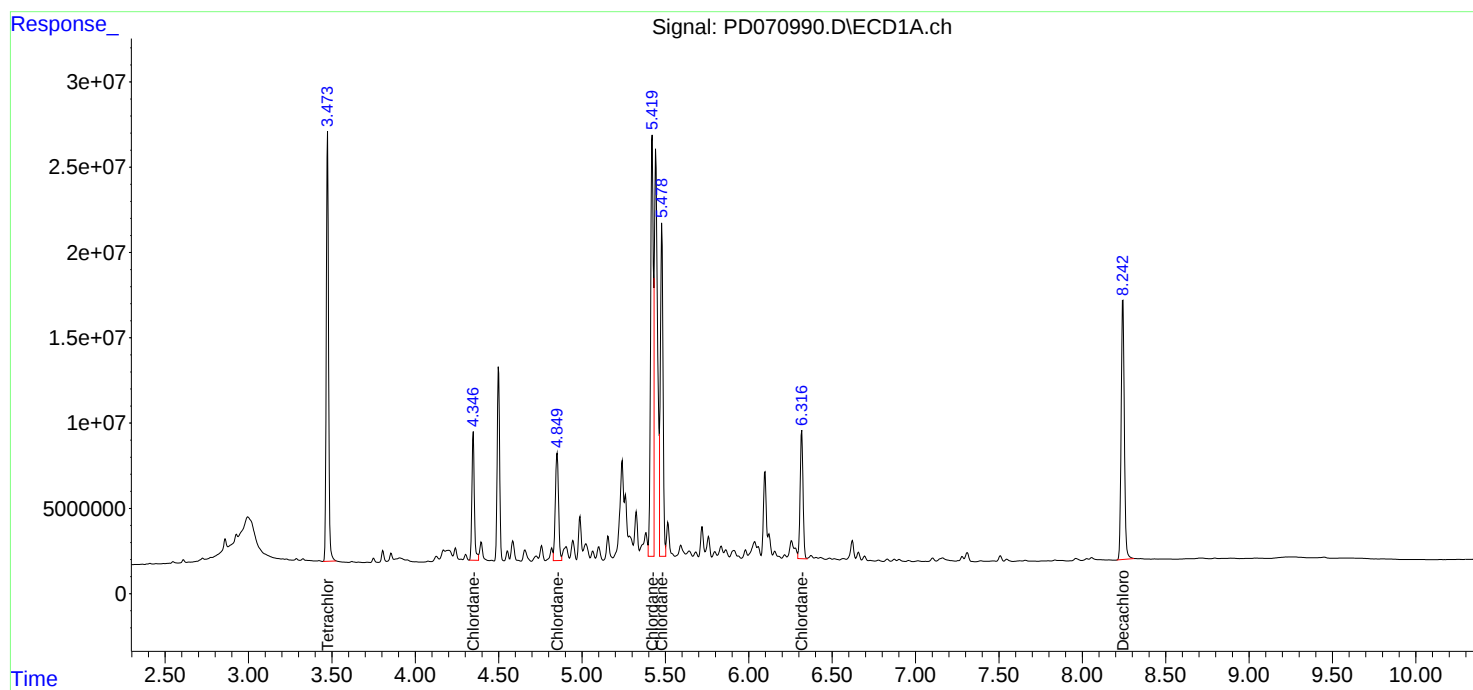


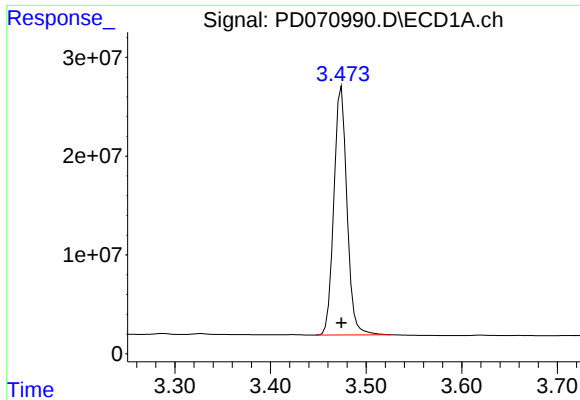

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 238764053
Conc: 73.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

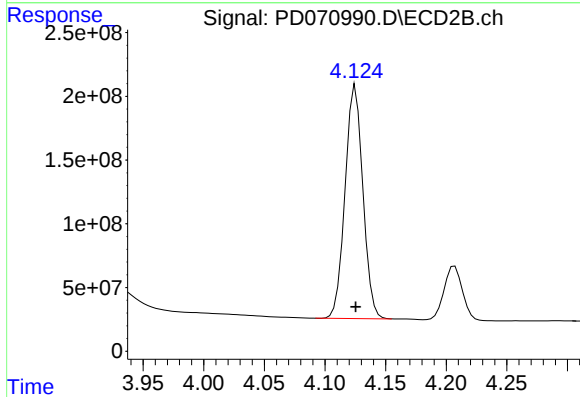


#1 Tetrachloro-m-xylene

R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 1870613920
Conc: 73.56 ng/ml

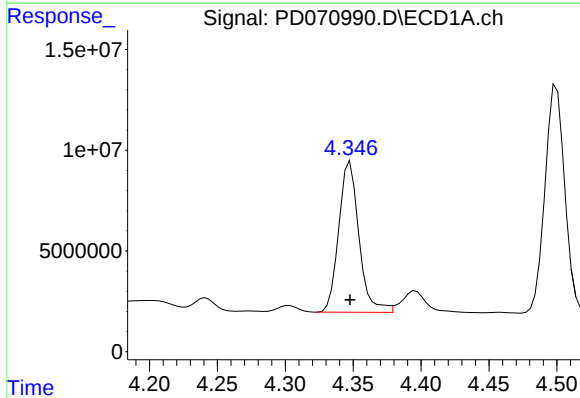


#23 Chlordane-1

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 77644286
Conc: 731.21 ng/ml

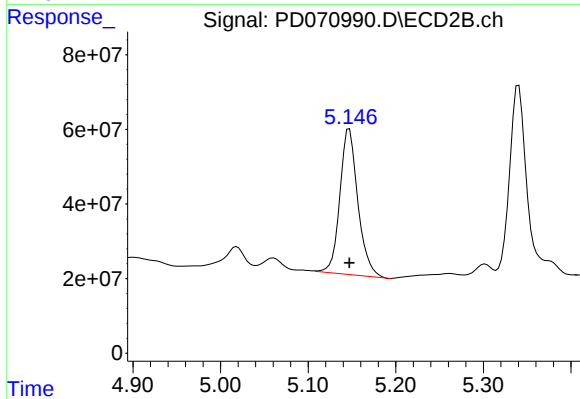

#23 Chlordane-1


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 558614087
Conc: 723.80 ng/ml

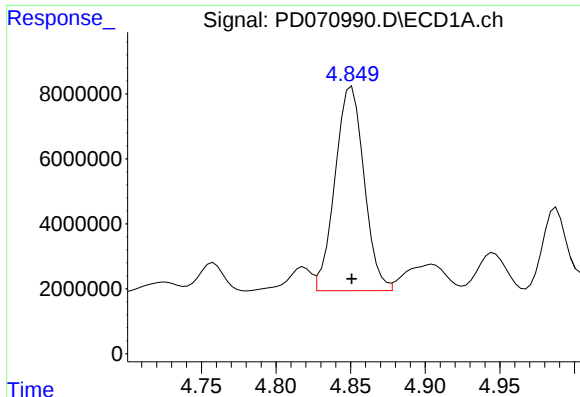

#24 Chlordane-2


R.T.: 4.851 min
Delta R.T.: 0.000 min
Response: 85264780
Conc: 726.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

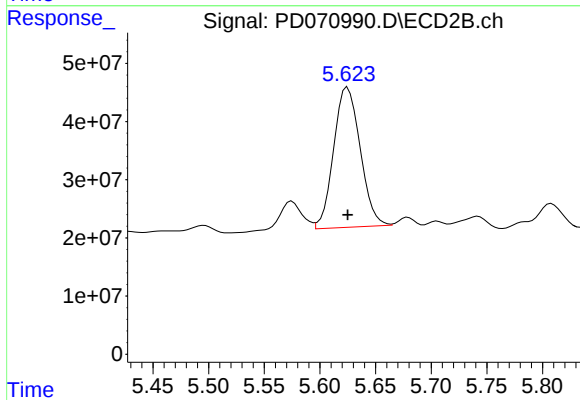


#24 Chlordane-2

R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 399806323
Conc: 726.91 ng/ml

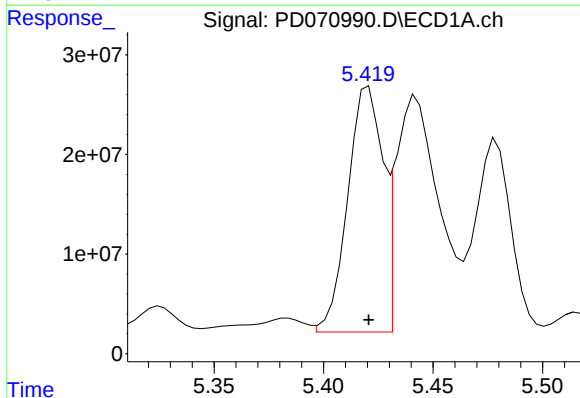


#25 Chlordane-3

R.T.: 5.421 min
Delta R.T.: 0.000 min
Response: 272722160
Conc: 740.22 ng/ml

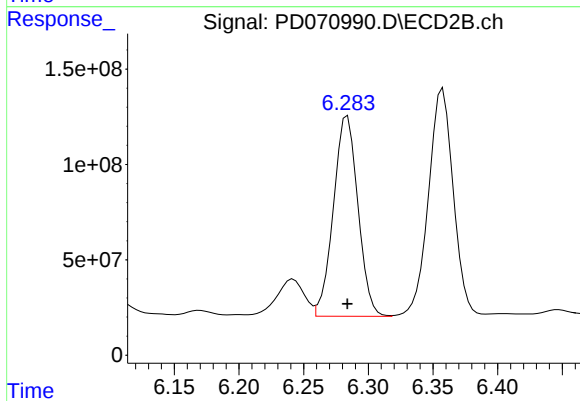

#25 Chlordane-3


R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 1385127098
Conc: 732.90 ng/ml

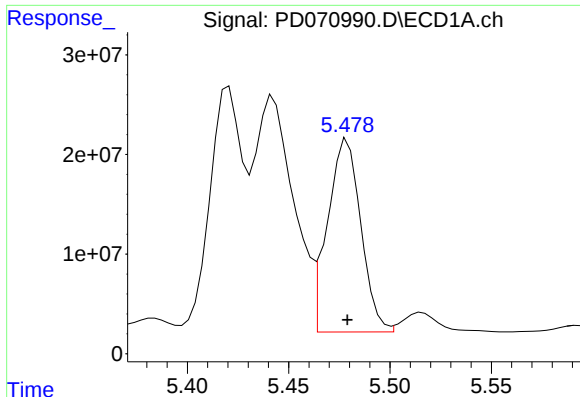

#26 Chlordane-4


R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 221860970
Conc: 737.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

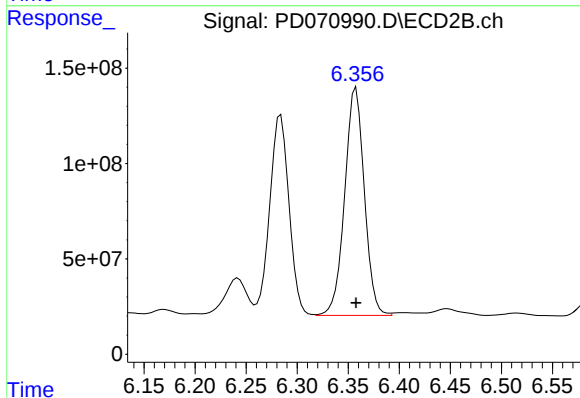


#26 Chlordane-4

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 1599058690
Conc: 733.00 ng/ml

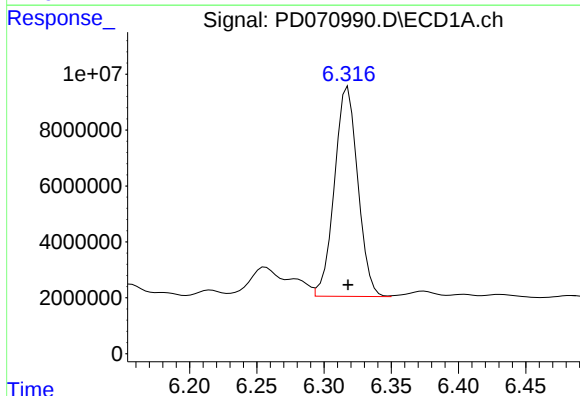


#27 Chlordane-5

R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 90361625
Conc: 733.98 ng/ml

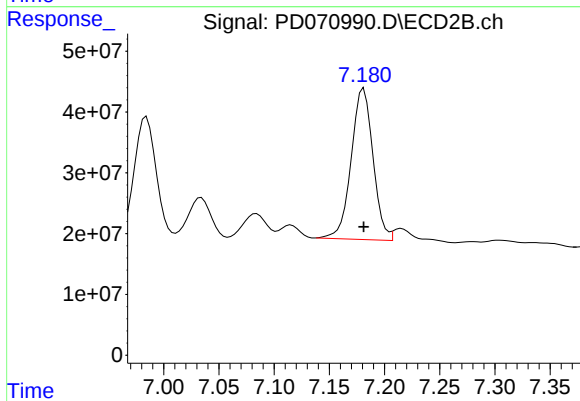

#27 Chlordane-5


R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 342433542
Conc: 733.81 ng/ml

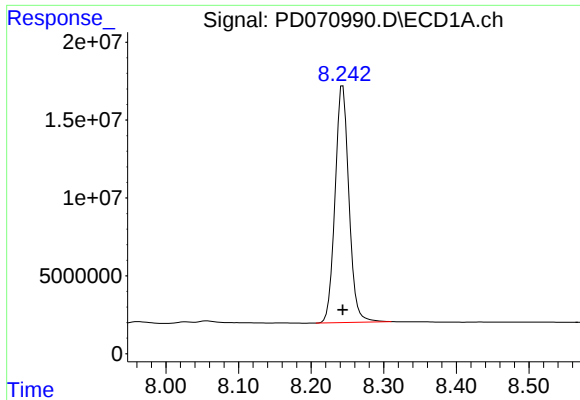

#28 Decachlorobiphenyl

R.T.: 8.244 min
Delta R.T.: 0.000 min
Response: 201622040
Conc: 73.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

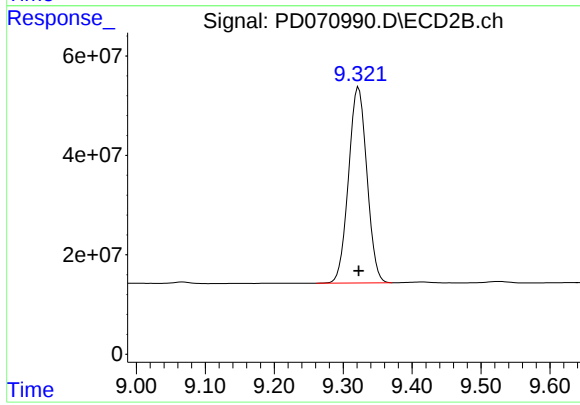

#28 Decachlorobiphenyl

R.T.: 9.322 min
Delta R.T.: 0.000 min
Response: 729099204
Conc: 73.51 ng/ml