

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
 Data File : PD070992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2022 21:57
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 04:20:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 04:20:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.125	78702819	689.5E6	24.473	26.554
28)	SA Decachlor...	8.243	9.321	71122727	269.6E6	25.709	26.598
Target Compounds							
23)	Chlordane-1	4.348	5.147	27380570	226.8E6	255.846	281.472
24)	Chlordane-2	4.850	5.625	32768932	157.7E6	271.336	276.598
25)	Chlordane-3	5.420	6.284	86882646	504.1E6	239.209	262.347
26)	Chlordane-4	5.478	6.357	72514081	585.8E6	243.101	263.655
27)	Chlordane-5	6.317	7.181	30291073	125.2E6	247.023	263.448



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
Data File : PD070992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2022 21:57
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 04:20:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 04:20:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

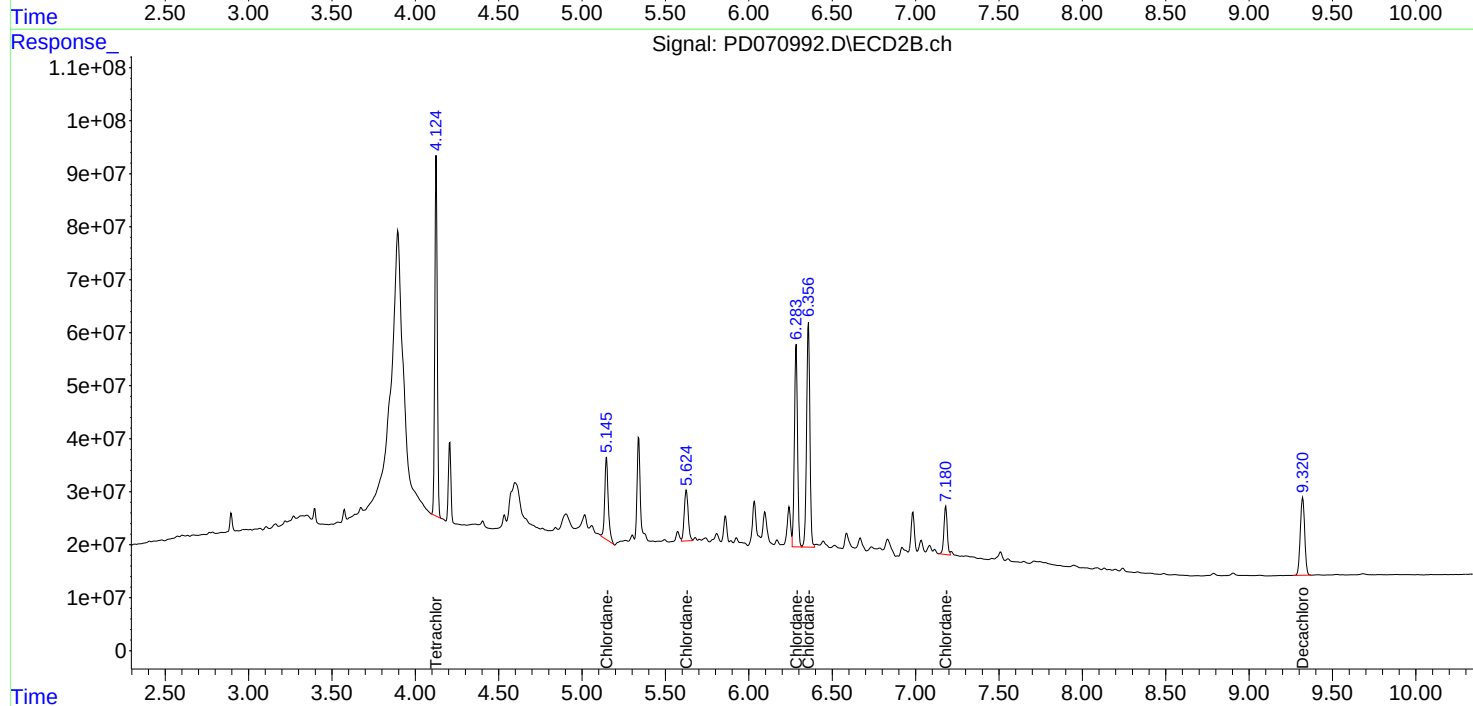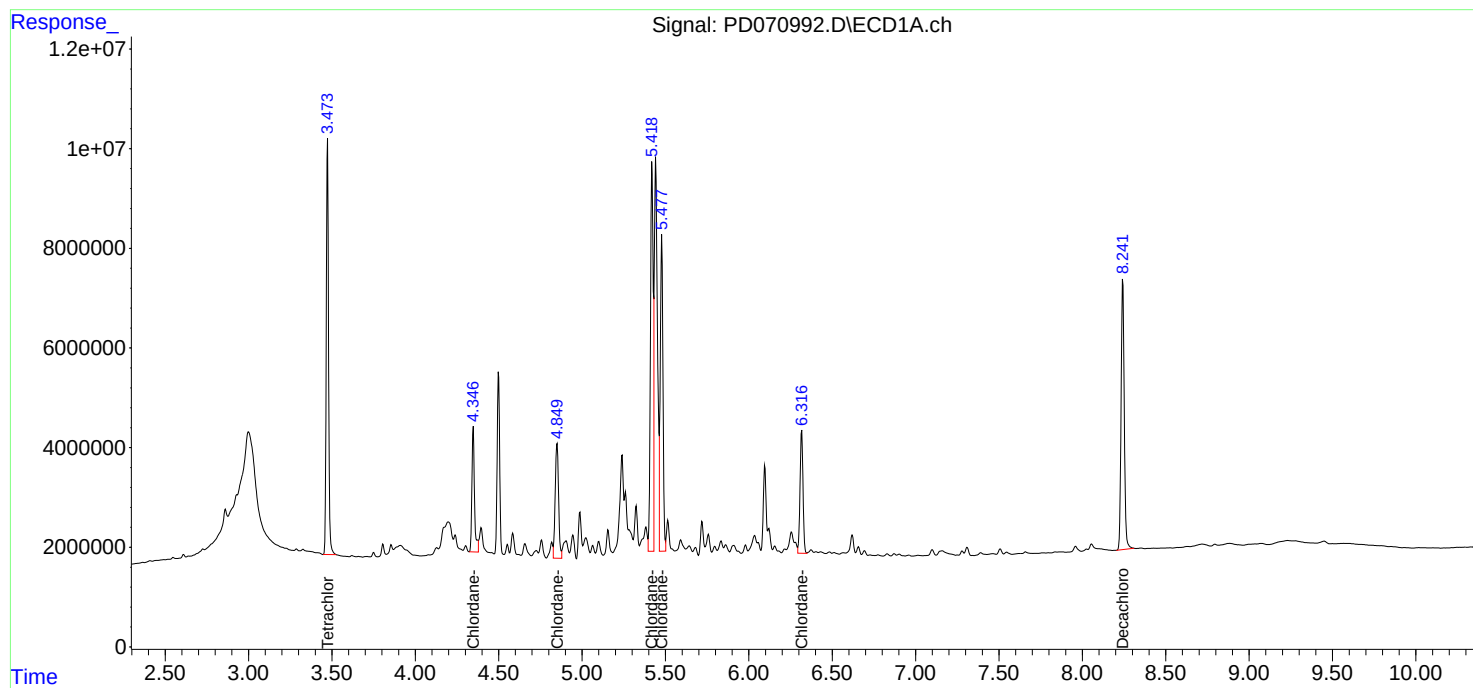


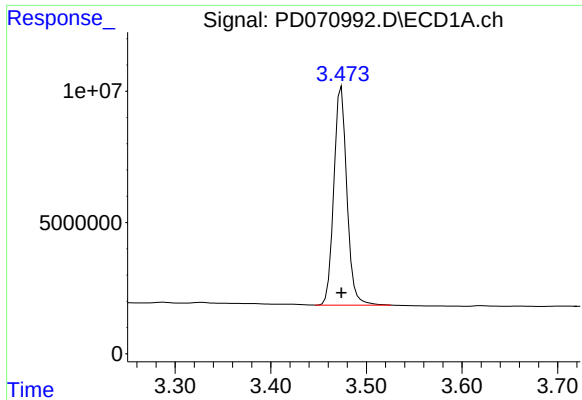

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 78702819
Conc: 24.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

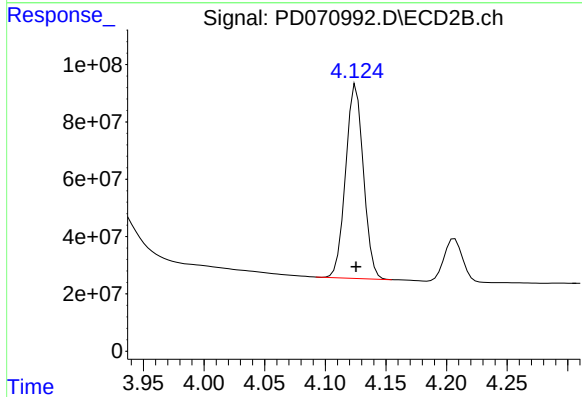


#1 Tetrachloro-m-xylene

R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 689531890
Conc: 26.55 ng/ml

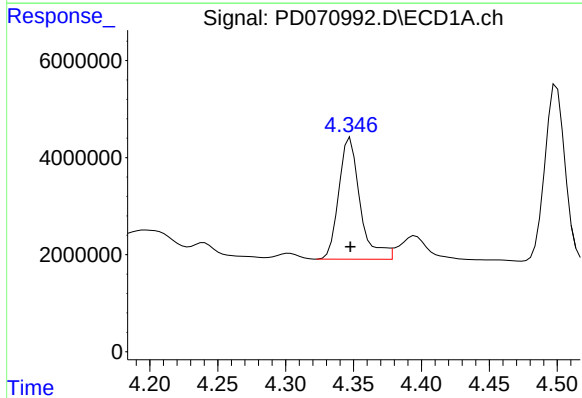


#23 Chlordane-1

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 27380570
Conc: 255.85 ng/ml

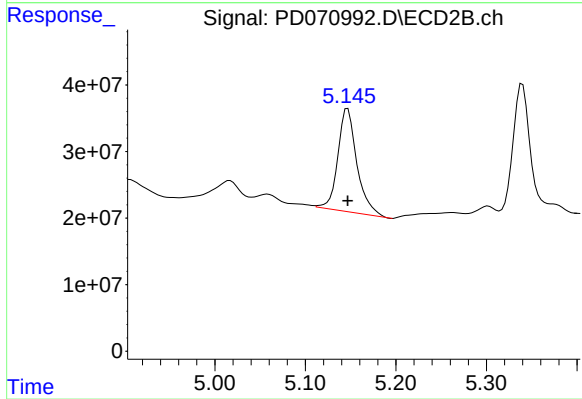

#23 Chlordane-1


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 226750296
Conc: 281.47 ng/ml

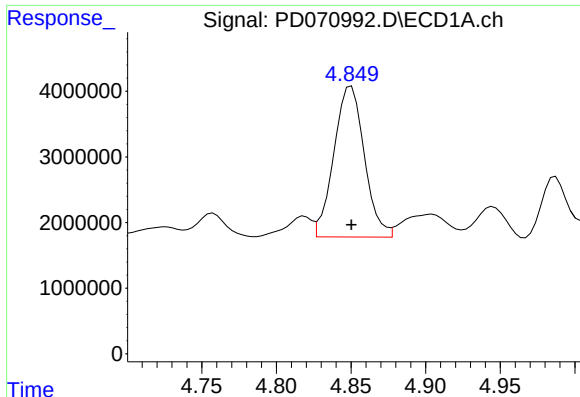

#24 Chlordane-2


R.T.: 4.850 min
Delta R.T.: 0.000 min
Response: 32768932
Conc: 271.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

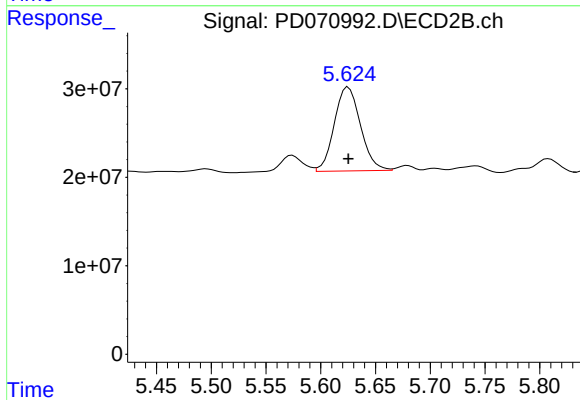


#24 Chlordane-2

R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 157723786
Conc: 276.60 ng/ml

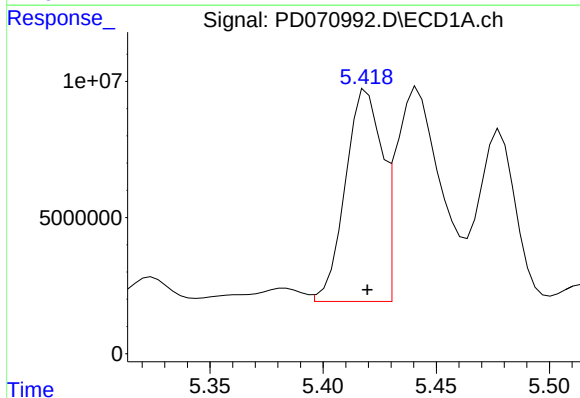


#25 Chlordane-3

R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 86882646
Conc: 239.21 ng/ml

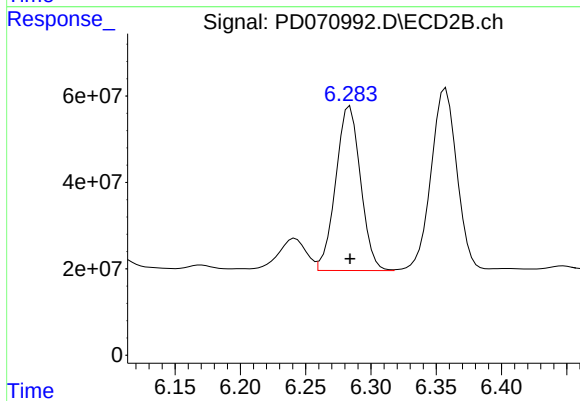

#25 Chlordane-3


R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 504114867
Conc: 262.35 ng/ml

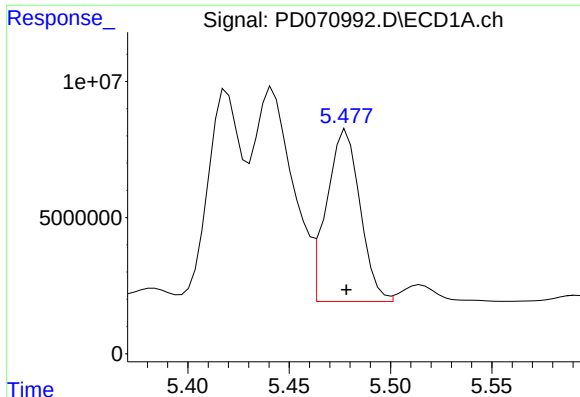

#26 Chlordane-4


R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 72514081
Conc: 243.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

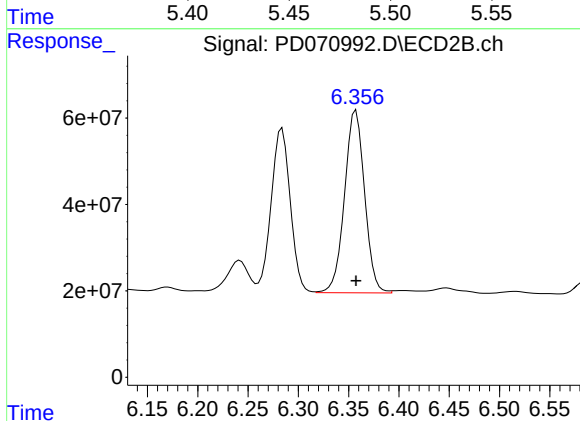


#26 Chlordane-4

R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 585834147
Conc: 263.66 ng/ml

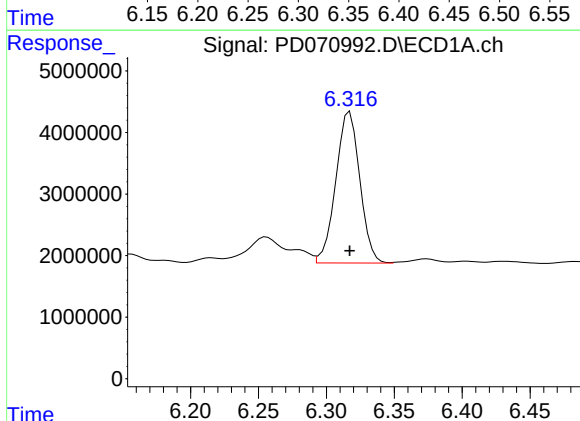


#27 Chlordane-5

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 30291073
Conc: 247.02 ng/ml

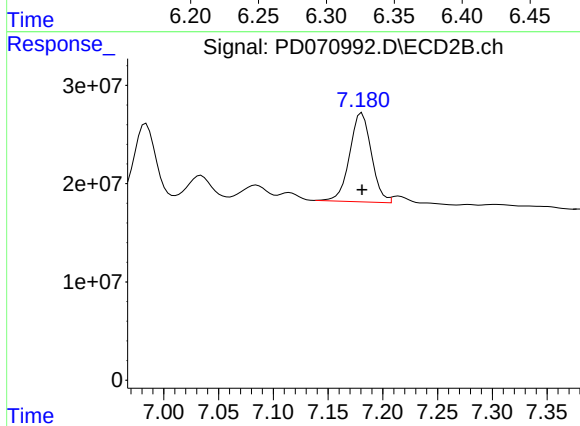

#27 Chlordane-5


R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 125183708
Conc: 263.45 ng/ml

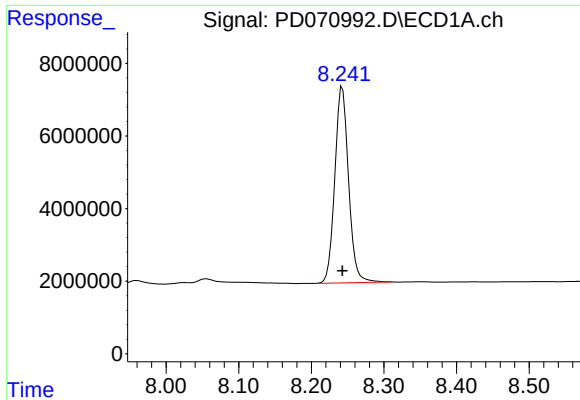

#28 Decachlorobiphenyl

R.T.: 8.243 min
Delta R.T.: 0.000 min
Response: 71122727
Conc: 25.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

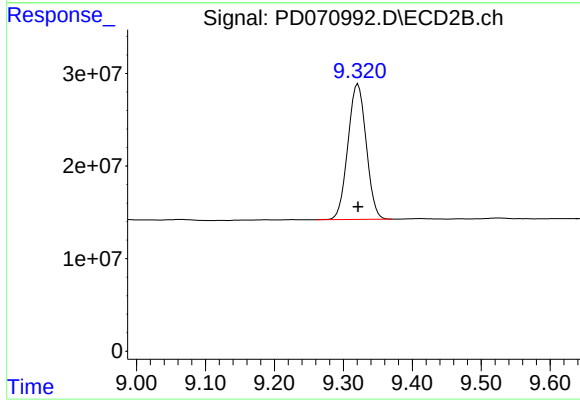

#28 Decachlorobiphenyl

R.T.: 9.321 min
Delta R.T.: 0.000 min
Response: 269569495
Conc: 26.60 ng/ml