

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
 Data File : PD071000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2022 23:54
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD071922CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 05:31:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 05:30:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.126	161.4E6	1304.9E6	55.712	45.132
28)	SA Decachlor...	8.243	9.321	142.0E6	523.5E6	46.491	45.899
Target Compounds							
23)	Chlordane-1	4.348	5.147	53325928	412.5E6	494.404	505.366
24)	Chlordane-2	4.850	5.625	58988226	294.6E6	478.522	494.032
25)	Chlordane-3	5.420	6.284	179.8E6	976.1E6	504.974	494.288
26)	Chlordane-4	5.479	6.358	148.4E6	1129.8E6	503.097	492.567
27)	Chlordane-5	6.317	7.181	62200699	243.5E6	507.990	498.349



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
Data File : PD071000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2022 23:54
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD071922CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 05:31:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 05:30:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

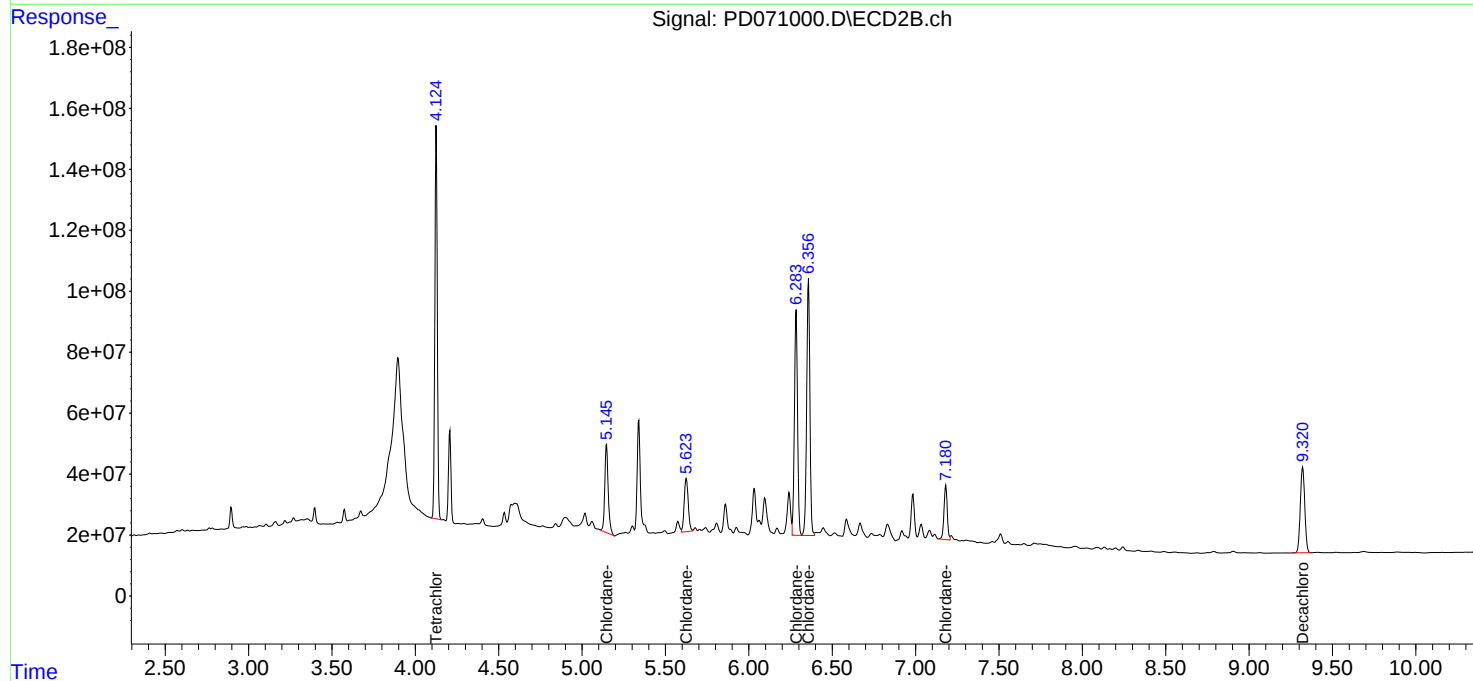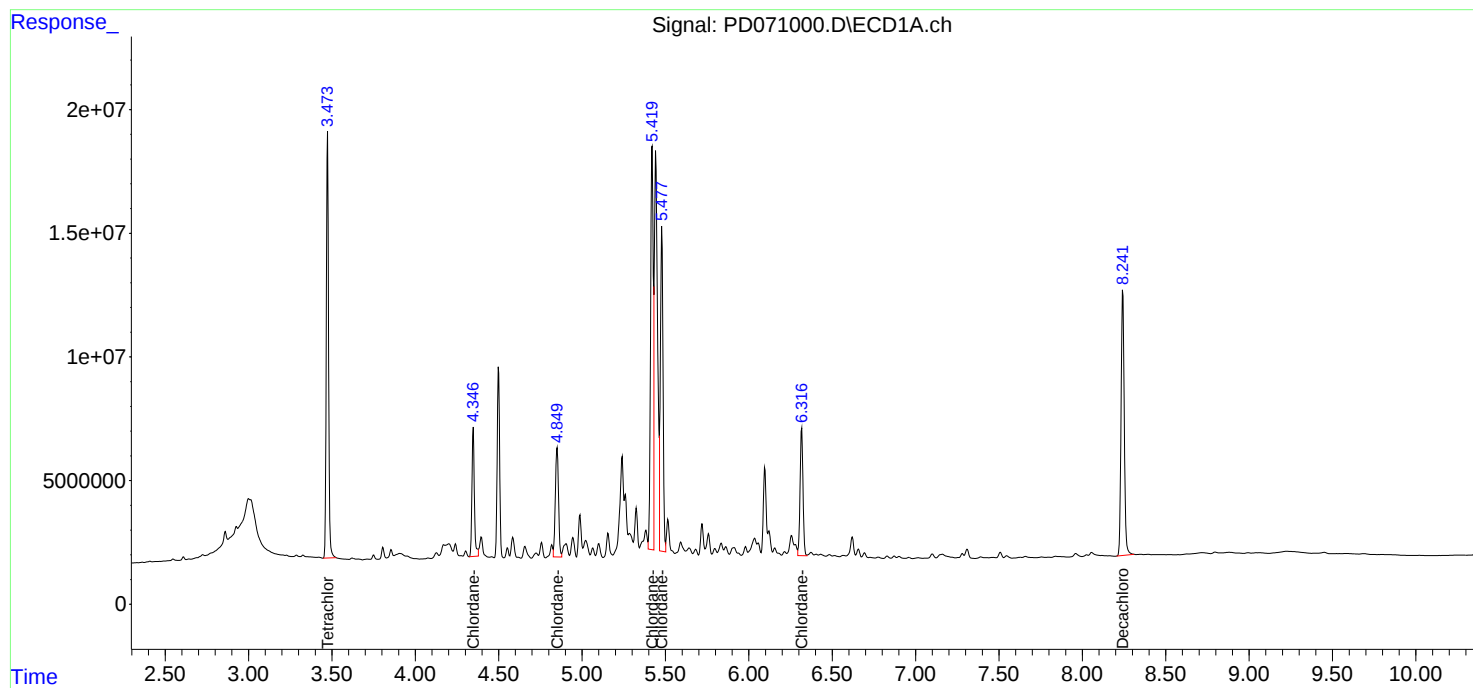


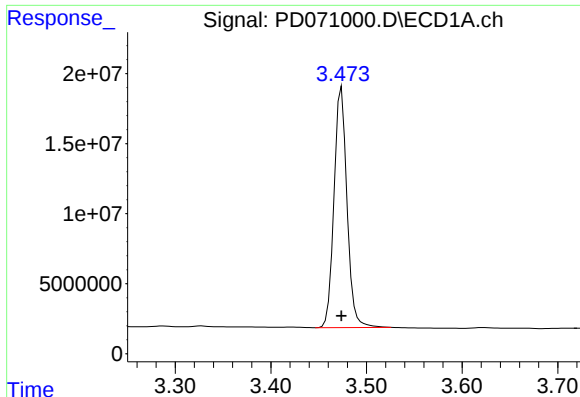

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 161447903
Conc: 55.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071922CHLOR

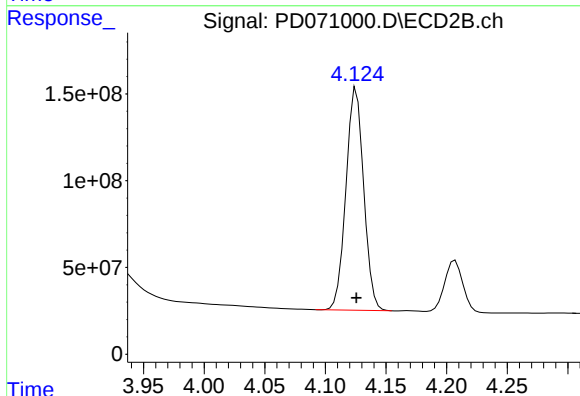


#1 Tetrachloro-m-xylene

R.T.: 4.126 min
Delta R.T.: 0.000 min
Response: 1304860444
Conc: 45.13 ng/ml

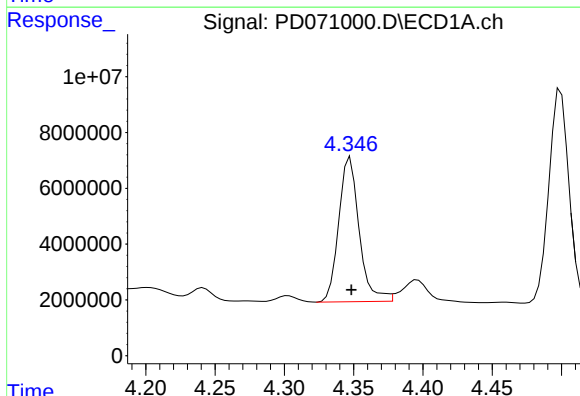


#23 Chlordane-1

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 53325928
Conc: 494.40 ng/ml

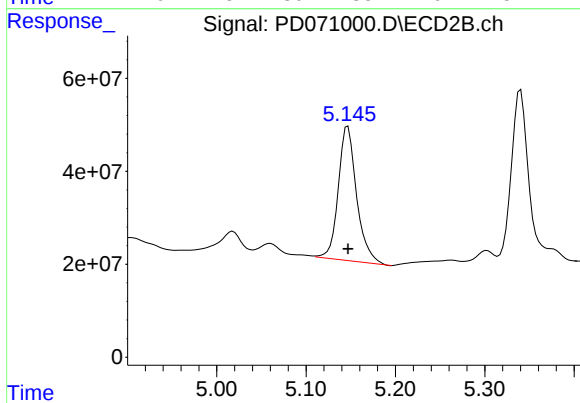

#23 Chlordane-1


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 412487796
Conc: 505.37 ng/ml

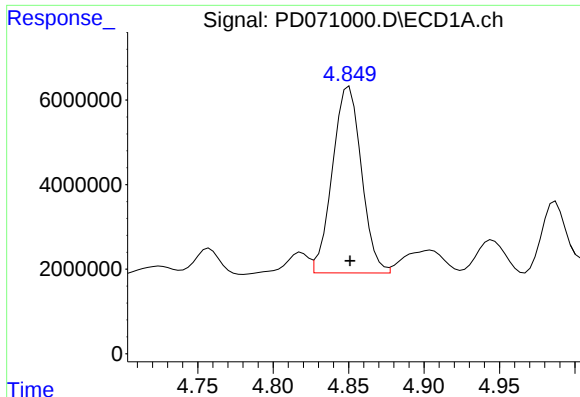

#24 Chlordane-2


R.T.: 4.850 min
Delta R.T.: 0.000 min
Response: 58988226
Conc: 478.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071922CHLOR

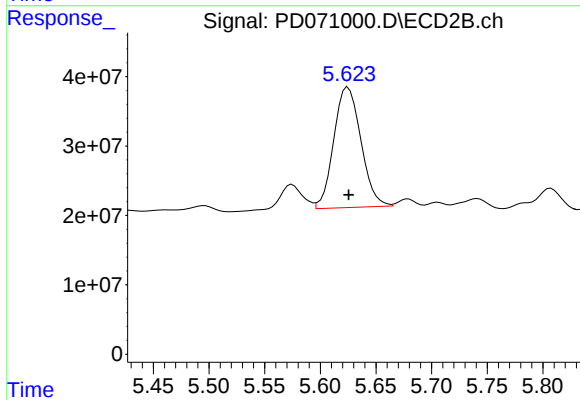


#24 Chlordane-2

R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 294629670
Conc: 494.03 ng/ml

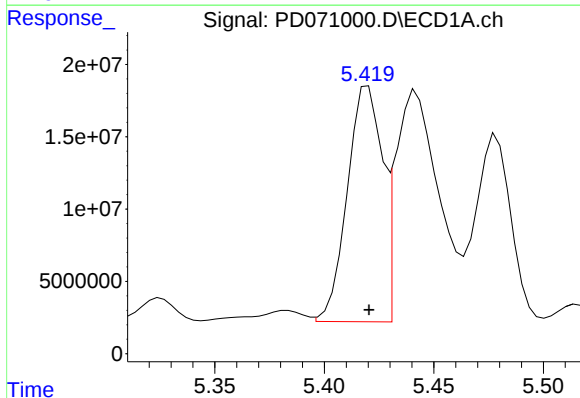


#25 Chlordane-3

R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 179846608
Conc: 504.97 ng/ml

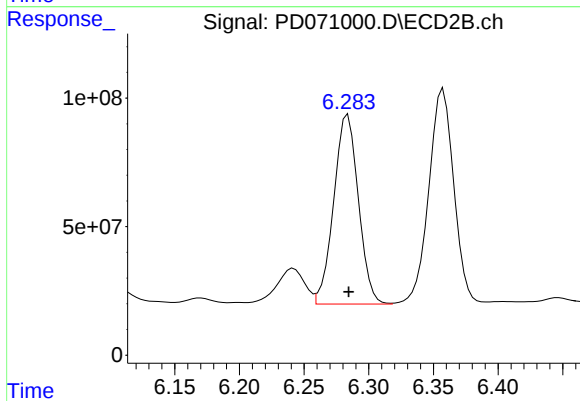

#25 Chlordane-3


R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 976130324
Conc: 494.29 ng/ml

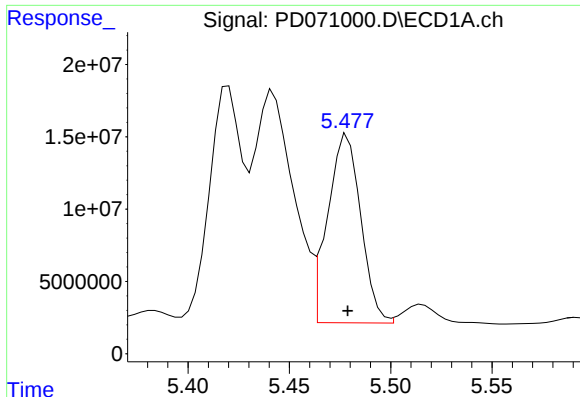

#26 Chlordane-4


R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 148373915
Conc: 503.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071922CHLOR

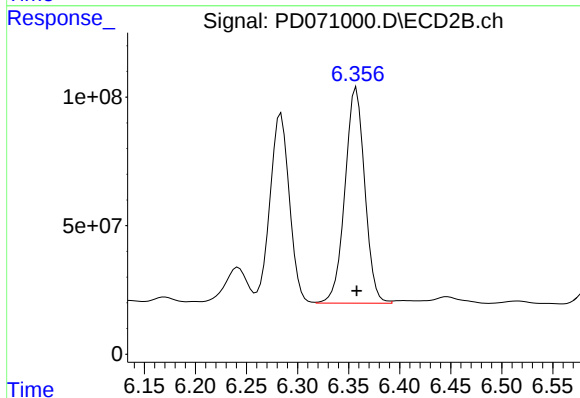


#26 Chlordane-4

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 1129822954
Conc: 492.57 ng/ml

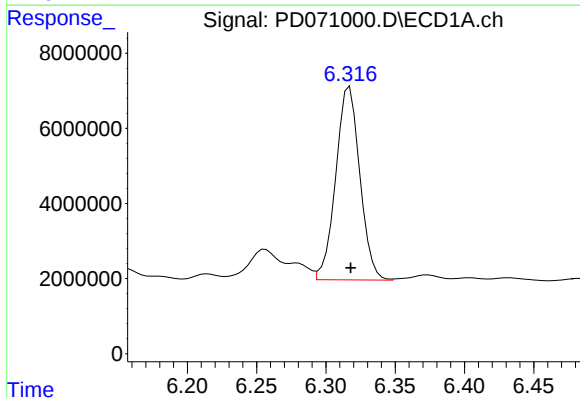


#27 Chlordane-5

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 62200699
Conc: 507.99 ng/ml

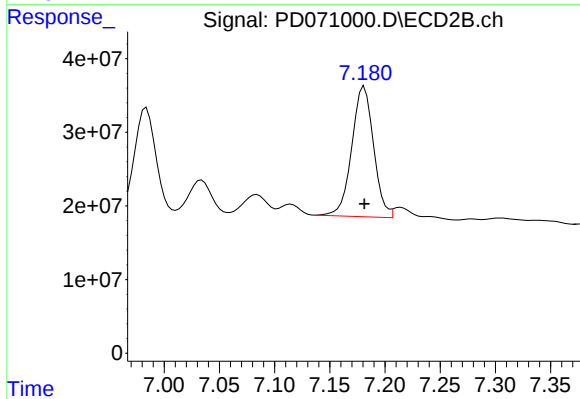

#27 Chlordane-5


R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 243500030
Conc: 498.35 ng/ml

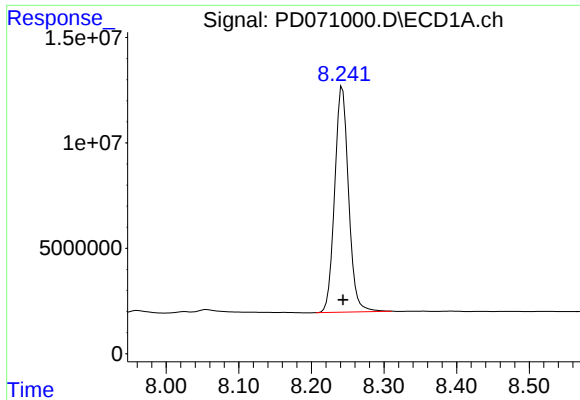

#28 Decachlorobiphenyl

R.T.: 8.243 min
Delta R.T.: 0.000 min
Response: 142045222
Conc: 46.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD071922CHLOR

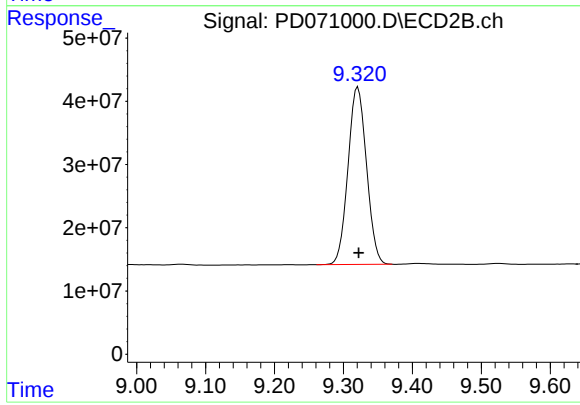

#28 Decachlorobiphenyl

R.T.: 9.321 min
Delta R.T.: -0.001 min
Response: 523478119
Conc: 45.90 ng/ml