

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
 Data File : PD071016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2022 04:15
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 06:37:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 05:30:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.126	164.1E6	1332.1E6	56.612	46.072
28)	SA Decachlor...	8.243	9.321	144.2E6	529.4E6	47.201	46.422
Target Compounds							
23)	Chlordane-1	4.347	5.147	54296607	413.6E6	503.404	506.769
24)	Chlordane-2	4.850	5.625	62338589	302.0E6	505.701	506.389
25)	Chlordane-3	5.419	6.284	181.0E6	996.9E6	508.338	504.819
26)	Chlordane-4	5.478	6.358	151.8E6	1150.3E6	514.720	501.506
27)	Chlordane-5	6.318	7.181	62704075	248.3E6	512.101	508.259



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
Data File : PD071016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2022 04:15
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 06:37:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 05:30:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

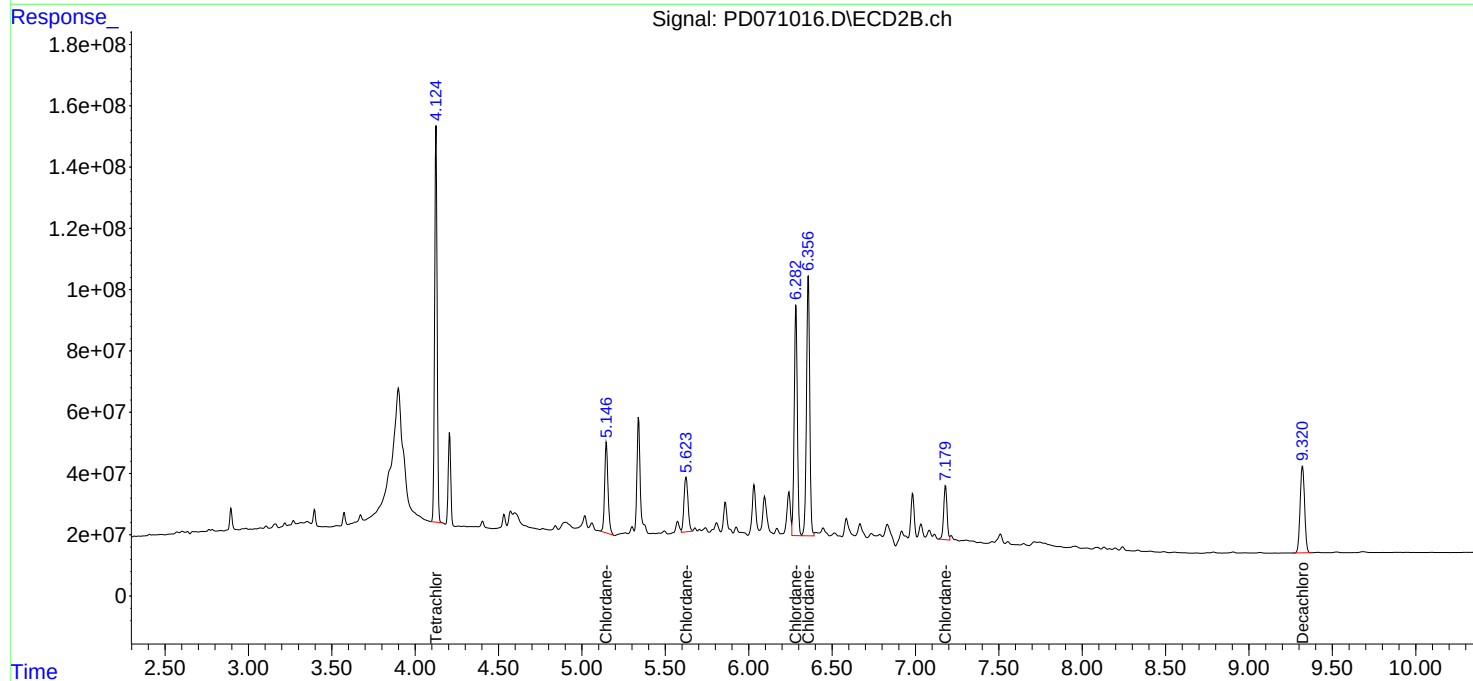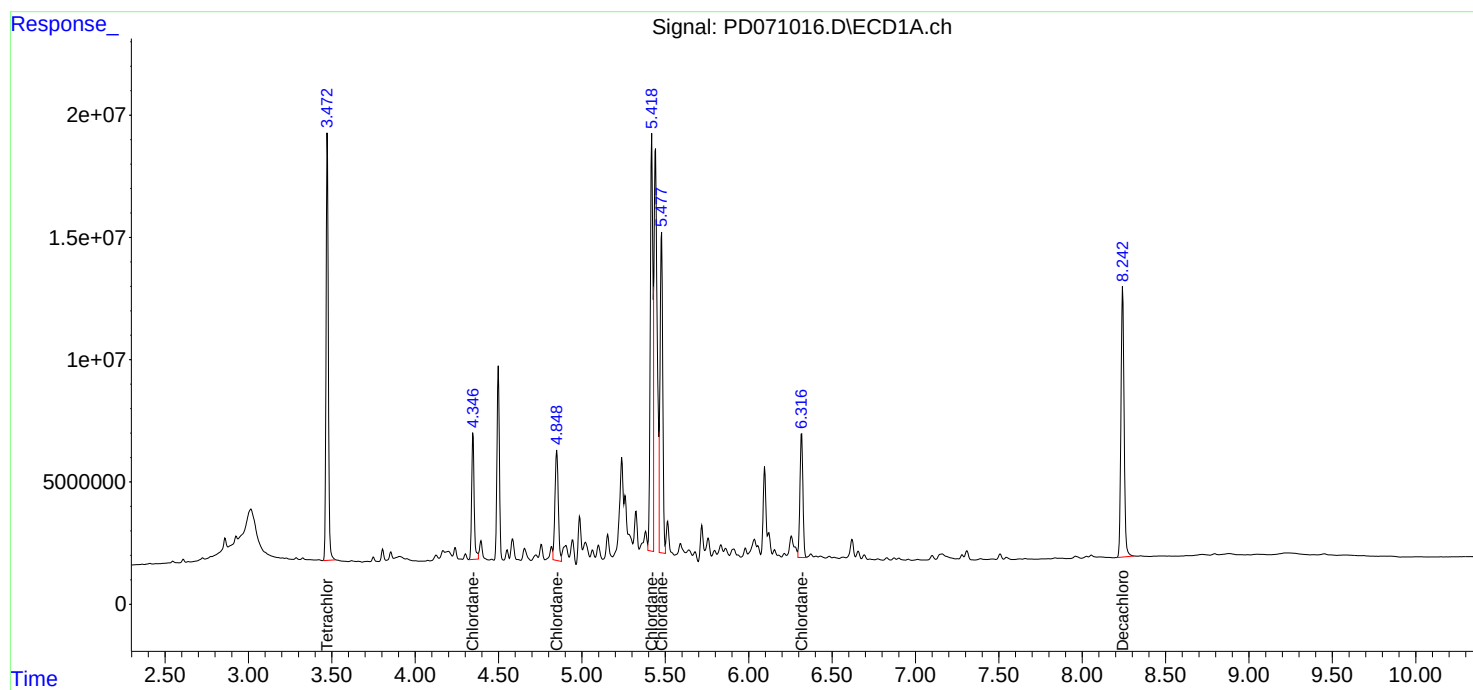


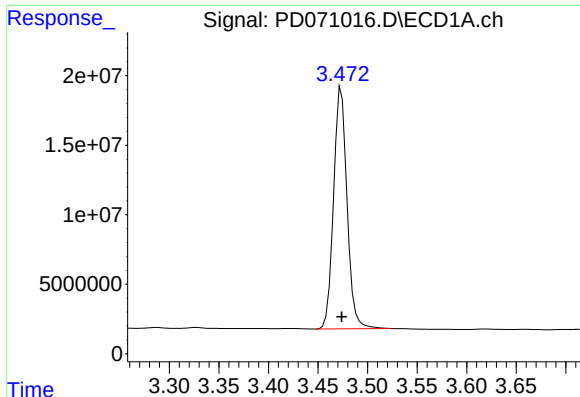

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 164054683
Conc: 56.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

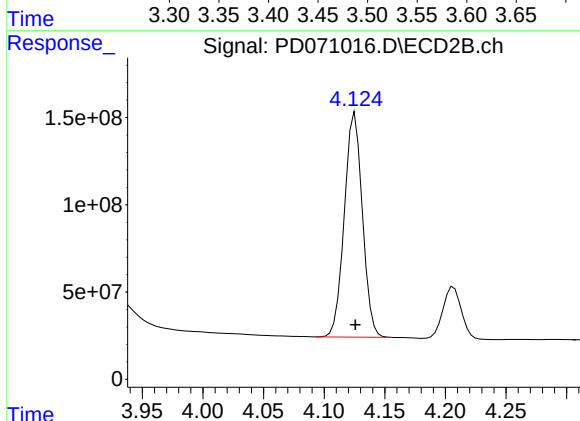


#1 Tetrachloro-m-xylene

R.T.: 4.126 min
Delta R.T.: 0.000 min
Response: 1332057814
Conc: 46.07 ng/ml

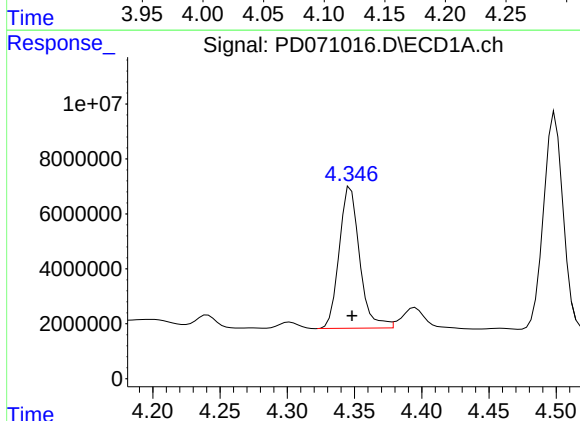


#23 Chlordane-1

R.T.: 4.347 min
Delta R.T.: -0.001 min
Response: 54296607
Conc: 503.40 ng/ml

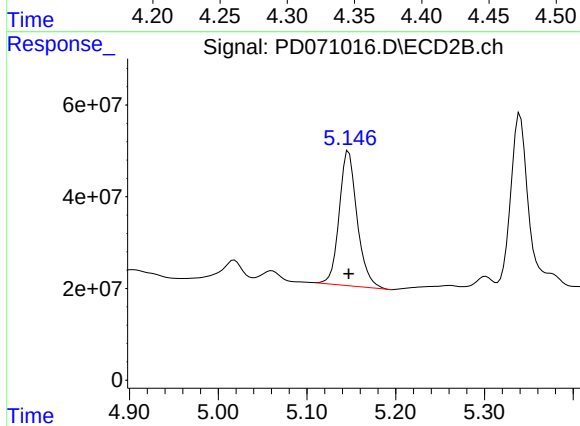

#23 Chlordane-1


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 413632941
Conc: 506.77 ng/ml

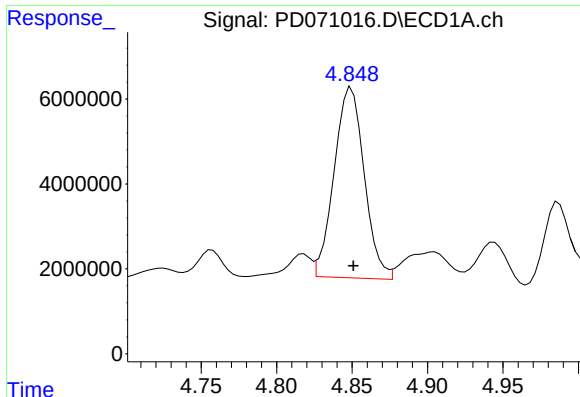

#24 Chlordane-2


R.T.: 4.850 min
Delta R.T.: -0.001 min
Response: 62338589
Conc: 505.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

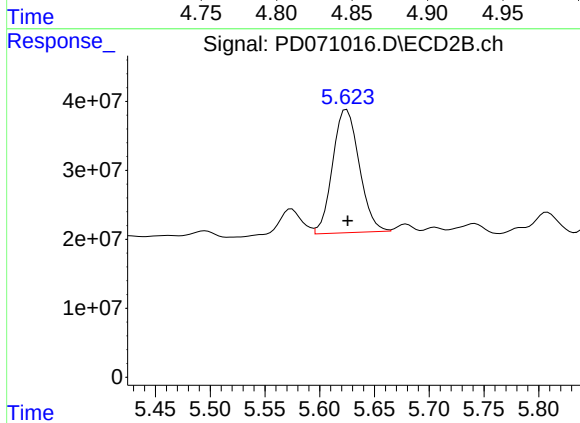


#24 Chlordane-2

R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 301999018
Conc: 506.39 ng/ml

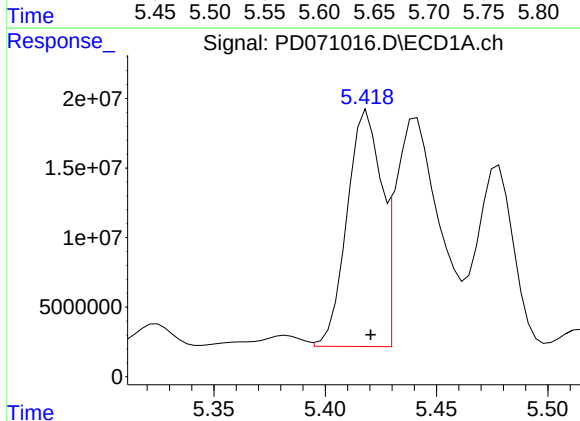


#25 Chlordane-3

R.T.: 5.419 min
Delta R.T.: -0.001 min
Response: 181044695
Conc: 508.34 ng/ml

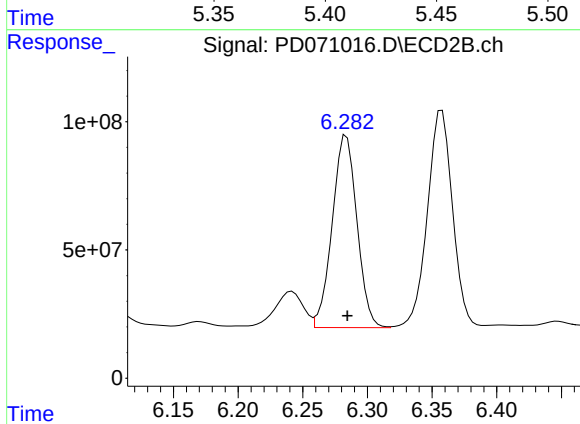

#25 Chlordane-3


R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 996926818
Conc: 504.82 ng/ml

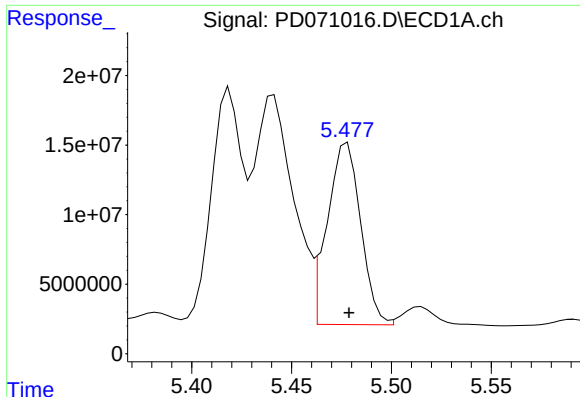

#26 Chlordane-4


R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 151801780
Conc: 514.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

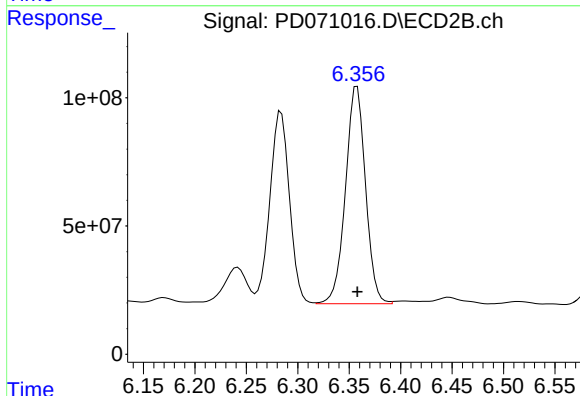


#26 Chlordane-4

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 1150325534
Conc: 501.51 ng/ml

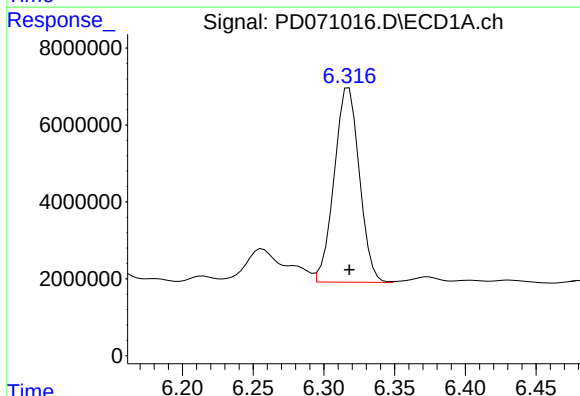


#27 Chlordane-5

R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 62704075
Conc: 512.10 ng/ml

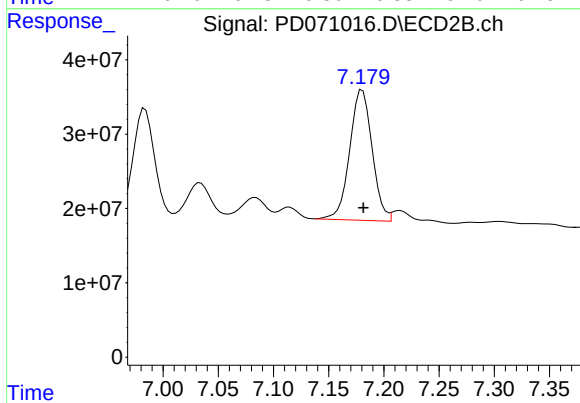

#27 Chlordane-5


R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 248342341
Conc: 508.26 ng/ml

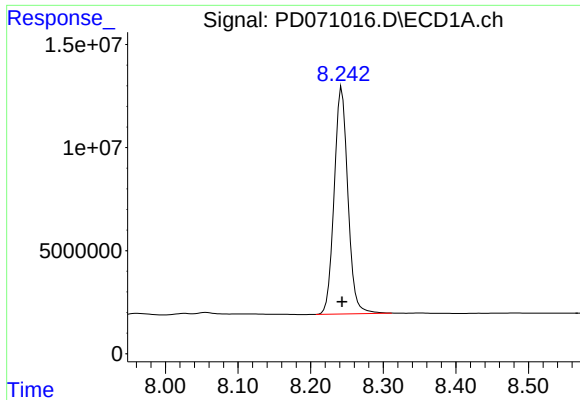

#28 Decachlorobiphenyl

R.T.: 8.243 min
Delta R.T.: 0.000 min
Response: 144212218
Conc: 47.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

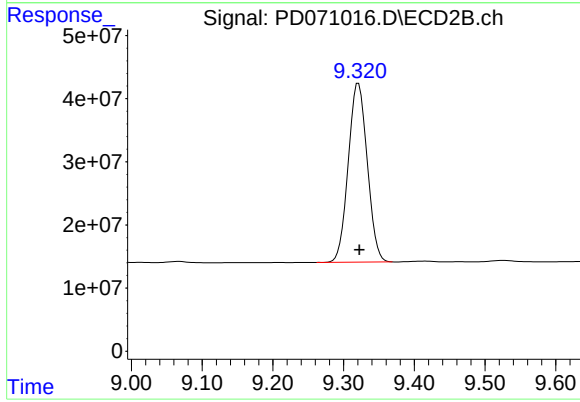

#28 Decachlorobiphenyl

R.T.: 9.321 min
Delta R.T.: -0.001 min
Response: 529442440
Conc: 46.42 ng/ml