

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
 Data File : PD071031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2022 08:36
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 09:06:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 05:30:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.125	167.3E6	1306.8E6	57.734	45.198
28)	SA Decachlor...	8.242	9.322	144.5E6	529.5E6	47.303	46.426
Target Compounds							
23)	Chlordane-1	4.348	5.146	54356398	408.3E6	503.958	500.278
24)	Chlordane-2	4.849	5.625	65589062	299.7E6	532.069	502.587
25)	Chlordane-3	5.420	6.284	180.6E6	987.6E6	507.114	500.118
26)	Chlordane-4	5.478	6.357	150.3E6	1142.3E6	509.534	498.002
27)	Chlordane-5	6.317	7.181	64248027	245.7E6	524.710	502.763



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071922\
Data File : PD071031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2022 08:36
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 09:06:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 05:30:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

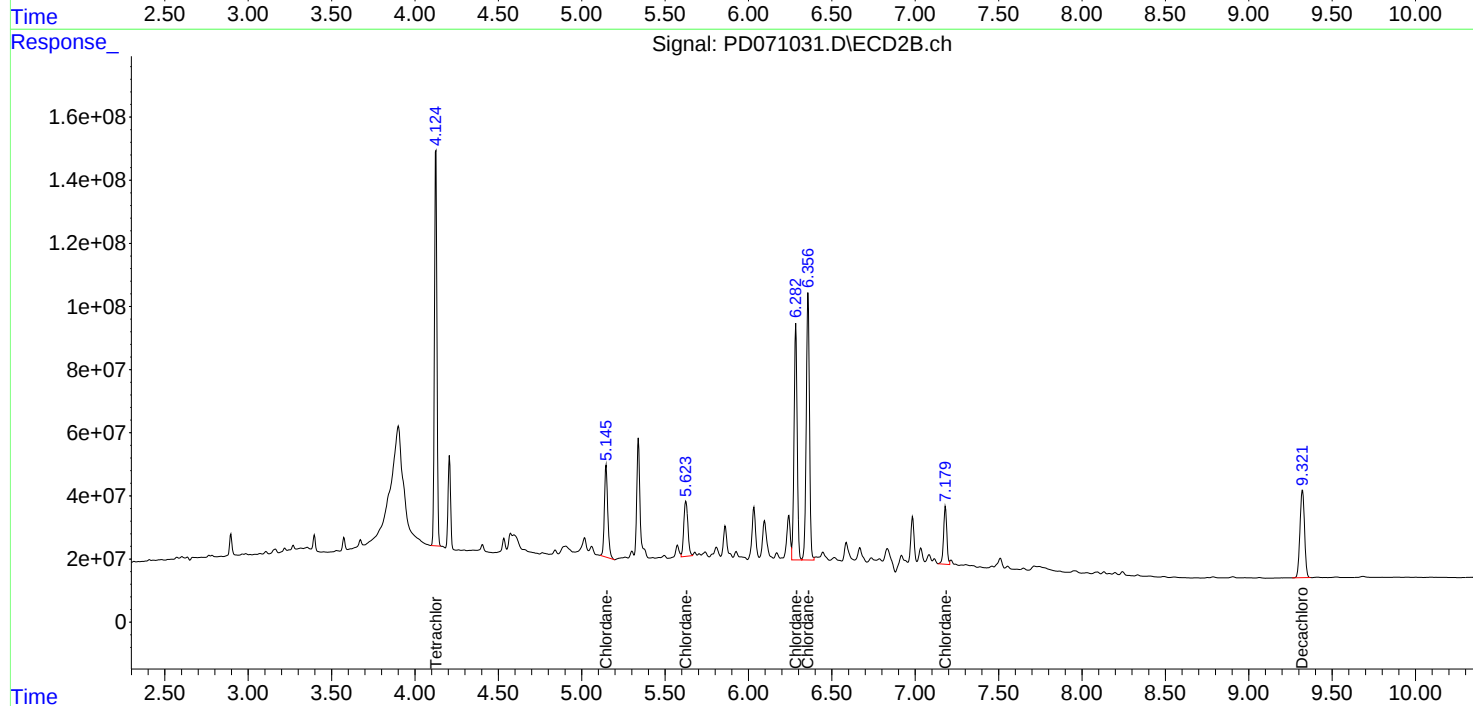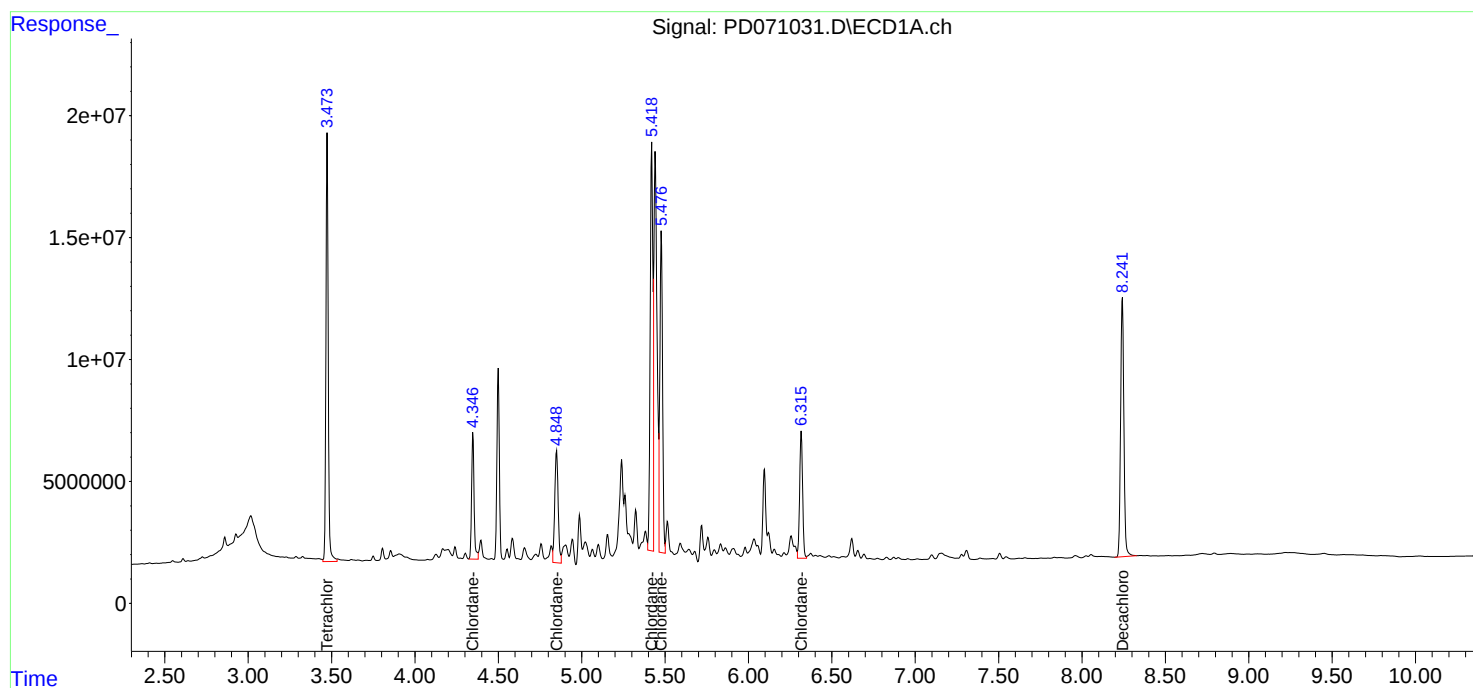


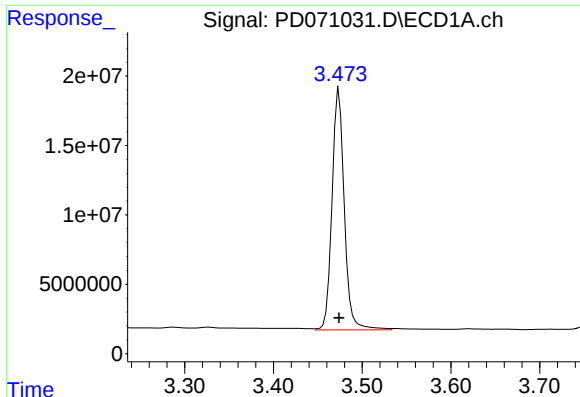

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 167307331
Conc: 57.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

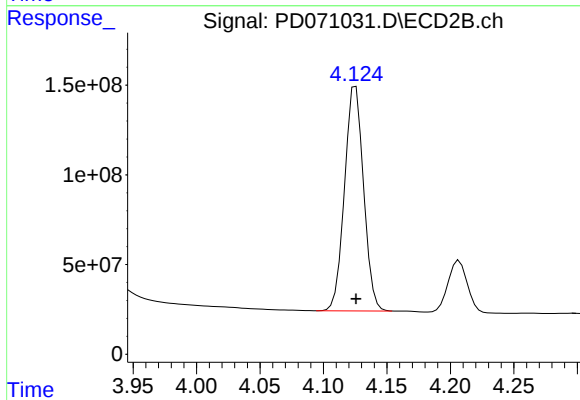


#1 Tetrachloro-m-xylene

R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 1306780081
Conc: 45.20 ng/ml

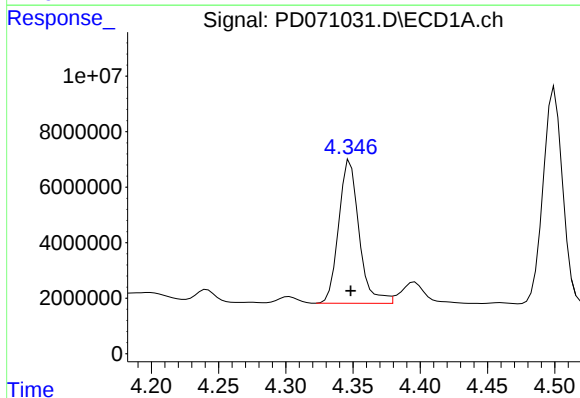


#23 Chlordane-1

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 54356398
Conc: 503.96 ng/ml

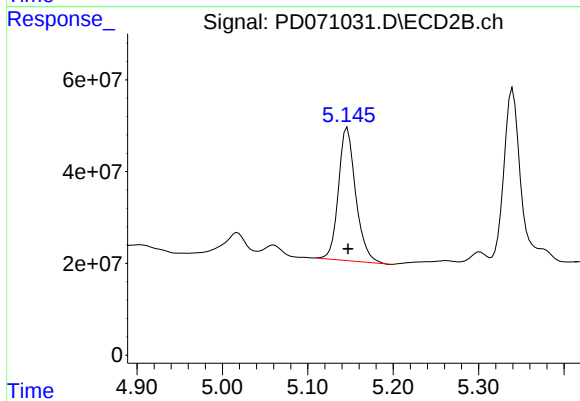

#23 Chlordane-1


R.T.: 5.146 min
Delta R.T.: 0.000 min
Response: 408335258
Conc: 500.28 ng/ml

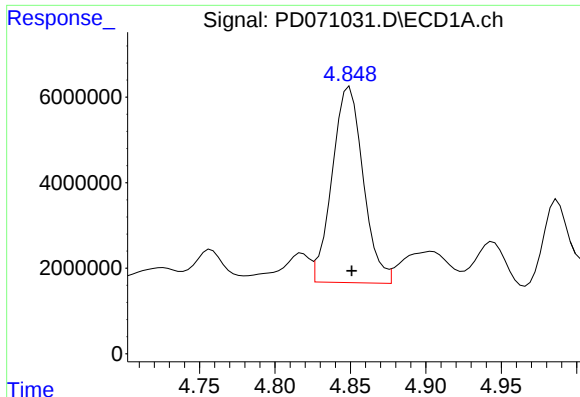

#24 Chlordane-2


R.T.: 4.849 min
Delta R.T.: -0.001 min
Response: 65589062
Conc: 532.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

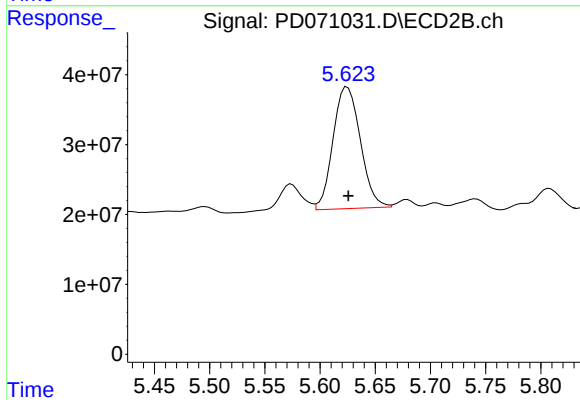


#24 Chlordane-2

R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 299731984
Conc: 502.59 ng/ml

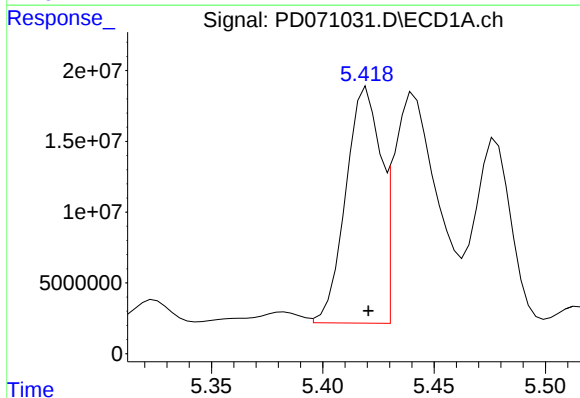


#25 Chlordane-3

R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 180608912
Conc: 507.11 ng/ml

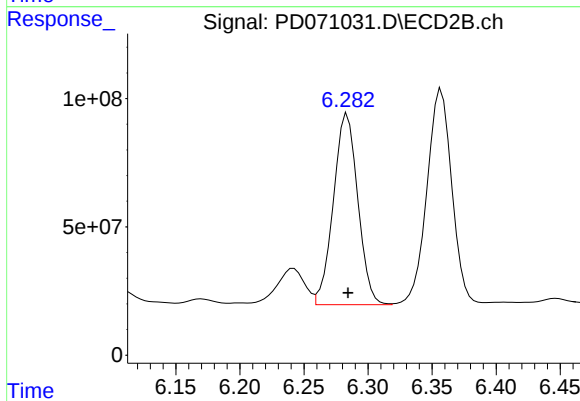

#25 Chlordane-3


R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 987642716
Conc: 500.12 ng/ml

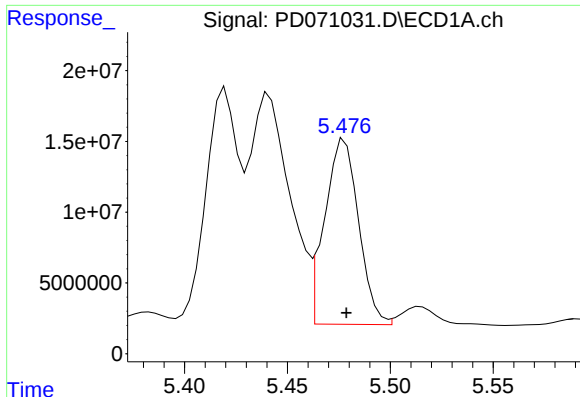

#26 Chlordane-4


R.T.: 5.478 min
Delta R.T.: 0.000 min
Response: 150272458
Conc: 509.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

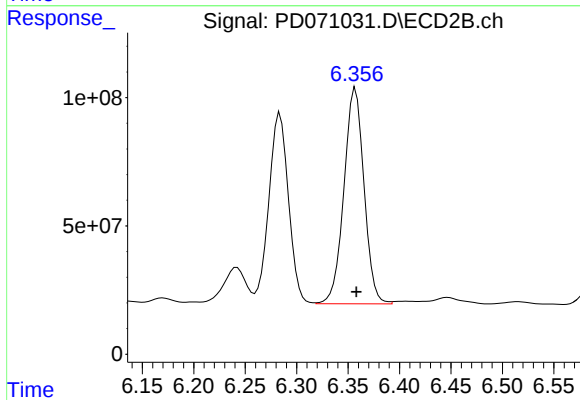


#26 Chlordane-4

R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 1142288541
Conc: 498.00 ng/ml

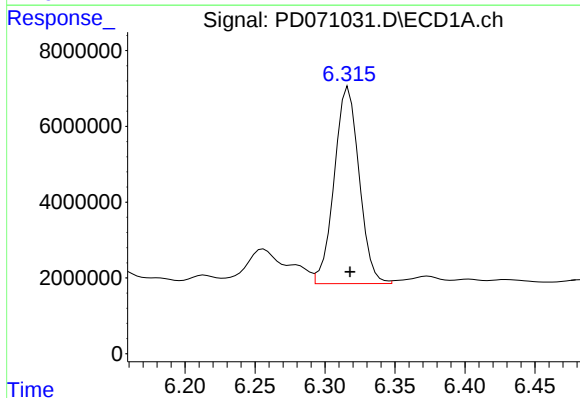


#27 Chlordane-5

R.T.: 6.317 min
Delta R.T.: -0.001 min
Response: 64248027
Conc: 524.71 ng/ml

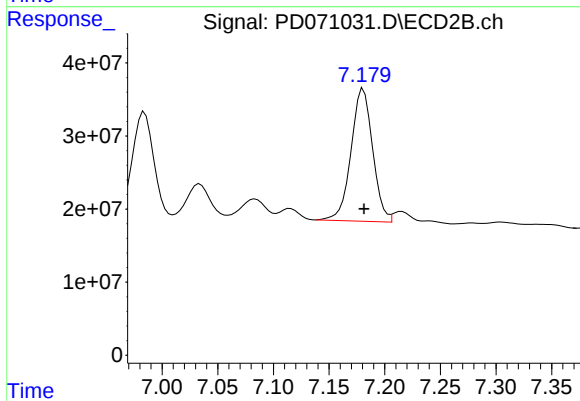

#27 Chlordane-5


R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 245657176
Conc: 502.76 ng/ml

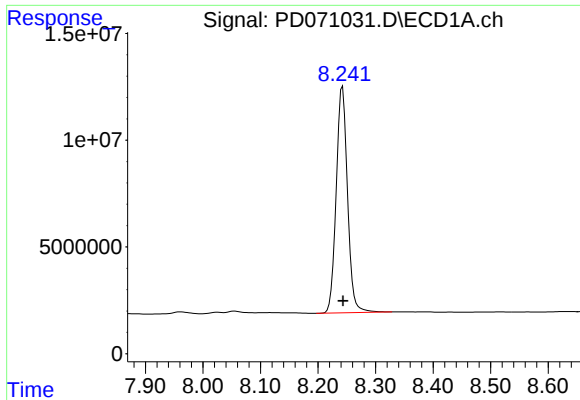

#28 Decachlorobiphenyl

R.T.: 8.242 min
Delta R.T.: -0.001 min
Response: 144526502
Conc: 47.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

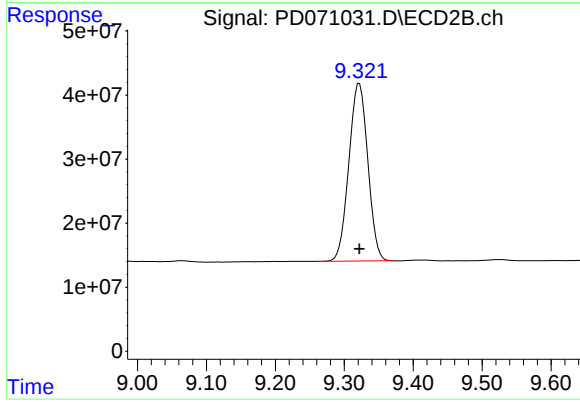

#28 Decachlorobiphenyl

R.T.: 9.322 min
Delta R.T.: 0.000 min
Response: 529484930
Conc: 46.43 ng/ml