

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071924\
 Data File : PD084016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2024 16:25
 Operator : AR\AJ
 Sample : PIBLK029
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 22:12:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.560	2.771	23545358	126.8E6	23.191	23.393
2) SA Decachlor...	9.113	7.896	47265662	138.2E6	22.183	20.684
Target Compounds						
7) B delta-BHC	4.788	0.000	1690639	0	0.798	N.D. #
8) B Heptachlo...	5.711	0.000	3975200	0	2.042	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071924\
Data File : PD084016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2024 16:25
Operator : AR\AJ
Sample : PIBLK029
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 22:12:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

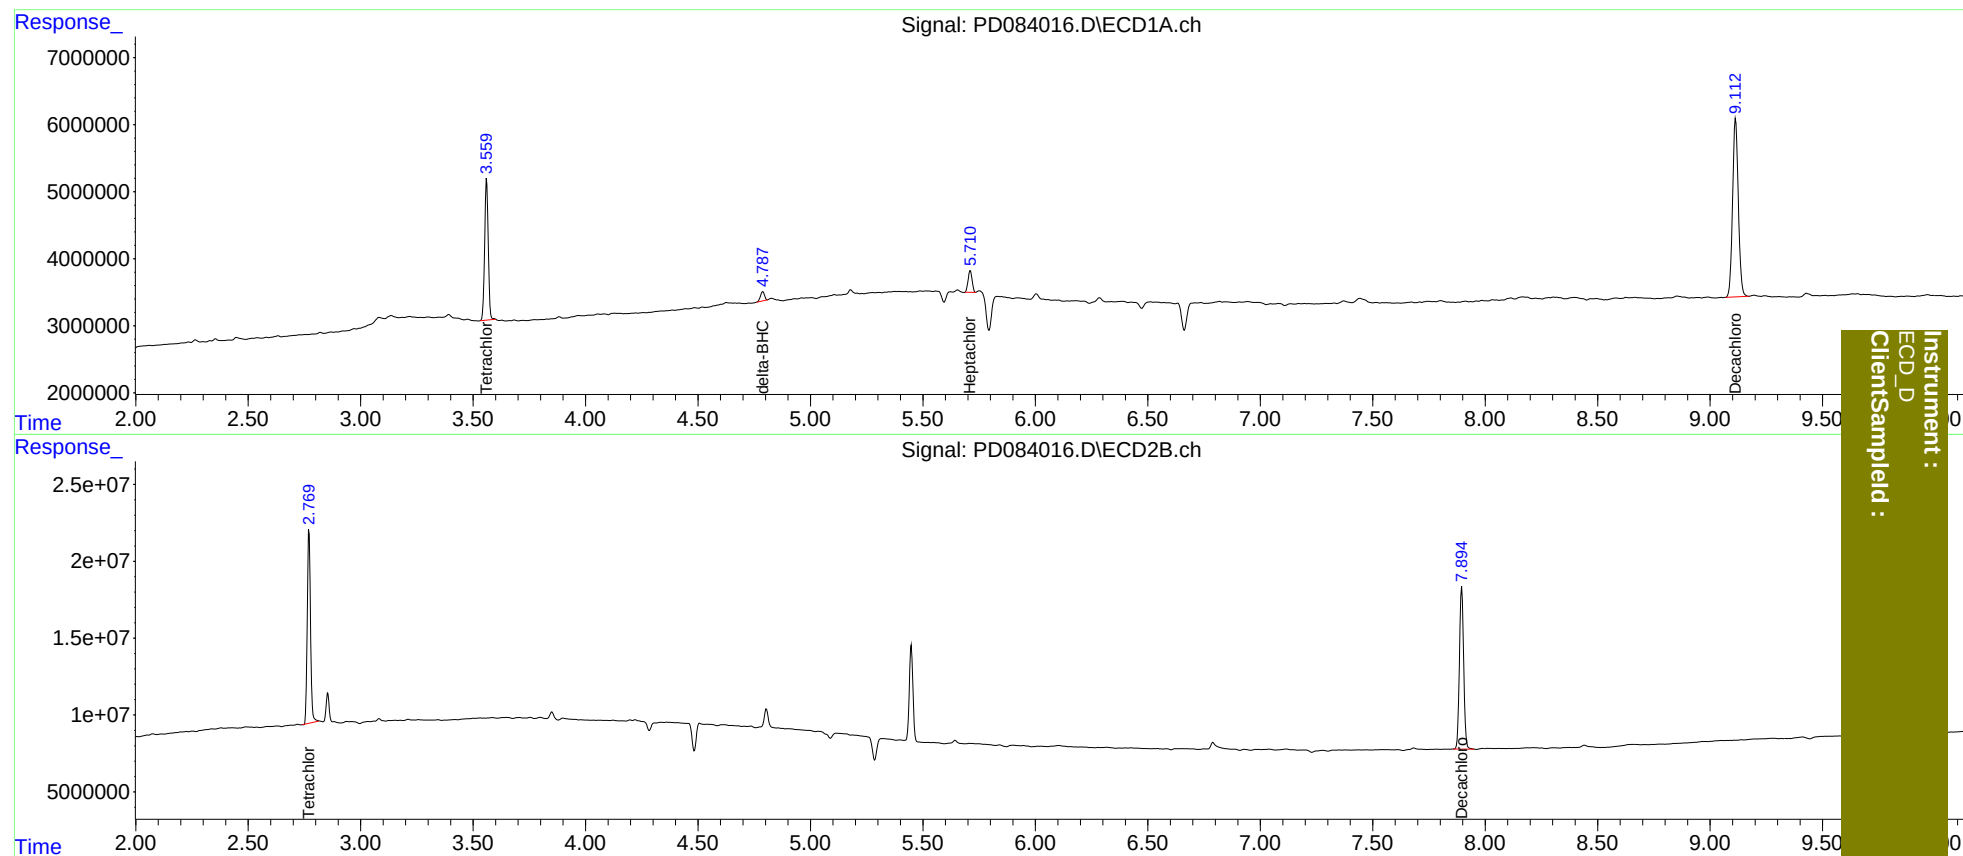


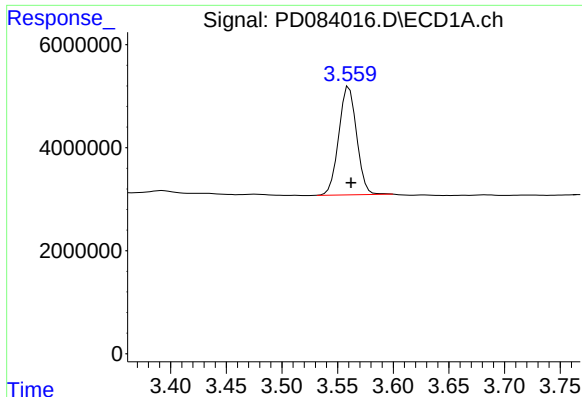

#1 Tetrachloro-m-xylene


R.T.: 3.560 min
Delta R.T.: -0.002 min
Response: 23545358
Conc: 23.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

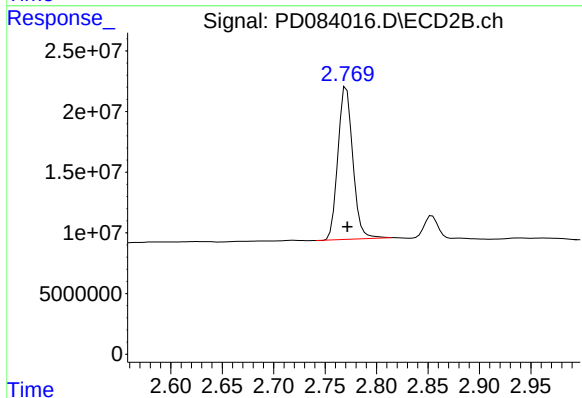


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 126780823
Conc: 23.39 ng/ml

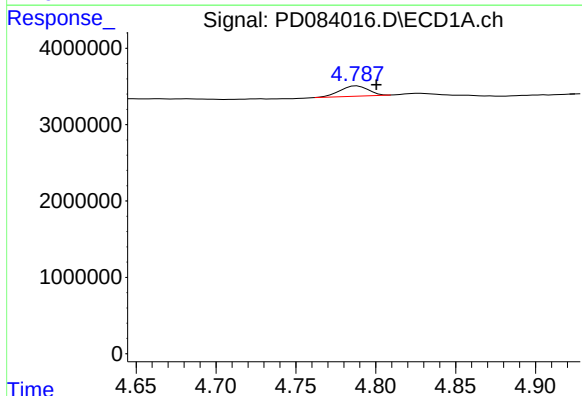


#7 delta-BHC

R.T.: 4.788 min
Delta R.T.: -0.012 min
Response: 1690639
Conc: 0.80 ng/ml

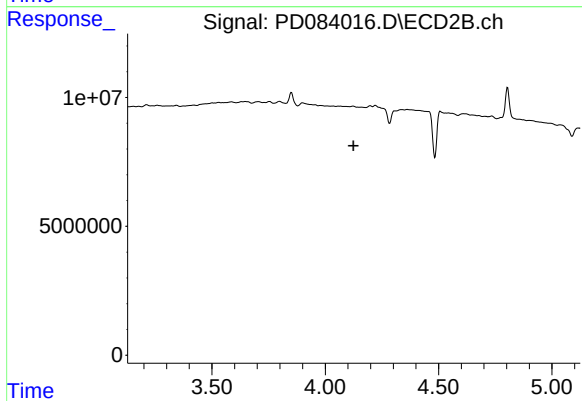

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.125 min
Response: 0
Conc: N.D.

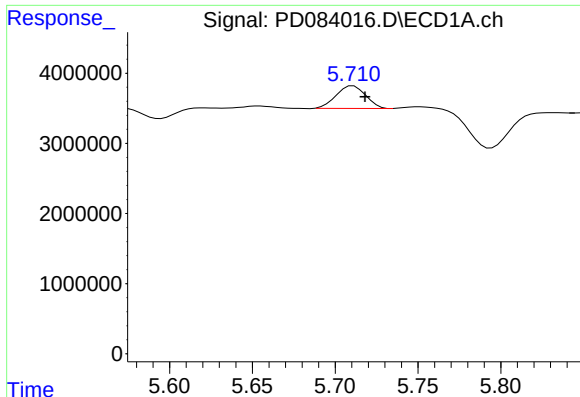

#8 Heptachlor epoxide


R.T.: 5.711 min
Delta R.T.: -0.007 min
Response: 3975200
Conc: 2.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

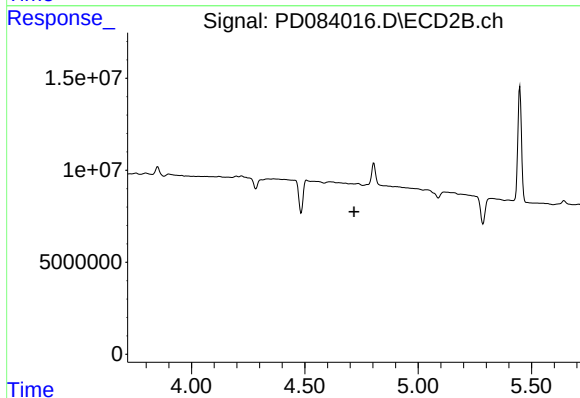


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.718 min
Response: 0
Conc: N.D.

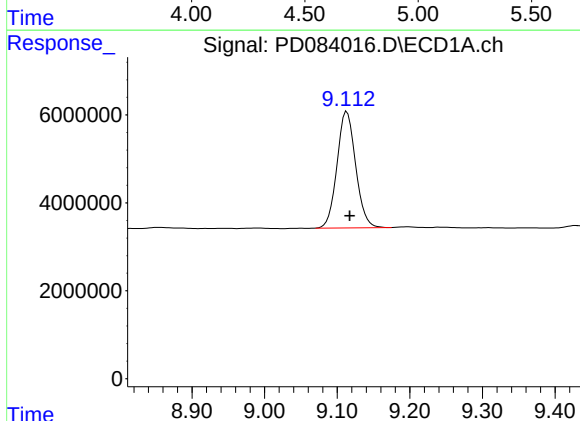

#27 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: -0.004 min
Response: 47265662
Conc: 22.18 ng/ml

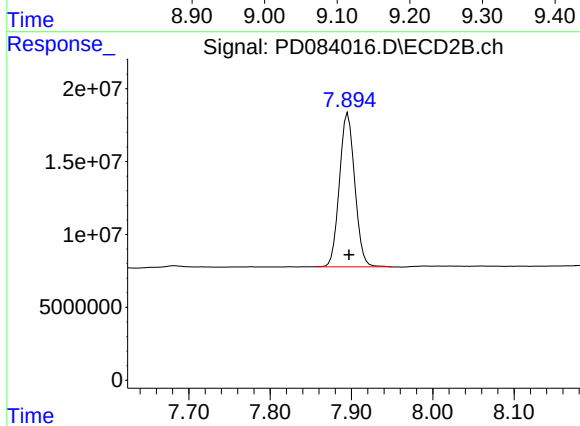

#27 Decachlorobiphenyl

R.T.: 7.896 min
Delta R.T.: -0.002 min
Response: 138185992
Conc: 20.68 ng/ml