

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071924\
 Data File : PD084008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jul 2024 11:43
 Operator : AR\AJ
 Sample : P3287-07DL2 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 XB506DL2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/22/2024
 Supervised By :Ankita Jodhani 07/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 22:10:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.560	2.770	1216622	5588144	1.198m	1.031m
2) SA Decachlor...	9.115	7.895	1974845	5606907	0.927	0.839m
Target Compounds						
2) A alpha-BHC	4.019	3.271	95592132	429.2E6	50.529	47.610
3) MA gamma-BHC...	4.353	3.599	76421486	336.2E6	41.409	39.277
4) MA Heptachlor	4.945	3.936	10288474	46815298	5.132	5.560
5) MB Aldrin	5.289	4.216	106.4E6	404.9E6	52.361	47.994
6) B beta-BHC	4.551	3.896	54012453	232.9E6	64.304	61.438
7) B delta-BHC	4.800	4.125	41747864	179.3E6	19.695	19.638
8) B Heptachlo...	5.715	4.717	26563503	101.1E6	13.644m	12.868
9) A Endosulfan I	6.103	5.086	69671402	244.0E6	37.617m	35.117
10) B trans-Chl...	5.973	4.966	73618172	267.6E6	38.665	34.634
11) B cis-Chlor...	6.052	5.030	69035118	249.9E6	35.268m	31.746
12) B 4,4'-DDE	6.225	5.218	87428331	303.0E6	44.138	40.474
13) MA Dieldrin	6.378	5.350	68967506	246.0E6	34.442m	31.769
14) MA Endrin	6.609	5.625	150.6E6	502.3E6	91.079m	75.846
15) B Endosulfa...	6.831	5.919	78867273	259.5E6	43.261	38.887
16) A 4,4'-DDD	6.743	5.772	33141256	128.3E6	22.971	21.540
17) MA 4,4'-DDT	7.059	6.022	21827100	74255660	14.434	12.701
18) B Endrin al...	6.961	6.097	107.3E6	349.9E6	78.483	69.758m
19) B Endosulfa...	7.195	6.319	60893743	201.7E6	34.359m	31.047m
20) A Methoxychlor	7.535	6.596	13809227	43448377	15.521	14.704
21) B Endrin ke...	7.682	6.826	172.2E6	548.9E6	88.211m	78.142

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071924\
Data File : PD084008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jul 2024 11:43
Operator : AR\AJ
Sample : P3287-07DL2 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 22:10:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

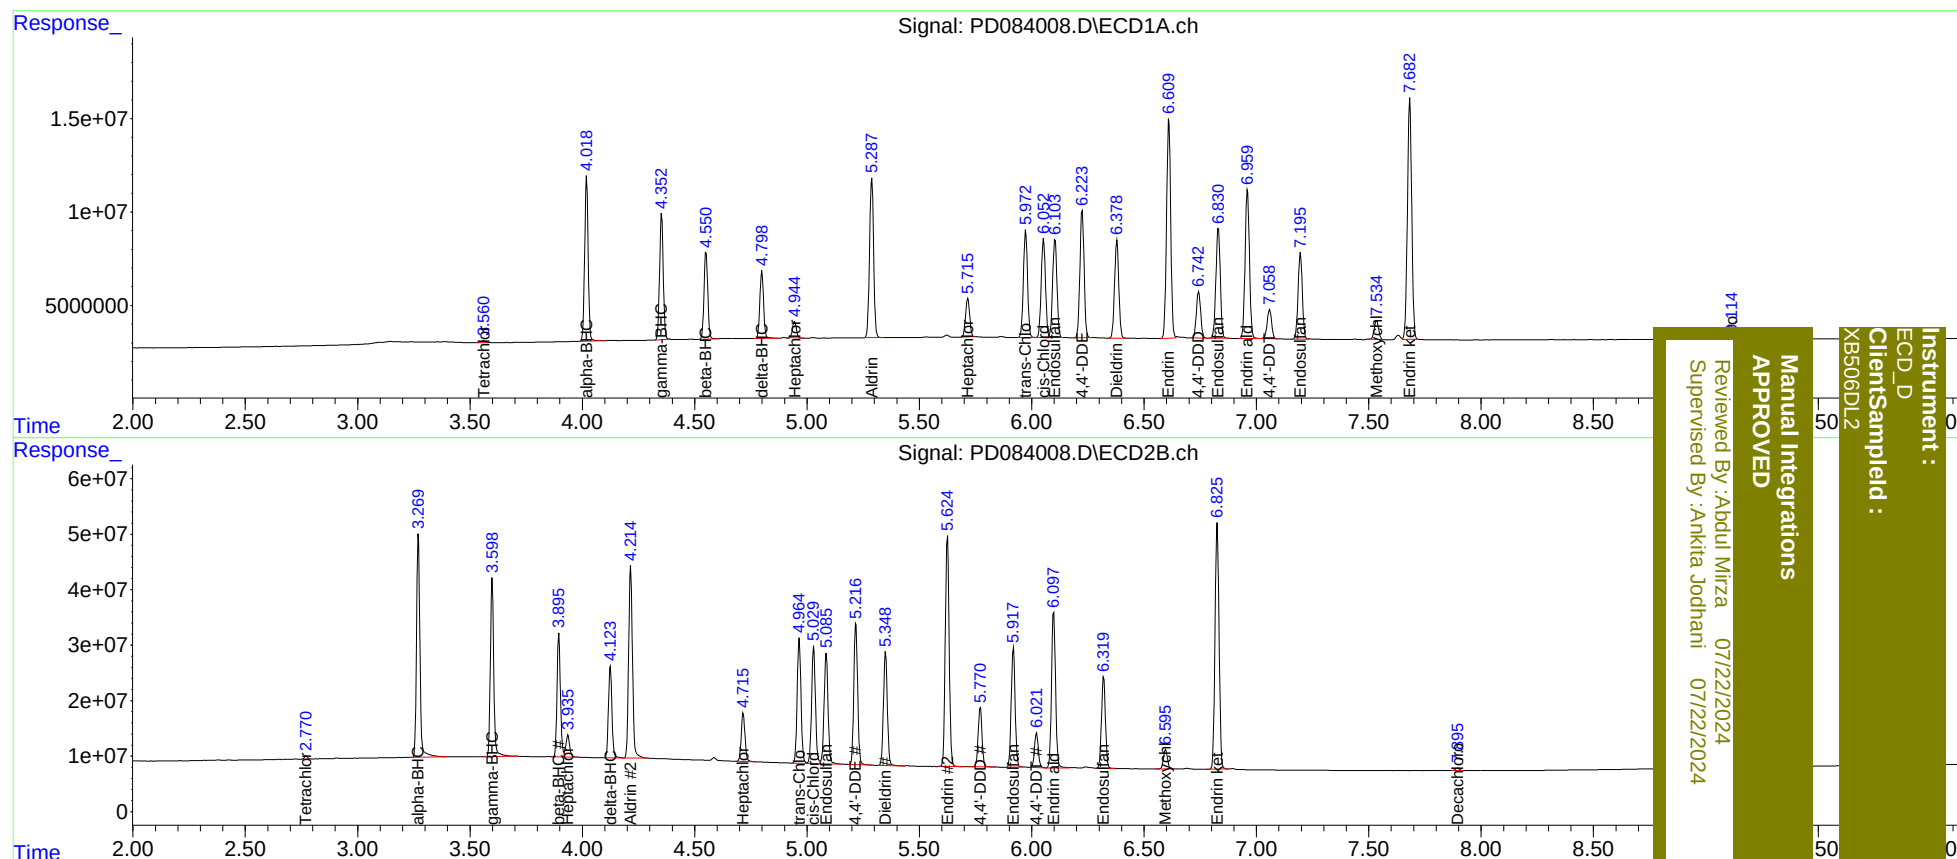

Instrument :
ECD_D
Client Sampled :
XB506DL2

Manual Integrations
APPROVED

Reviewed By: Aboul Mirza 07/22/2024
Supervised By: Ankita Jodhani 07/22/2024