

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072219\
 Data File : PD054062.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jul 2019 10:34
 Operator : SM\AJ
 Sample : K3591-07
 Misc : TOX LOD 50 PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:48:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX071919.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 03:25:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.313	3.983	12009729	18577608	19.463	19.725
7) SA Decachlor...	8.007	9.024	14389077	20058532	21.090	21.064

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072219\
Data File : PD054062.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2019 10:34
Operator : SM\AJ
Sample : K3591-07
Misc : TOX LOD 50 PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
LOD-MDL-WATER-01-QT3-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 01:48:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 03:25:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

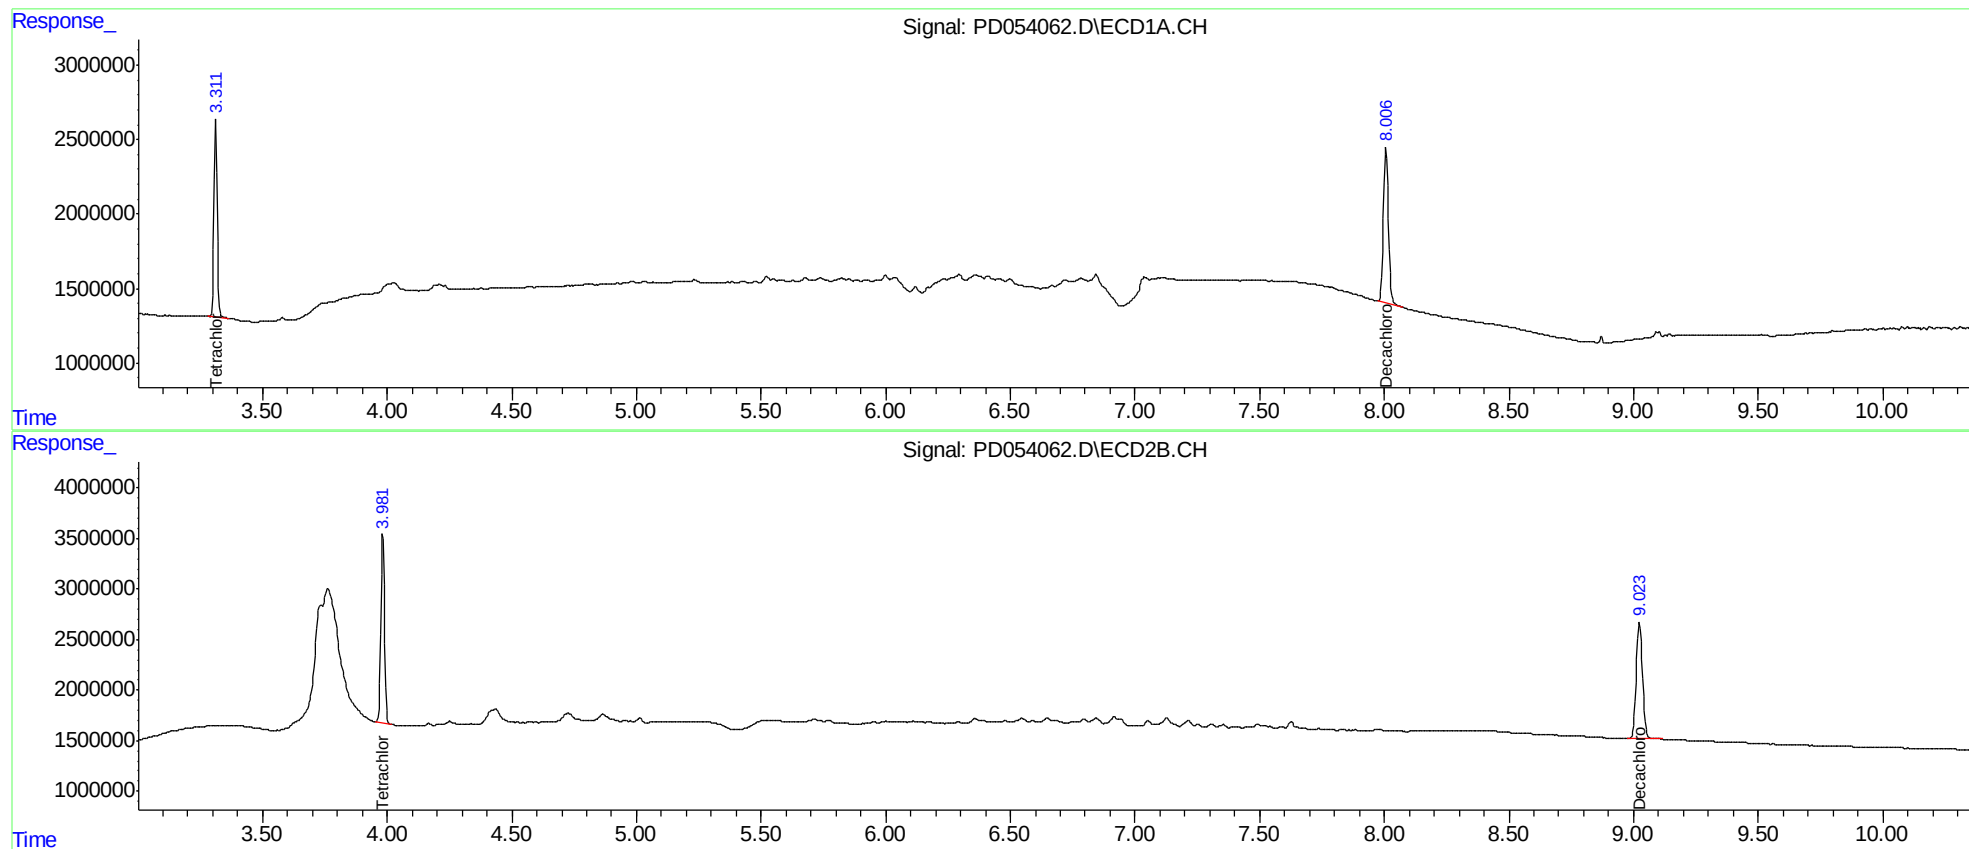


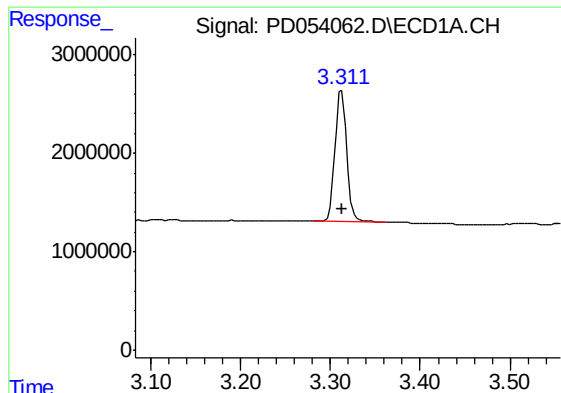

#1 Tetrachloro-m-xylene


R.T.: 3.313 min
Delta R.T.: 0.000 min
Response: 12009729
Conc: 19.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOD-MDL-WATER-01-QT3-2019

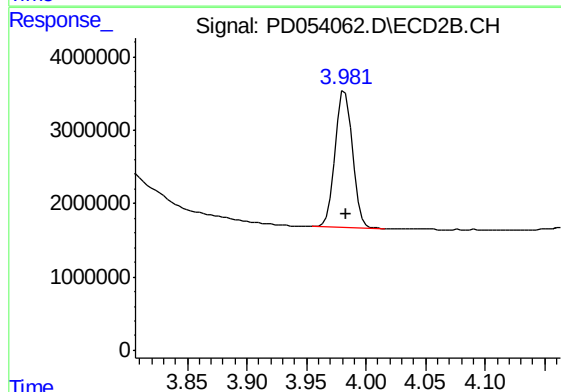


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 18577608
Conc: 19.73 ng/ml

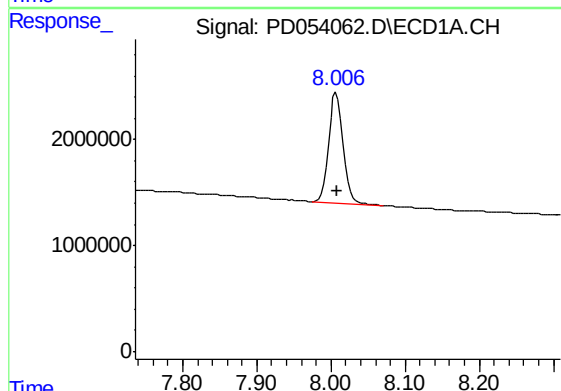

#7 Decachlorobiphenyl

R.T.: 8.007 min
Delta R.T.: 0.000 min
Response: 14389077
Conc: 21.09 ng/ml

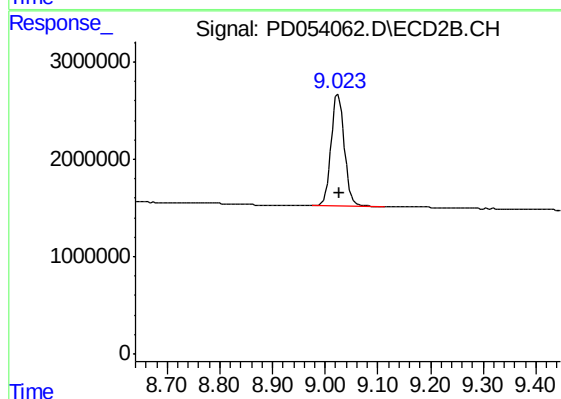

#7 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: -0.002 min
Response: 20058532
Conc: 21.06 ng/ml