

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072022\
 Data File : PD071041.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2022 13:08
 Operator : AR\AJ
 Sample : N3739-02MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 H0B39MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/21/2022
 Supervised By :Ankita Jodhani 07/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 23:53:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.480	4.126	48244514	514.6E6	20.051	21.929
27)	SA Decachlor...	8.252	9.326	96699293	377.7E6	38.088	40.898
Target Compounds							
2)	A alpha-BHC	3.923	4.531	199.1E6	1621.1E6	53.061	53.711
3)	MA gamma-BHC...	4.207	4.825	190.2E6	1378.8E6	52.237	53.281
4)	MA Heptachlor	4.506	5.342	186.7E6	980.6E6	53.569m	48.931
5)	MB Aldrin	4.755	5.654	191.0E6	836.4E6	52.855	48.061
6)	B beta-BHC	4.455	5.001	75906144	518.9E6	48.450m	38.800
7)	B delta-BHC	4.662	5.226	183.5E6	1086.2E6	52.681	47.890
8)	B Heptachlo...	5.201	6.049	172.7E6	686.6E6	51.877	46.234
9)	A Endosulfan I	5.541	6.414	159.4E6	637.5E6	52.863	48.074
10)	B trans-Chl...	5.428	6.287	176.5E6	703.6E6	50.720	46.731
11)	B cis-Chlor...	5.487	6.359	174.7E6	668.7E6	51.110	46.299
12)	B 4,4'-DDE	5.653	6.514	333.8E6	1330.4E6	103.745	97.001
13)	MA Dieldrin	5.785	6.676	363.9E6	1411.6E6	108.681	101.940
14)	MA Endrin	6.044	6.899	319.8E6	1055.1E6	115.348	101.052
15)	B Endosulfa...	6.317	7.113	289.6E6	1161.7E6	105.595	100.860
16)	A 4,4'-DDD	6.171	7.014	276.3E6	1109.6E6	106.074	101.459
17)	MA 4,4'-DDT	6.411	7.316	298.6E6	1170.2E6	111.593	104.563
18)	B Endrin al...	6.487	7.239	220.4E6	891.6E6	96.196	91.704
19)	B Endosulfa...	6.701	7.463	276.4E6	1084.8E6	98.661	95.689
20)	A Methoxychlor	6.963	7.776	717.1E6	2683.2E6	518.625	512.843
21)	B Endrin ke...	7.194	7.944	328.5E6	1263.0E6	105.978	102.285

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072022\
Data File : PD071041.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2022 13:08
Operator : AR\AJ
Sample : N3739-02MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 23:53:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

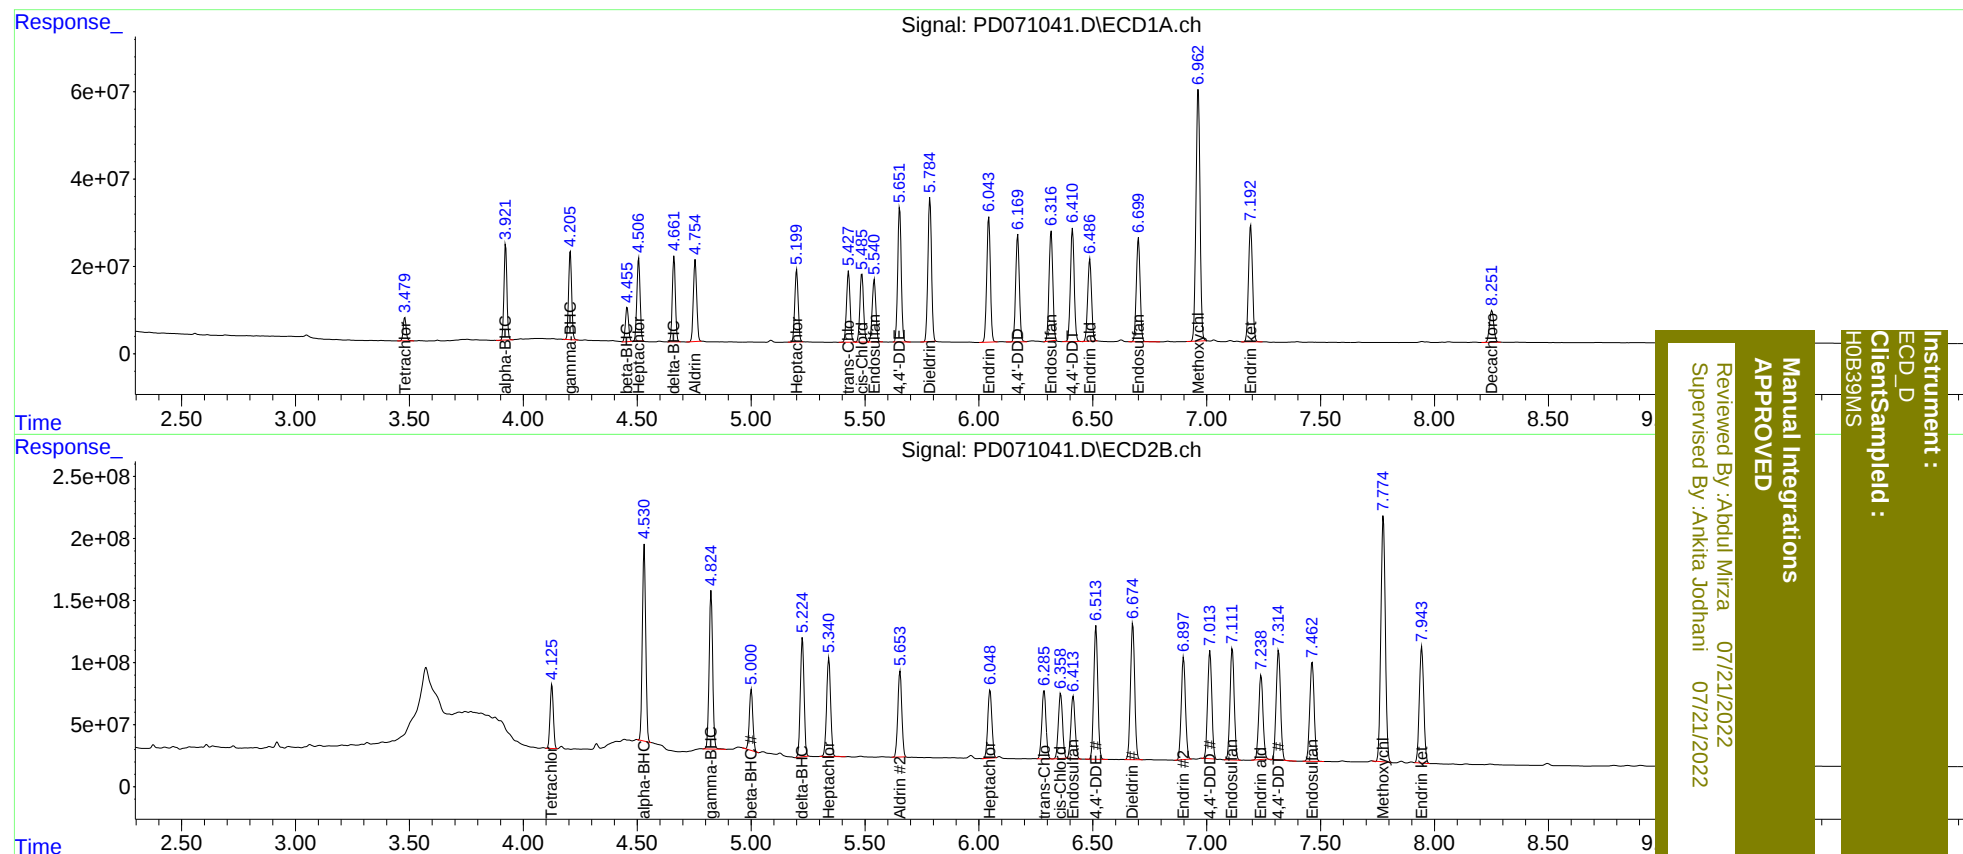

Instrument :
ECD_D
ClientSampled :
HOB39MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 07/21/2022
Supervised By: Ankita Jodhani 07/21/2022