

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072022\
 Data File : PD071051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2022 15:32
 Operator : AR\AJ
 Sample : N3709-10MS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 H0B25MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/21/2022
 Supervised By : Ankita Jodhani 07/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 23:57:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.126	29987415	317.3E6	12.463	13.522
27)	SA Decachlor...	8.244	9.325	55234908	227.0E6	21.756	24.578
Target Compounds							
2)	A alpha-BHC	3.915	4.531	181.0E6	1284.2E6	48.243m	42.549
3)	MA gamma-BHC...	4.200	4.825	150.7E6	1068.2E6	41.395	41.276
4)	MA Heptachlor	4.500	5.340	166.3E6	728.3E6	47.724	36.338m
5)	MB Aldrin	4.747	5.654	173.7E6	712.5E6	48.079m	40.942
6)	B beta-BHC	4.449	5.001	55507249	430.7E6	35.430	32.207
7)	B delta-BHC	4.654	5.225	148.6E6	837.6E6	42.646	36.928
8)	B Heptachlo...	5.193	6.049	141.2E6	590.5E6	42.412	39.766
9)	A Endosulfan I	5.533	6.414	118.3E6	447.1E6	39.235	33.717
10)	B trans-Chl...	5.420	6.286	166.1E6	543.5E6	47.740	36.098
11)	B cis-Chlor...	5.479	6.358	149.0E6	520.3E6	43.611	36.025
12)	B 4,4'-DDE	5.644	6.513	249.4E6	995.1E6	77.517	72.549
13)	MA Dieldrin	5.777	6.675	290.7E6	1049.8E6	86.814	75.814
14)	MA Endrin	6.036	6.898	235.2E6	880.7E6	84.851	84.343
15)	B Endosulfa...	6.309	7.112	225.2E6	903.8E6	82.118	78.470
16)	A 4,4'-DDD	6.162	7.014	204.3E6	837.8E6	78.435	76.603
17)	MA 4,4'-DDT	6.403	7.315	226.0E6	890.7E6	84.458	79.590
18)	B Endrin al...	6.479	7.238	172.8E6	662.6E6	75.450	68.150
19)	B Endosulfa...	6.692	7.462	206.6E6	804.2E6	73.772	70.931
20)	A Methoxychlor	6.954	7.774	571.6E6	2060.6E6	413.362	393.840
21)	B Endrin ke...	7.186	7.944	243.8E6	938.2E6	78.646	75.977

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072022\
Data File : PD071051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2022 15:32
Operator : AR\AJ
Sample : N3709-10MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 23:57:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

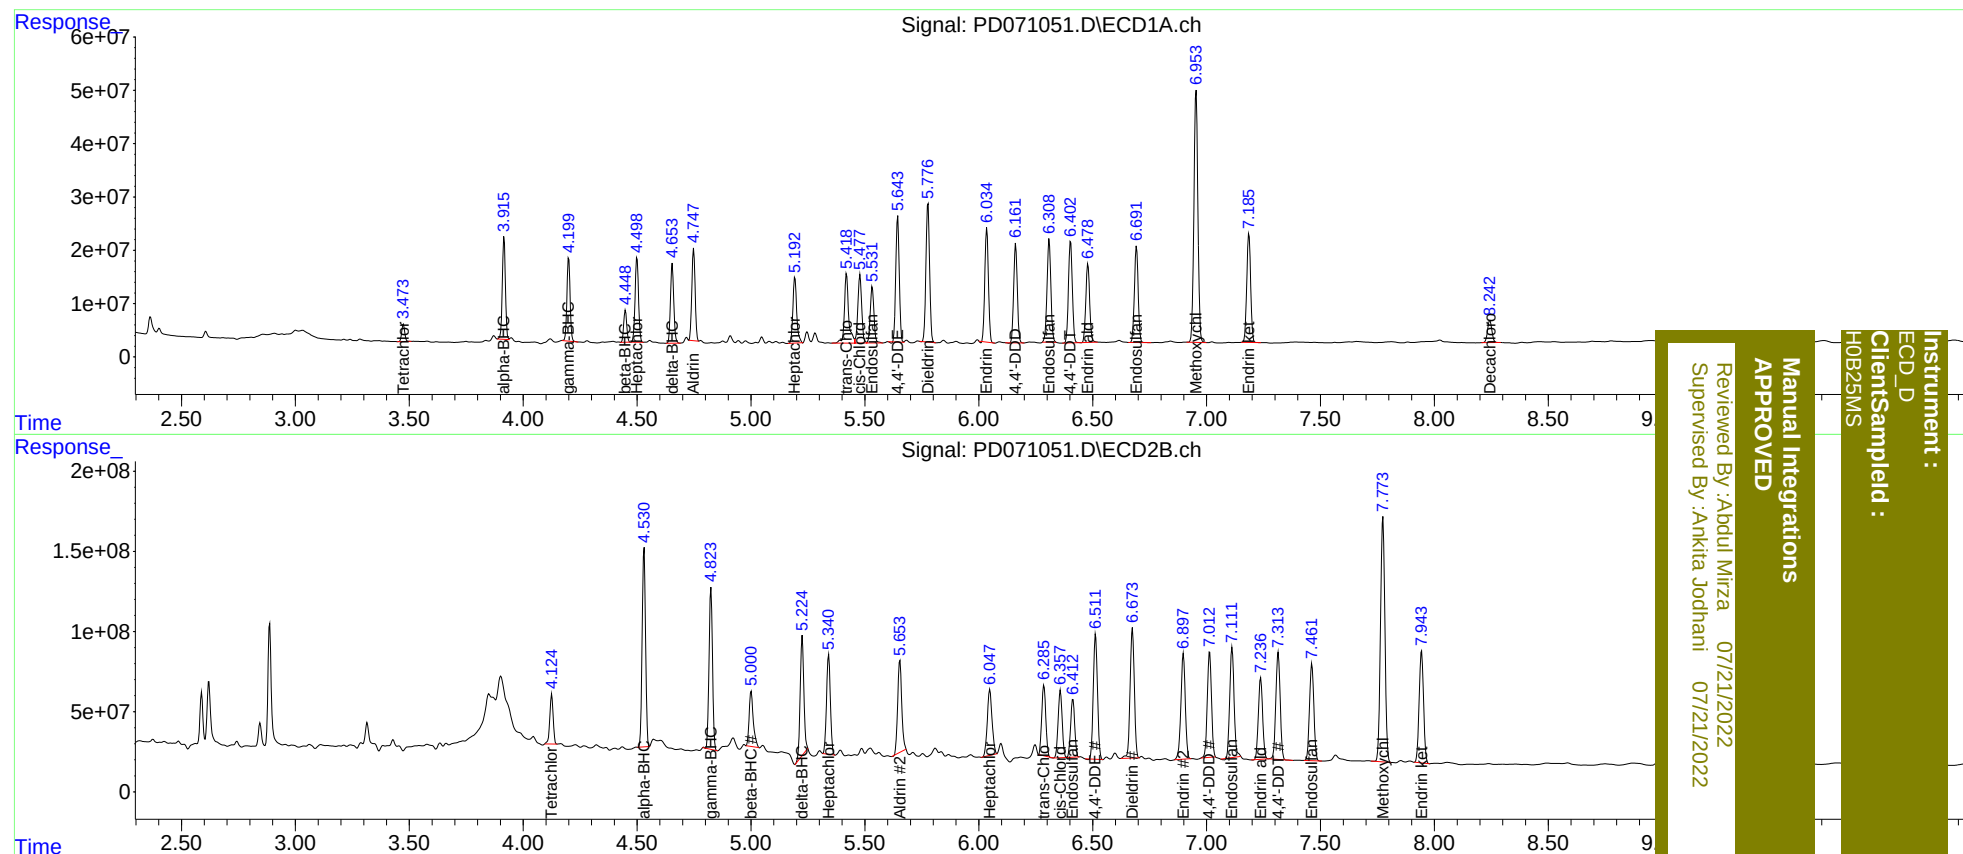

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 07/21/2022
Supervised By: Ankita Jodhani 07/21/2022

Instrument :
ECD_D
ClientSampled :
HOB25MS