

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072022\
 Data File : PD071052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2022 15:46
 Operator : AR\AJ
 Sample : N3709-11MSD
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 H0B25MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/21/2022
 Supervised By : Ankita Jodhani 07/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 23:58:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 14 05:14:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.126	30057243	317.9E6	12.492	13.547
27)	SA Decachlor...	8.243	9.324	55297773	214.5E6	21.781	23.230
Target Compounds							
2)	A alpha-BHC	3.916	4.532	180.8E6	1268.3E6	48.182	42.022
3)	MA gamma-BHC...	4.200	4.825	150.5E6	1060.2E6	41.348	40.969
4)	MA Heptachlor	4.500	5.340	166.3E6	723.4E6	47.727	36.094m
5)	MB Aldrin	4.747	5.653	174.0E6	777.4E6	48.163m	44.668m
6)	B beta-BHC	4.450	5.001	55424843	428.4E6	35.377	32.031
7)	B delta-BHC	4.655	5.225	148.2E6	833.0E6	42.555	36.728
8)	B Heptachlo...	5.193	6.049	140.6E6	585.4E6	42.214	39.420
9)	A Endosulfan I	5.533	6.414	117.9E6	446.0E6	39.117	33.636
10)	B trans-Chl...	5.420	6.286	160.6E6	539.6E6	46.151	35.838
11)	B cis-Chlor...	5.479	6.359	148.5E6	521.0E6	43.443	36.072
12)	B 4,4'-DDE	5.644	6.512	255.2E6	1010.8E6	79.323m	73.696m
13)	MA Dieldrin	5.777	6.675	290.2E6	1008.1E6	86.664	72.801
14)	MA Endrin	6.036	6.898	235.6E6	881.8E6	84.971	84.458
15)	B Endosulfa...	6.309	7.112	223.9E6	899.5E6	81.648	78.096
16)	A 4,4'-DDD	6.162	7.014	203.9E6	831.3E6	78.293	76.006
17)	MA 4,4'-DDT	6.404	7.315	224.9E6	885.1E6	84.039	79.090
18)	B Endrin al...	6.479	7.238	172.6E6	656.7E6	75.327	67.547
19)	B Endosulfa...	6.692	7.462	205.6E6	788.5E6	73.396	69.547
20)	A Methoxychlor	6.954	7.774	569.8E6	2056.9E6	412.097	393.129
21)	B Endrin ke...	7.185	7.944	243.3E6	924.3E6	78.495	74.854

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072022\
Data File : PD071052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2022 15:46
Operator : AR\AJ
Sample : N3709-11MSD
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 23:58:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 14 05:14:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

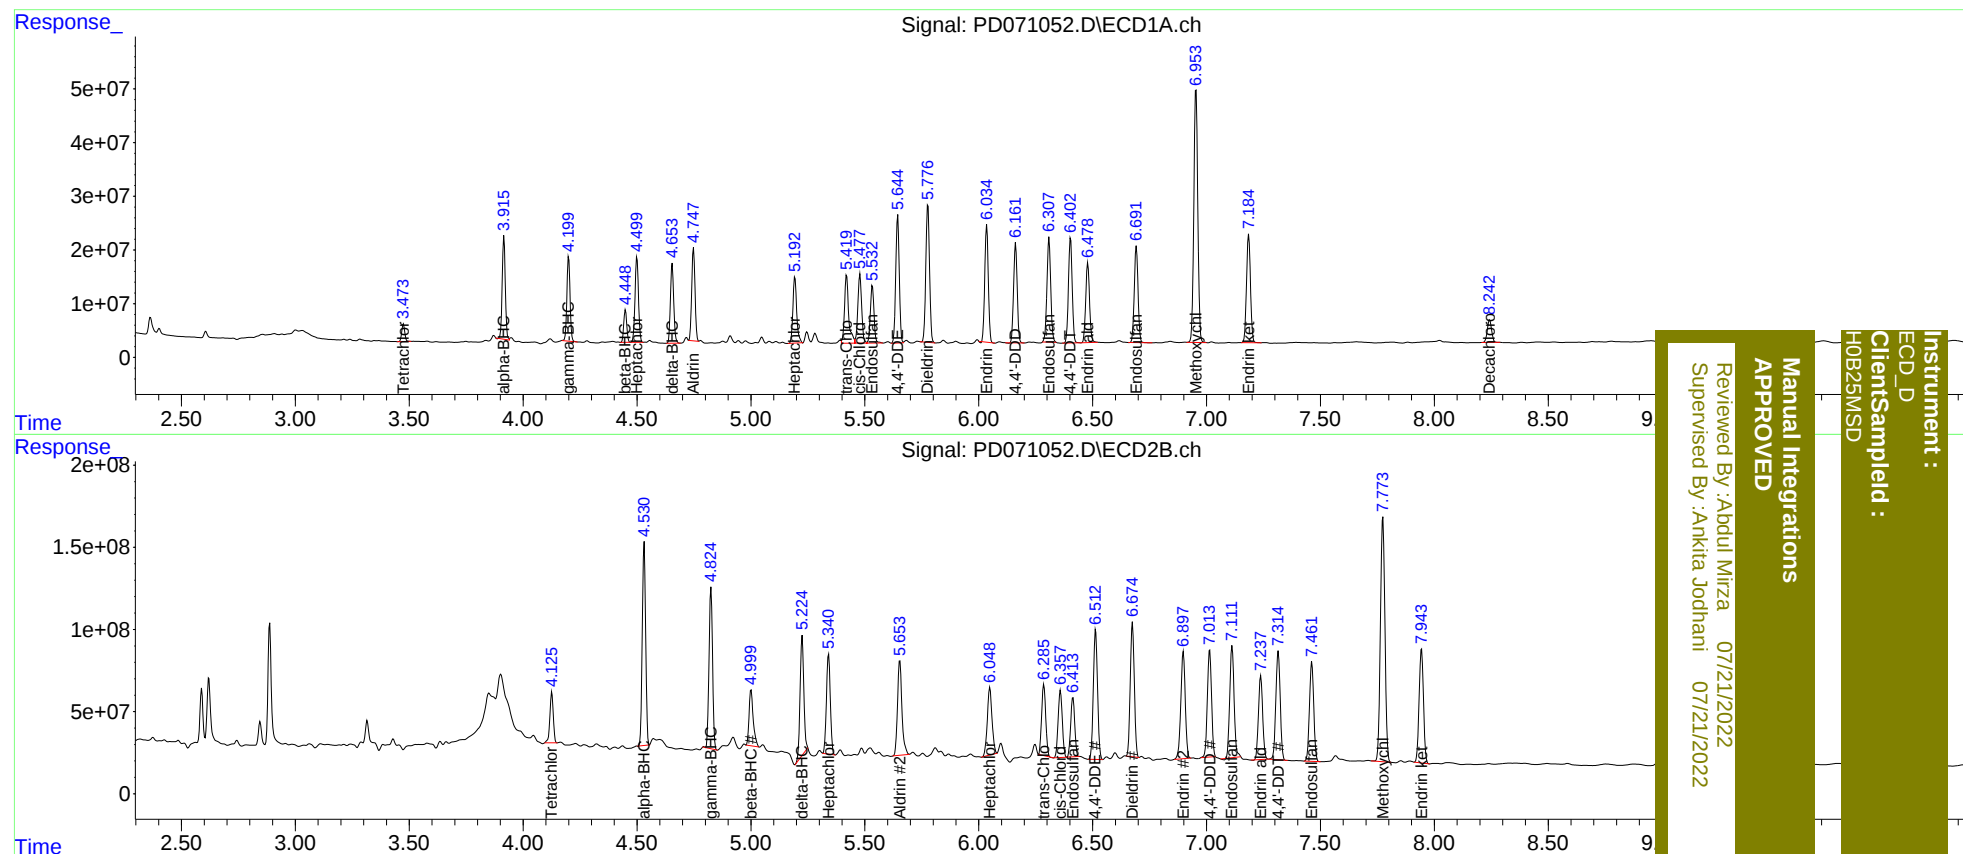

Reviewed By: Abdul Mirza 07/21/2022
Supervised By: Ankita Jodhani 07/21/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
HOB25MSD