

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072023\
 Data File : PD076923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2023 14:25
 Operator : AR\AJ
 Sample : 03534-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A4729

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/21/2023
 Supervised By : Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 21:40:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.763	33814092	18486199	15.895	17.319
2)	SA Decachlor...	9.085	7.904	63810553	30685905	26.265	28.626
Target Compounds							
7)	B delta-BHC	4.796	4.130	4122062	5658735	1.229m	3.707 #
8)	B Heptachlo...	5.687	4.708	19657170	2267173	6.561	1.612m#
10)	B trans-Chl...	5.970	4.943	8755487	6962094	2.847m	5.149m#
17)	MA 4,4'-DDT	7.008	6.020	7046554	4347667	3.156m	4.641 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072023\
Data File : PD076923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2023 14:25
Operator : AR\AJ
Sample : 03534-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 21:40:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

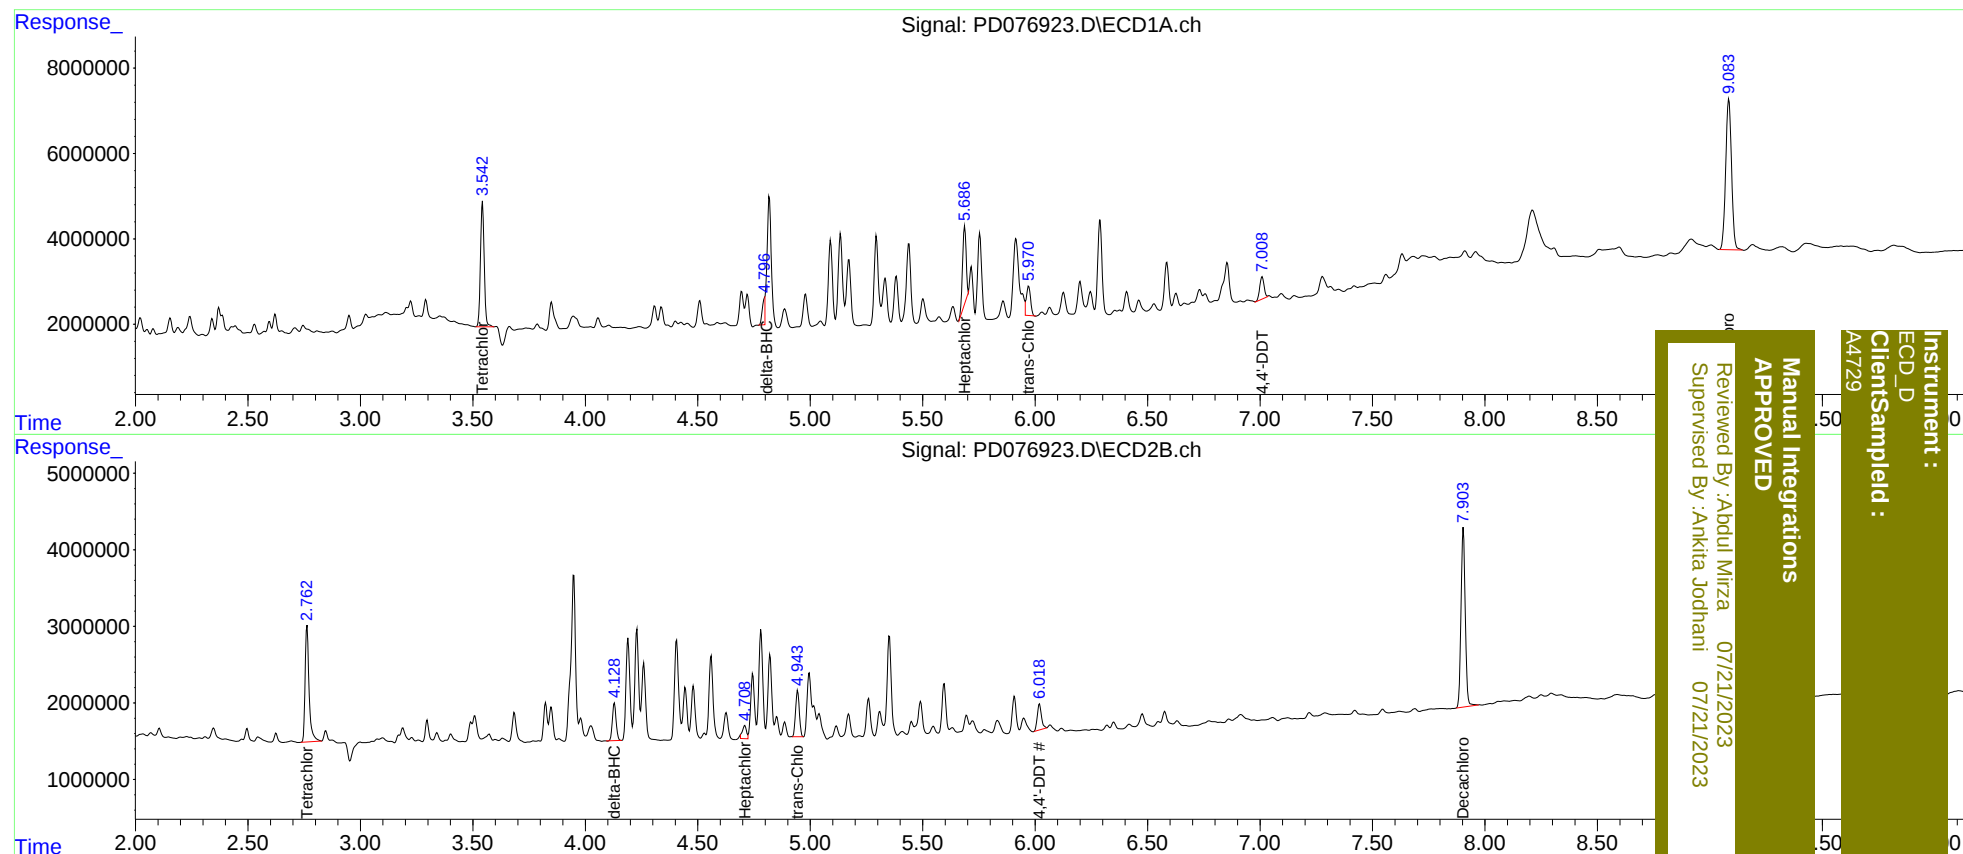

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 07/21/2023
Supervised By: Ankita Jodhani 07/21/2023

Instrument :
ECD_D
ClientSampled :
A4729