

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072023\
 Data File : PD076919.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2023 13:32
 Operator : AR\AJ
 Sample : 03534-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A4723

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/21/2023
 Supervised By : Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 21:36:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.764	36581251	19283907	17.196	18.066
2) SA Decachlor...	9.083	7.903	71521115	30458223	29.439	28.413
Target Compounds						
7) B delta-BHC	4.793	4.130	3733796	2388495	1.113m	1.565 #
8) B Heptachlo...	5.684	4.709	9531187	1215971	3.181m	0.864m#
10) B trans-Chl...	5.969	4.943	5907198	4520956	1.921m	3.343m#
17) MA 4,4'-DDT	7.007	6.019	5534346	3227101	2.479m	3.445 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072023\
Data File : PD076919.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2023 13:32
Operator : AR\AJ
Sample : 03534-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 21:36:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

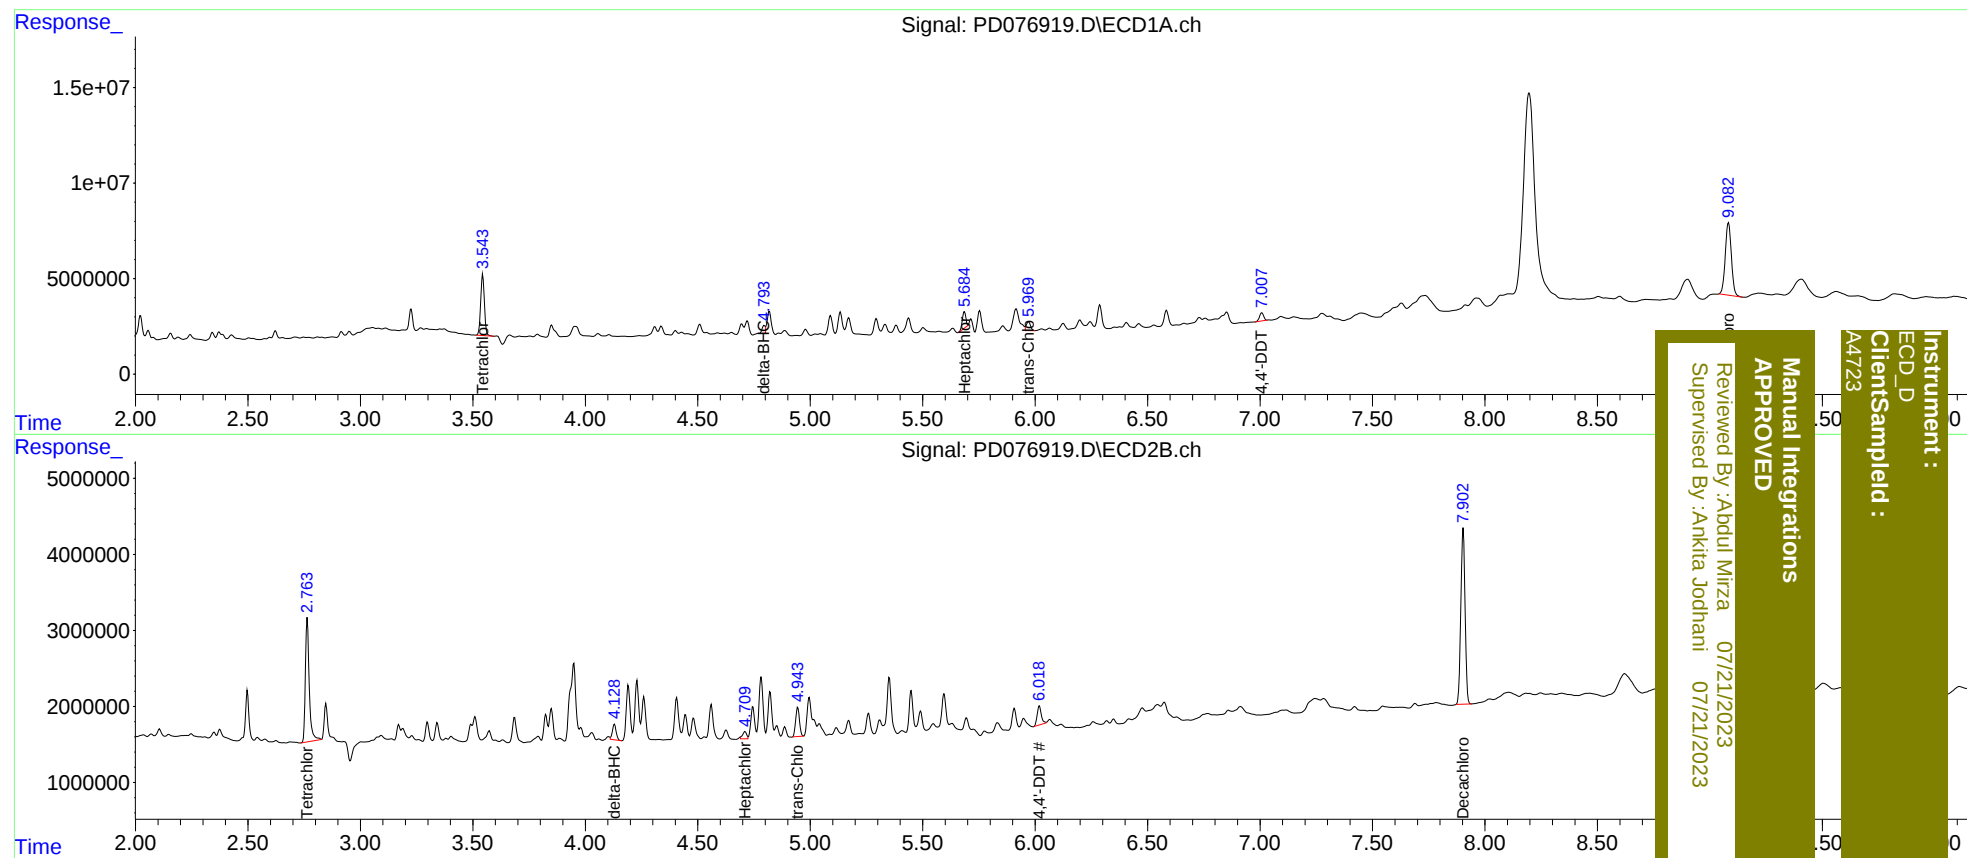

Instrument :
ECD_D
ClientSampled :
A4723

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 07/21/2023
Supervised By: Ankita Jodhani 07/21/2023