

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072023\
 Data File : PD076927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2023 15:19
 Operator : AR\AJ
 Sample : 03534-19
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A4737

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/21/2023
 Supervised By : Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 21:44:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.764	85859048	14671163	40.359	13.745 #
27)	SA Decachlor...	9.082	7.903	56882819	29340024	23.413	27.370
Target Compounds							
3)	MA gamma-BHC...	4.337	3.572	600.1E6	78174381	180.911m	52.181m#
7)	B delta-BHC	4.797	4.130	1268.3E6	320.3E6	378.206m	209.868 #
10)	B trans-Chl...	5.970	4.943	246.2E6	181.6E6	80.079m	134.289m#
17)	MA 4,4'-DDT	7.008	6.018	162.1E6	88883286	72.580m	94.881m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072023\
Data File : PD076927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2023 15:19
Operator : AR\AJ
Sample : 03534-19
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 21:44:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

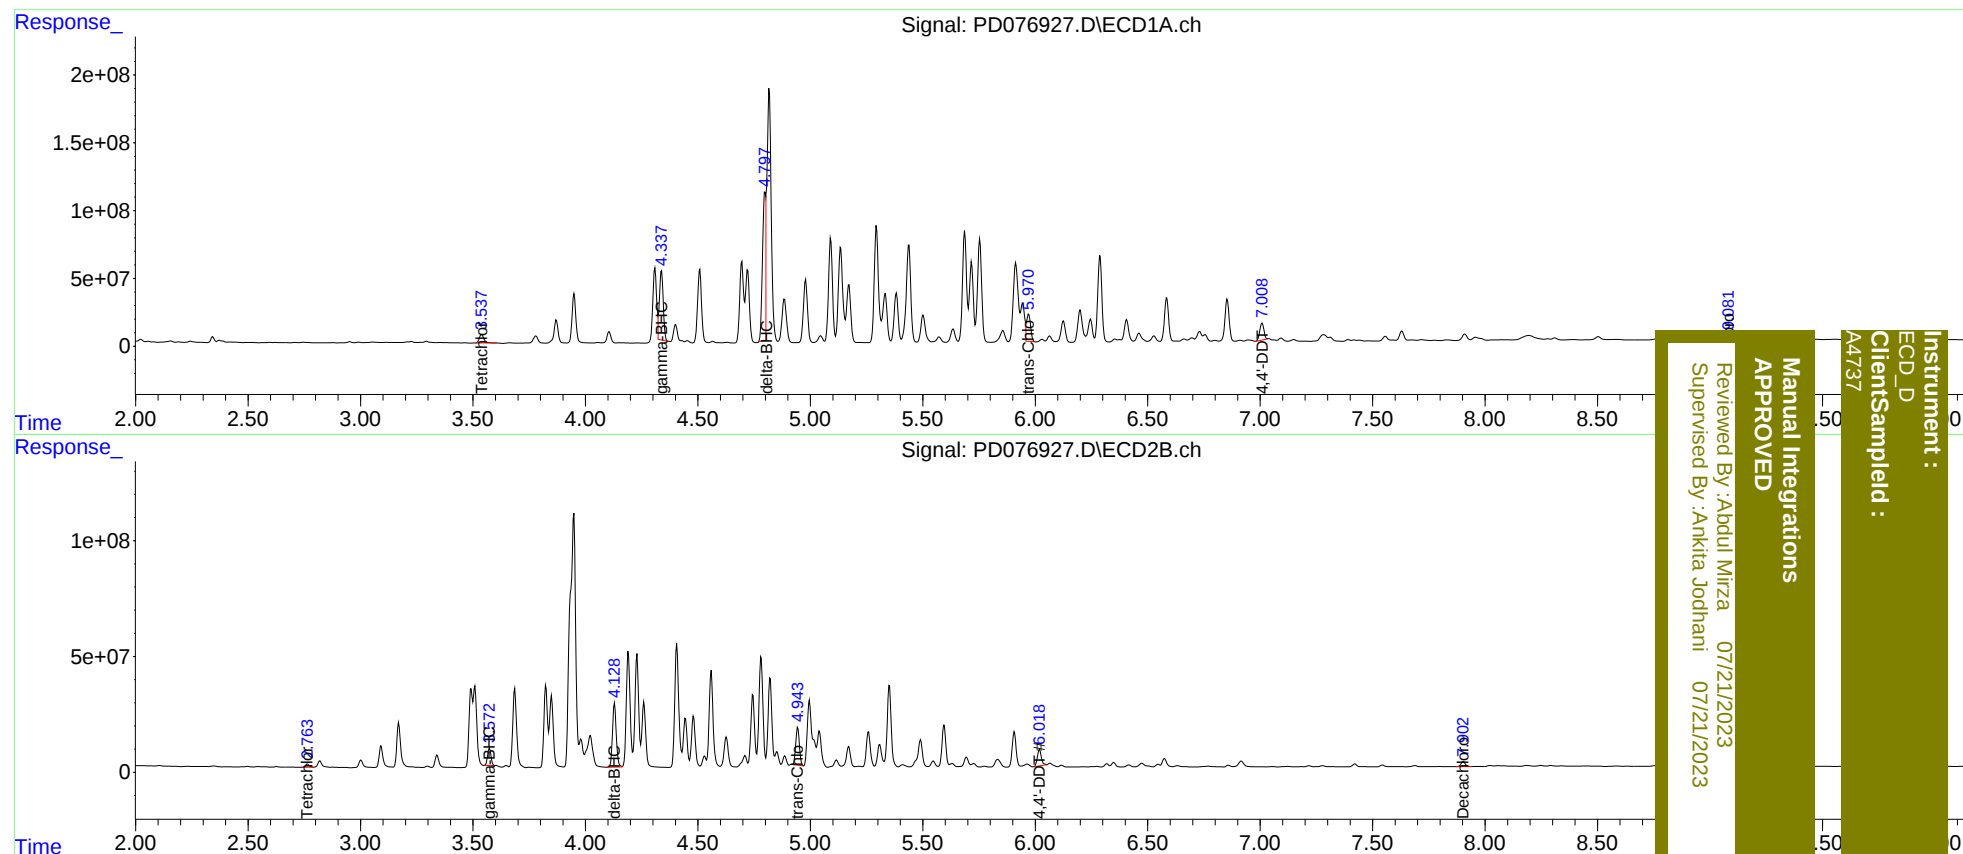

Instrument :
ECD_D
ClientSampled :
A4737

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/21/2023
Supervised By :Ankita Jodhani 07/21/2023