

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072023\
 Data File : PD076928.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2023 15:32
 Operator : AR\AJ
 Sample : 03534-23MS
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A4737MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/21/2023
 Supervised By : Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 21:45:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.764	83325742	13867341	39.169	12.991 #
27)	SA Decachlor...	9.082	7.903	53556848	27320601	22.044	25.486
Target Compounds							
2)	A alpha-BHC	3.999	3.264	184.8E6	85378370	52.147m	53.956m
3)	MA gamma-BHC...	4.336	3.572	758.2E6	73625294	228.585m	49.145m#
4)	MA Heptachlor	4.923	3.935	169.4E6	557.2E6	48.719m	372.633m#
5)	MB Aldrin	5.293	4.229	1024.2E6	593.2E6	299.520m	394.173 #
6)	B beta-BHC	4.525	3.891	56642229	30297281	37.266m	42.292
7)	B delta-BHC	4.796	4.128	1030.0E6	392.1E6	307.146m	256.864
8)	B Heptachlo...	5.687	4.712	756.8E6	137.4E6	252.596	97.634m#
9)	A Endosulfan I	6.080	5.087	171.7E6	43879024	60.290	35.415 #
10)	B trans-Chl...	5.967	4.943	238.4E6	188.6E6	77.528m	139.472m#
11)	B cis-Chlor...	6.031	5.038	171.3E6	274.7E6	54.027	194.734 #
12)	B 4,4'-DDE	6.201	5.219	565.1E6	123.2E6	193.973	101.978 #
13)	MA Dieldrin	6.357	5.350	373.4E6	529.7E6	118.338	379.809m#
14)	MA Endrin	6.586	5.625	699.9E6	146.8E6	271.525	118.688m#
15)	B Endosulfa...	6.807	5.911	261.7E6	306.6E6	98.424	254.954 #
16)	A 4,4'-DDD	6.723	5.773	341.3E6	111.0E6	151.033	117.090
17)	MA 4,4'-DDT	7.035	6.022	260.5E6	202.7E6	116.677m	216.329 #
18)	B Endrin al...	6.938	6.099	208.0E6	79161049	111.216	94.373
19)	B Endosulfa...	7.172	6.322	270.9E6	132.9E6	108.481	119.149
20)	A Methoxychlor	7.513	6.598	731.6E6	303.1E6	552.711	567.998m
21)	B Endrin ke...	7.658	6.828	292.3E6	130.7E6	105.587m	102.141

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072023\
Data File : PD076928.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2023 15:32
Operator : AR\AJ
Sample : 03534-23MS
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 21:45:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

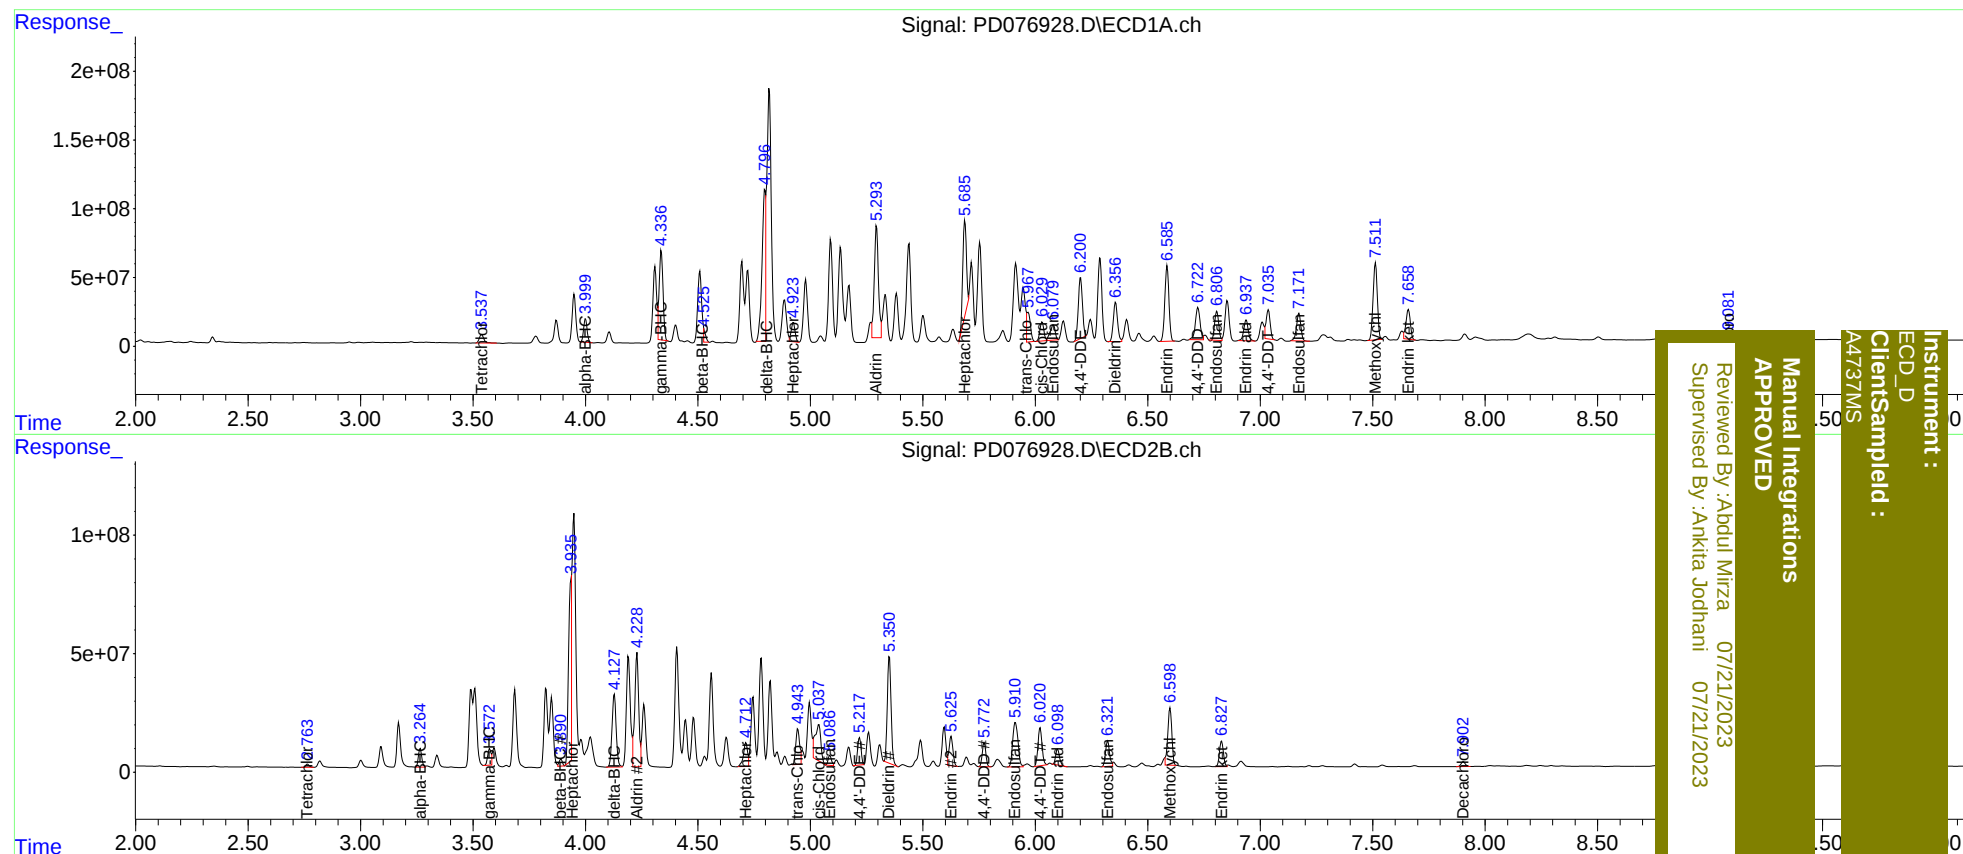

Instrument :
ECD_D
ClientSampled :
A4737MS

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 07/21/2023
Supervised By: Ankita Jodhani 07/21/2023