

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072023\
 Data File : PD076929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2023 15:46
 Operator : AR\AJ
 Sample : 03534-24MSD
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A4737MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/21/2023
 Supervised By : Ankita Jodhani 07/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 21:46:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.764	83105688	14251382	39.065	13.351 #
27)	SA Decachlor...	9.083	7.904	58228139	27843181	23.967	25.974
Target Compounds							
2)	A alpha-BHC	4.000	3.265	159.2E6	84095021	44.929	53.145
3)	MA gamma-BHC...	4.336	3.572	757.5E6	67852359	228.356m	45.291m#
4)	MA Heptachlor	4.923	3.933	180.5E6	556.4E6	51.911m	372.154m#
5)	MB Aldrin	5.293	4.229	1067.8E6	607.2E6	312.271m	403.457 #
6)	B beta-BHC	4.526	3.891	48446428	30453329	31.874m	42.510 #
7)	B delta-BHC	4.797	4.128	1193.8E6	399.9E6	355.997m	262.001 #
8)	B Heptachlo...	5.688	4.712	700.0E6	131.8E6	233.621	93.717m#
9)	A Endosulfan I	6.080	5.087	169.2E6	43752883	59.406	35.314 #
10)	B trans-Chl...	5.969	4.943	240.5E6	196.0E6	78.202m	144.956m#
11)	B cis-Chlor...	6.031	5.038	168.7E6	279.0E6	53.217	197.790 #
12)	B 4,4'-DDE	6.201	5.218	550.8E6	127.6E6	189.044	105.551 #
13)	MA Dieldrin	6.357	5.350	370.4E6	540.9E6	117.405	387.879m#
14)	MA Endrin	6.586	5.625	685.3E6	153.5E6	265.832	124.101m#
15)	B Endosulfa...	6.806	5.912	274.4E6	314.8E6	103.193m	261.726 #
16)	A 4,4'-DDD	6.722	5.774	331.6E6	111.7E6	146.739	117.886
17)	MA 4,4'-DDT	7.009	6.023	205.4E6	205.4E6	92.015m	219.257 #
18)	B Endrin al...	6.938	6.099	207.0E6	82878694	110.722	98.805m
19)	B Endosulfa...	7.173	6.322	267.9E6	131.6E6	107.275	117.909
20)	A Methoxychlor	7.512	6.599	711.7E6	309.4E6	537.661	579.812m
21)	B Endrin ke...	7.658	6.829	290.8E6	132.2E6	105.043m	103.290

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072023\
Data File : PD076929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2023 15:46
Operator : AR\AJ
Sample : 03534-24MSD
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 21:46:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

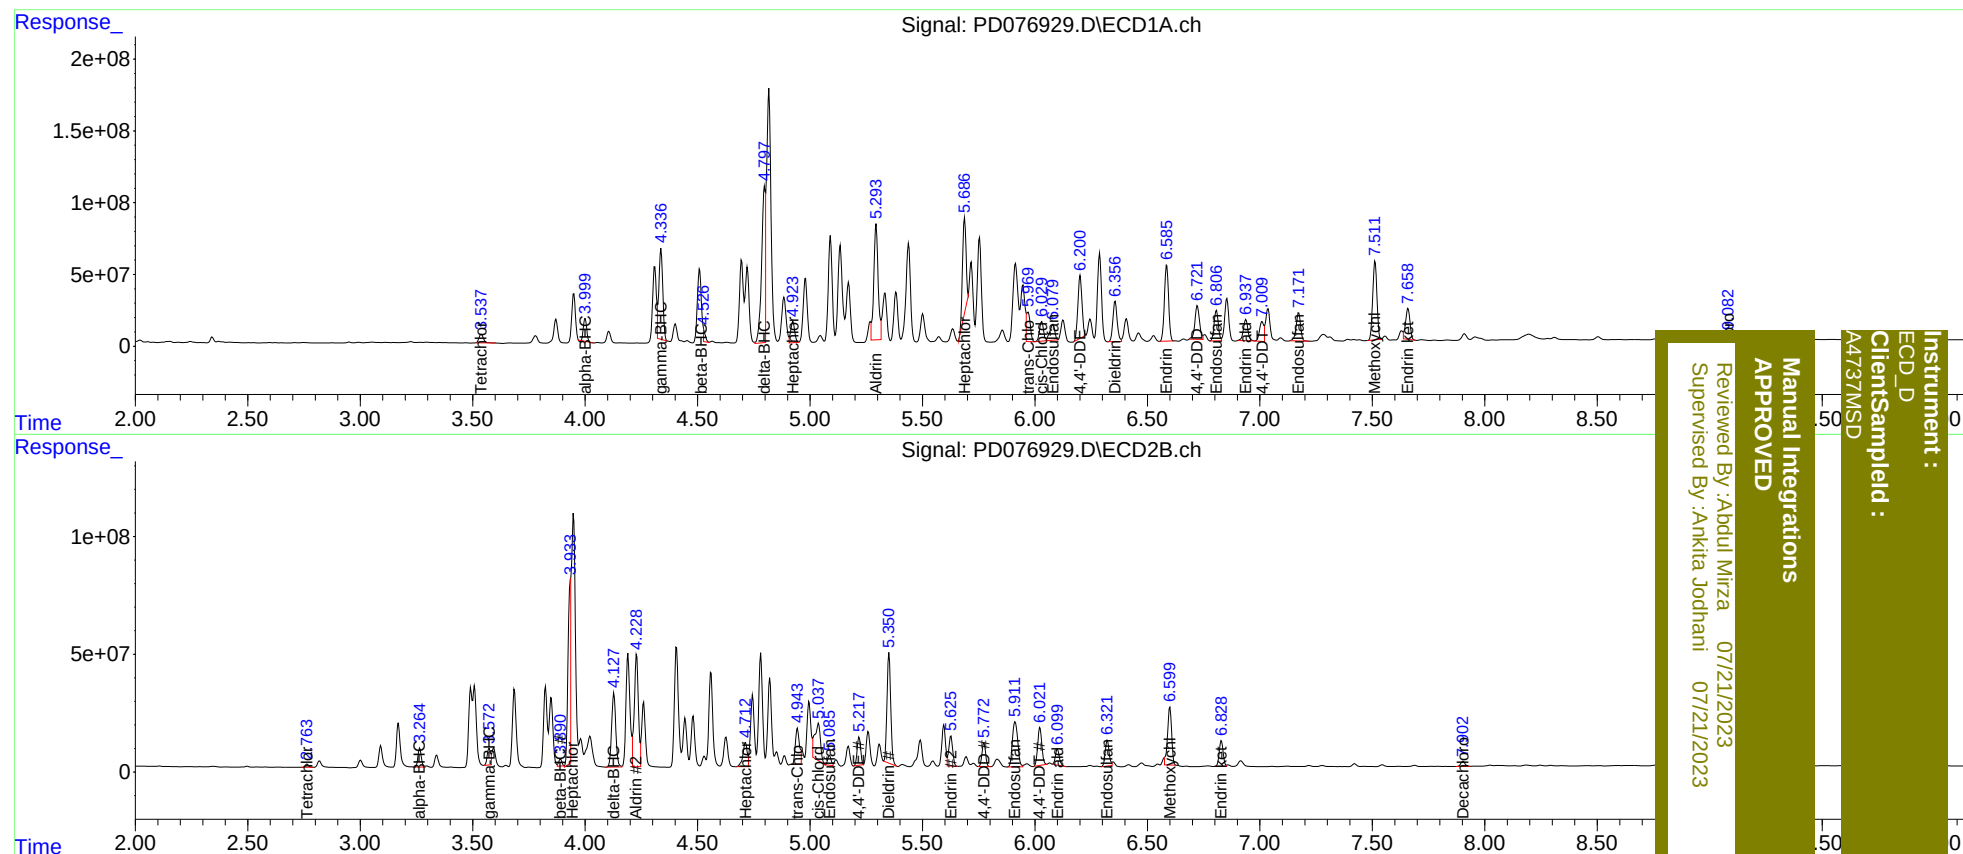

Reviewed By: Abdul Mirza 07/21/2023
Supervised By: Ankita Jodhani 07/21/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
A4737MSD