

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072122\
 Data File : PD071069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2022 20:55
 Operator : AR\AJ
 Sample : N3776-01 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 72-11966

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/21/2022
 Supervised By :Ankita Jodhani 07/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 23:49:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 05:30:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.473	4.126	6012686	63099909	2.075m	2.182
28) SA Decachlor...	8.241	9.318	9354261	17359054	3.062	1.522m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072122\
Data File : PD071069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2022 20:55
Operator : AR\AJ
Sample : N3776-01 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
72-11966


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/21/2022
Supervised By : Ankita Jodhani 07/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 23:49:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 05:30:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

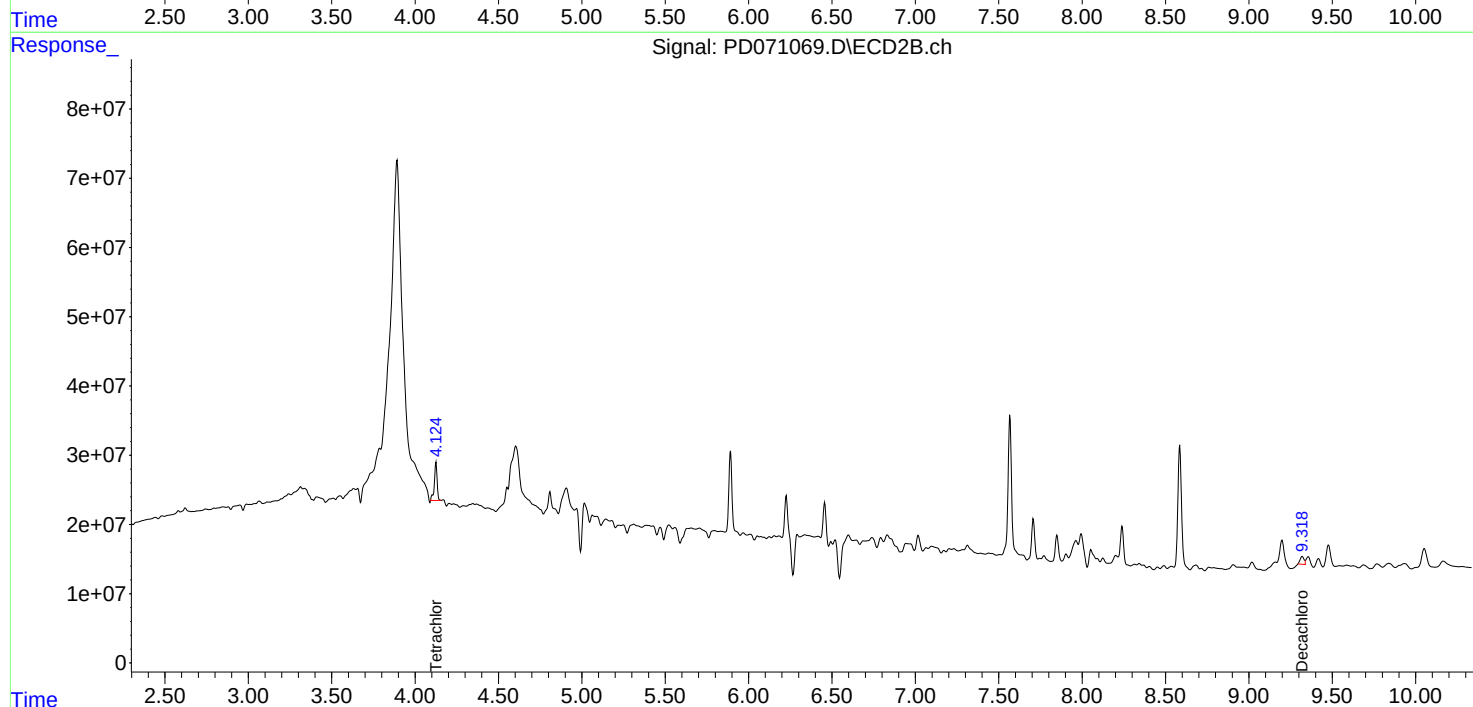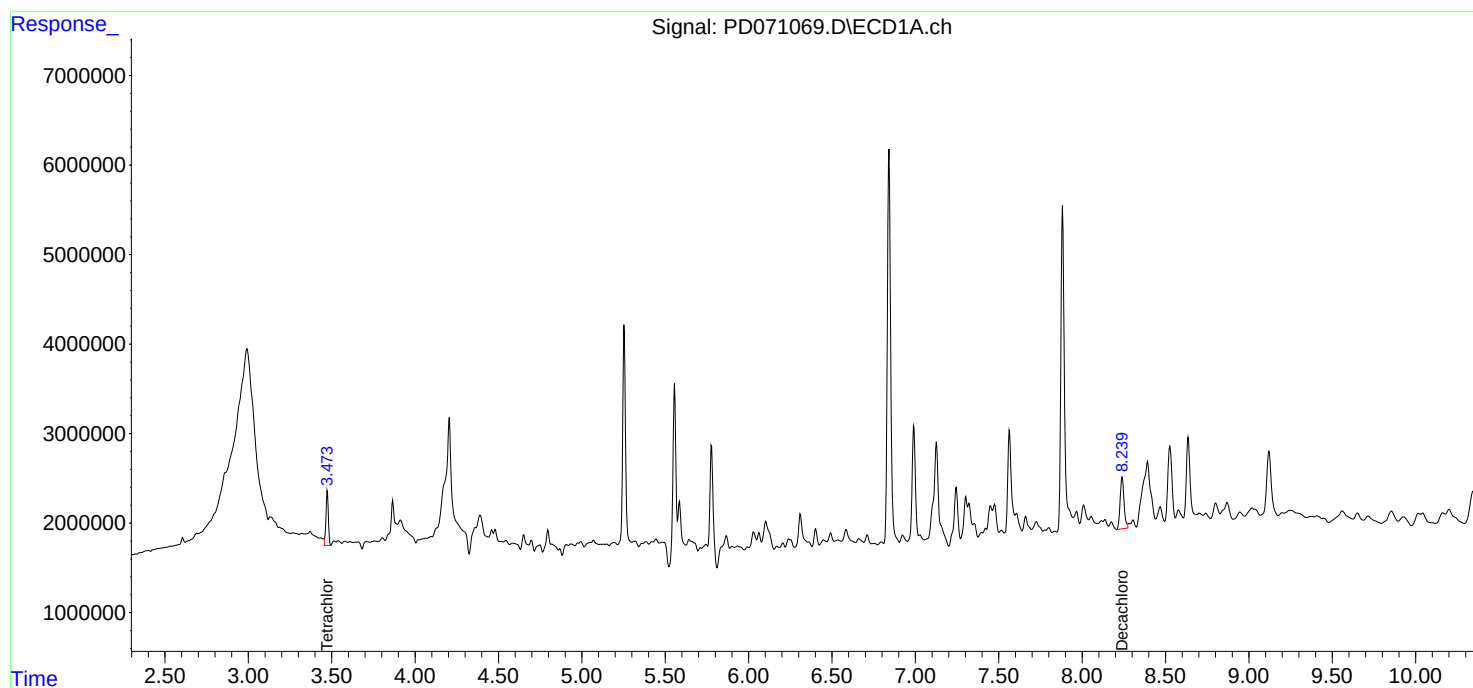

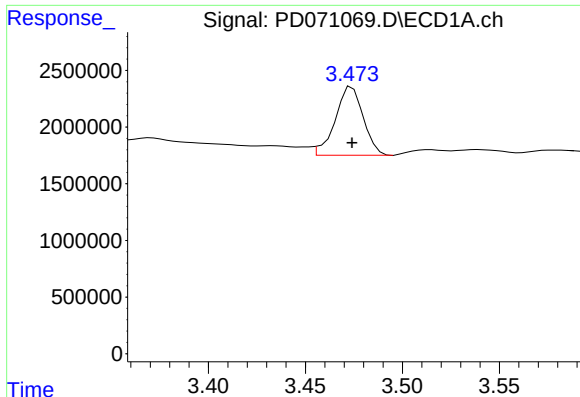


#1 Tetrachloro-m-xylene

R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 6012686
Conc: 2.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
72-11966


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/21/2022
Supervised By :Ankita Jodhani 07/21/2022

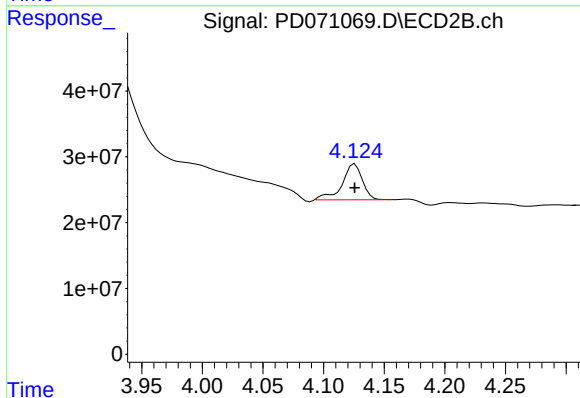


#1 Tetrachloro-m-xylene

R.T.: 4.126 min
Delta R.T.: 0.000 min
Response: 63099909
Conc: 2.18 ng/ml

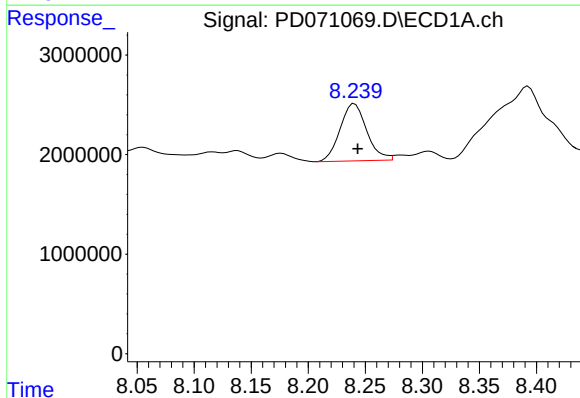

#28 Decachlorobiphenyl

R.T.: 8.241 min
Delta R.T.: -0.003 min
Response: 9354261
Conc: 3.06 ng/ml

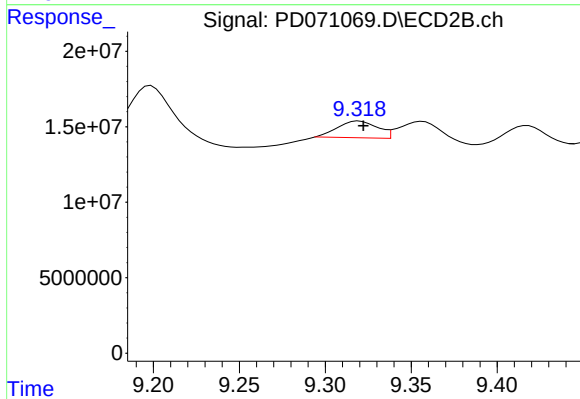

#28 Decachlorobiphenyl

R.T.: 9.318 min
Delta R.T.: -0.004 min
Response: 17359054
Conc: 1.52 ng/ml m