

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072123\
 Data File : PD076934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2023 07:36
 Operator : AR\AJ
 Sample : PIBLK217
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 21:14:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.764	52642234	27738877	24.745	25.987
27)	SA Decachlor...	9.091	7.906	126.3E6	61409130	51.989	57.286
Target Compounds							
4)	MA Heptachlor	0.000	3.894f	0	291784	N.D.	0.195
5)	MB Aldrin	0.000	4.221	0	379754	N.D.	0.252
6)	B beta-BHC	0.000	3.894	0	291784	N.D.	0.407
7)	B delta-BHC	4.773	0.000	6993414	0	2.085	N.D. #
8)	B Heptachlo...	0.000	4.740	0	231567	N.D.	0.165
10)	B trans-Chl...	5.987	0.000	1438834	0	0.468	N.D. #
11)	B cis-Chlor...	5.987f	0.000	1438834	0	0.454	N.D. #
18)	B Endrin al...	0.000	6.111	0	268543	N.D.	0.320
21)	B Endrin ke...	0.000	6.792f	0	52029	N.D.	<MDL
26)	Toxaphene-5	0.000	6.749	0	139689	N.D.	3.773


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072123\
Data File : PD076934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2023 07:36
Operator : AR\AJ
Sample : PIBLK217
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 21:14:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

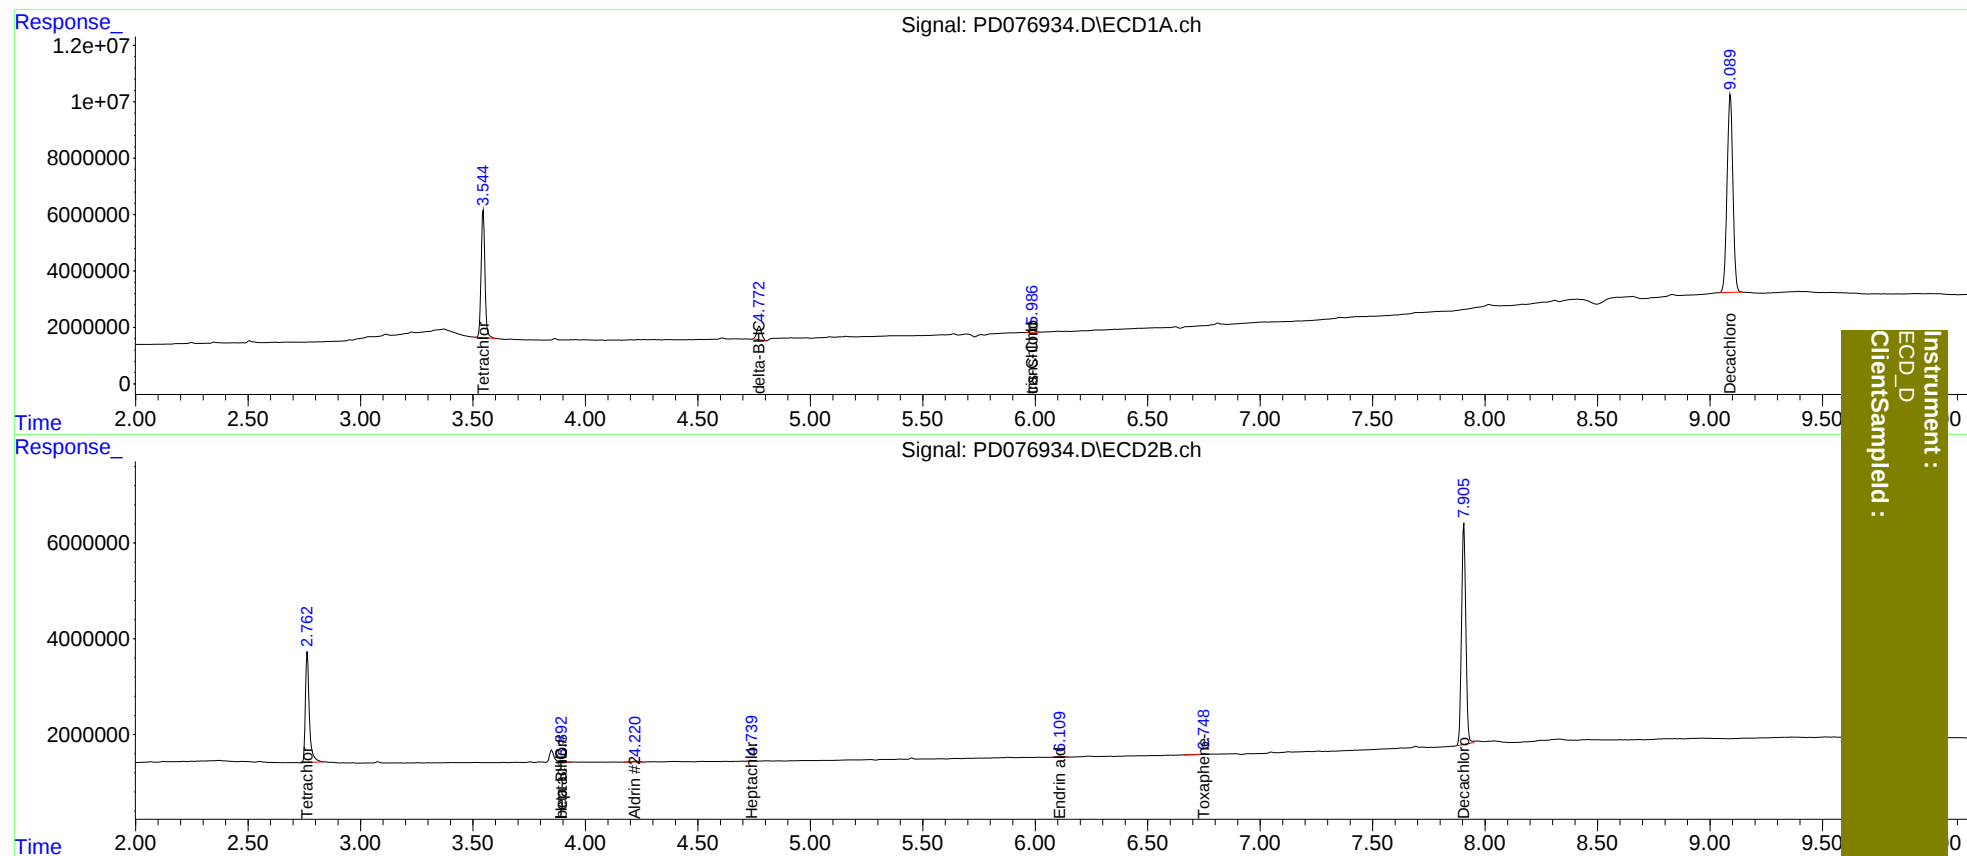


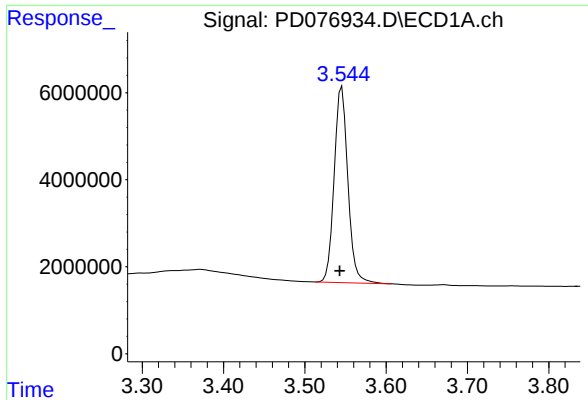

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.003 min
Response: 52642234
Conc: 24.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

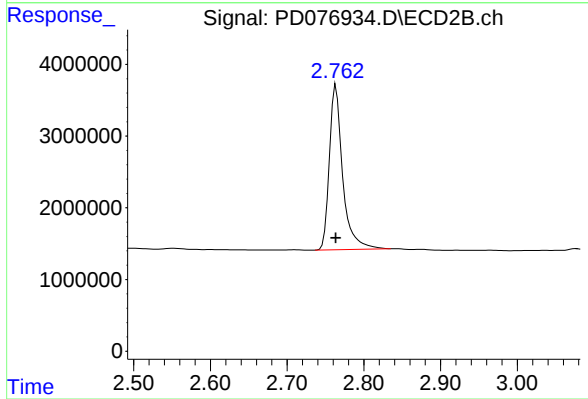


#1 Tetrachloro-m-xylene

R.T.: 2.764 min
Delta R.T.: 0.000 min
Response: 27738877
Conc: 25.99 ng/ml

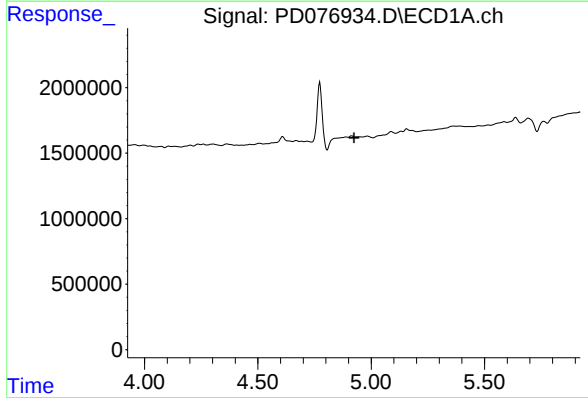


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.924 min
Response: 0
Conc: N.D.

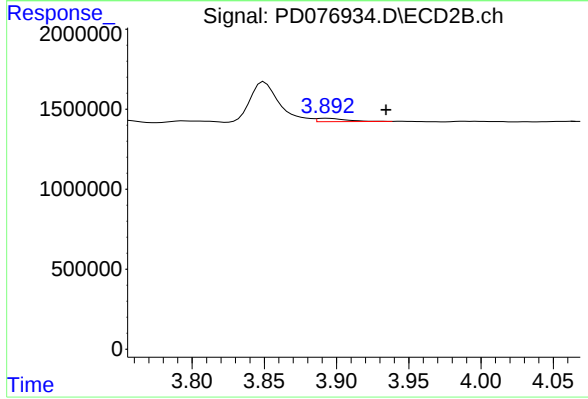

#4 Heptachlor

R.T.: 3.894 min
Delta R.T.: -0.041 min
Response: 291784
Conc: 0.20 ng/ml

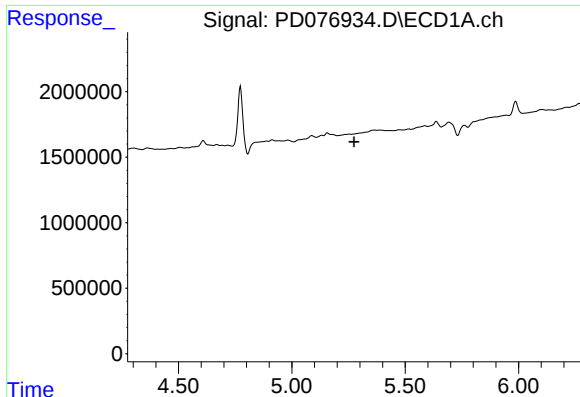

#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

#5 Aldrin


R.T.: 4.221 min
Delta R.T.: 0.005 min
Response: 379754
Conc: 0.25 ng/ml

#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.537 min
Response: 0
Conc: N.D.

#6 beta-BHC


R.T.: 3.894 min
Delta R.T.: 0.000 min
Response: 291784
Conc: 0.41 ng/ml

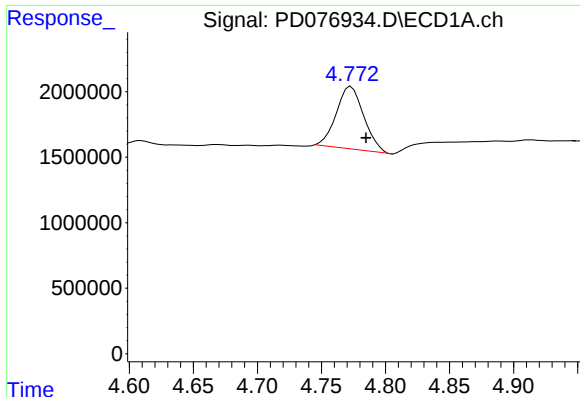

#7 delta-BHC


R.T.: 4.773 min
Delta R.T.: -0.012 min
Response: 6993414
Conc: 2.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

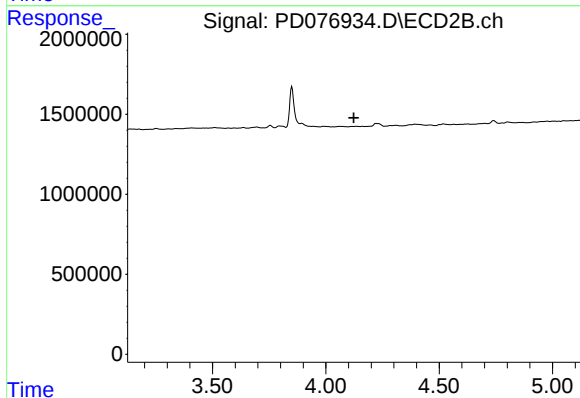


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.123 min
Response: 0
Conc: N.D.

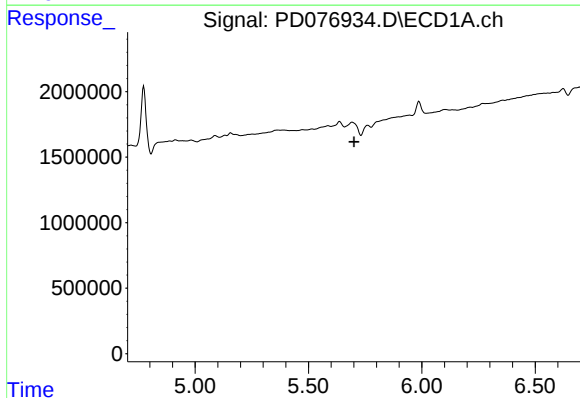


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.701 min
Response: 0
Conc: N.D.

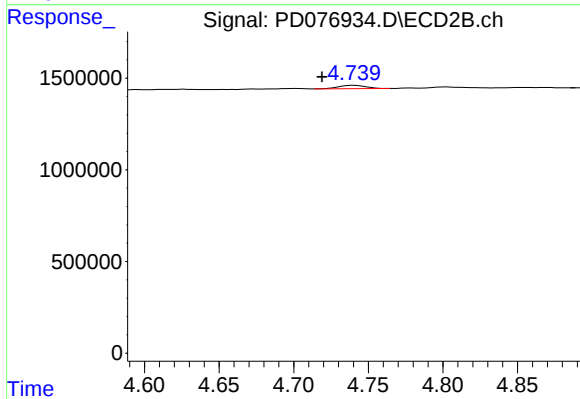

#8 Heptachlor epoxide


R.T.: 4.740 min
Delta R.T.: 0.021 min
Response: 231567
Conc: 0.16 ng/ml

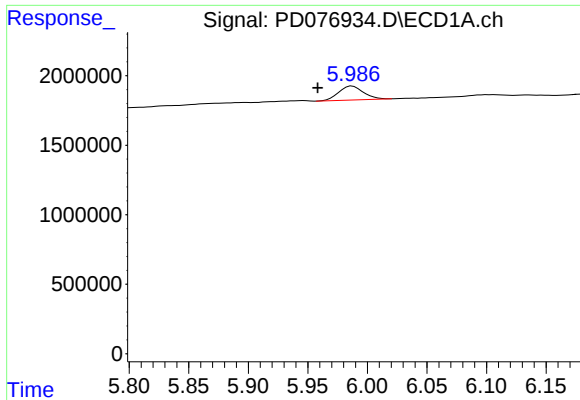

#10 trans-Chlordane


R.T.: 5.987 min
Delta R.T.: 0.029 min
Response: 1438834
Conc: 0.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

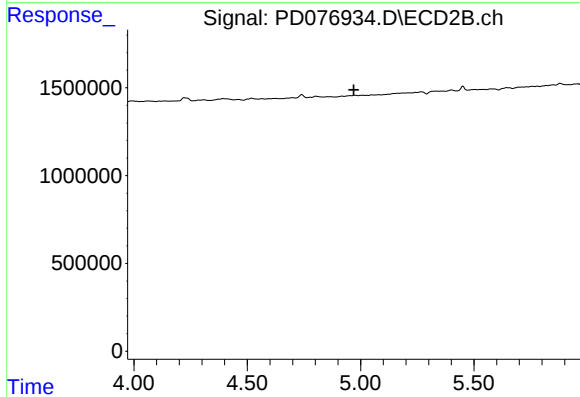


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.969 min
Response: 0
Conc: N.D.

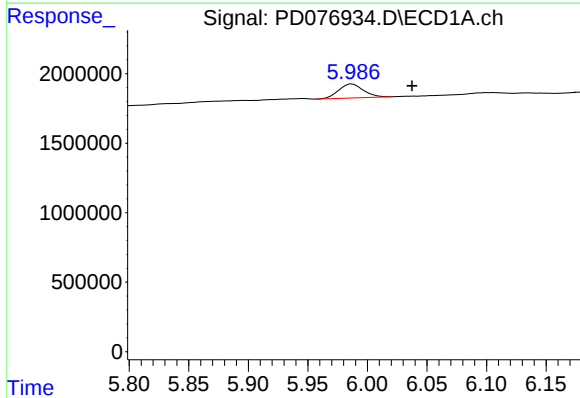


#11 cis-Chlordane

R.T.: 5.987 min
Delta R.T.: -0.050 min
Response: 1438834
Conc: 0.45 ng/ml

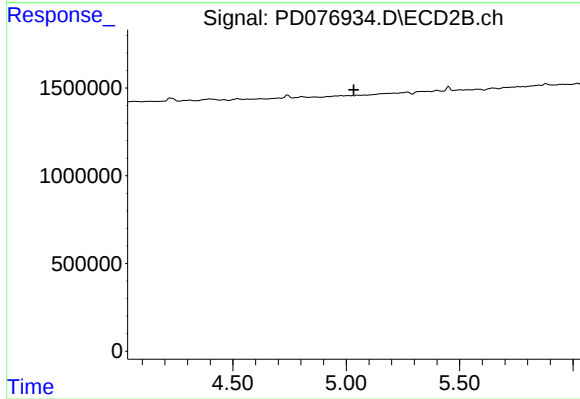

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.033 min
Response: 0
Conc: N.D.

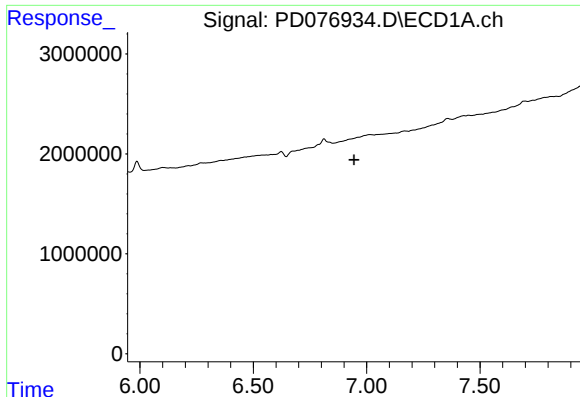

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.945 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

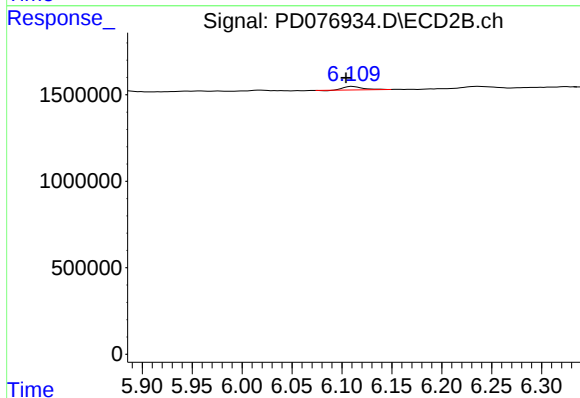


#18 Endrin aldehyde

R.T.: 6.111 min
Delta R.T.: 0.006 min
Response: 268543
Conc: 0.32 ng/ml

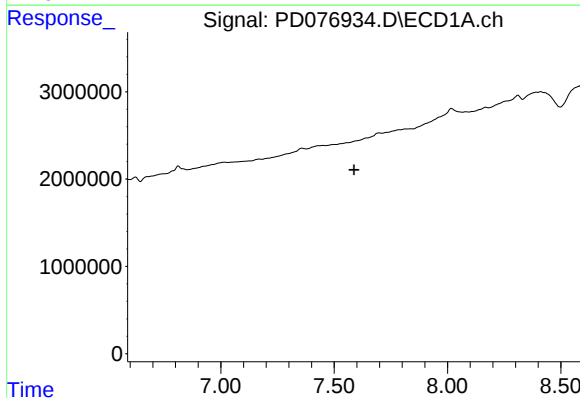


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 7.588 min
Response: 0
Conc: N.D.

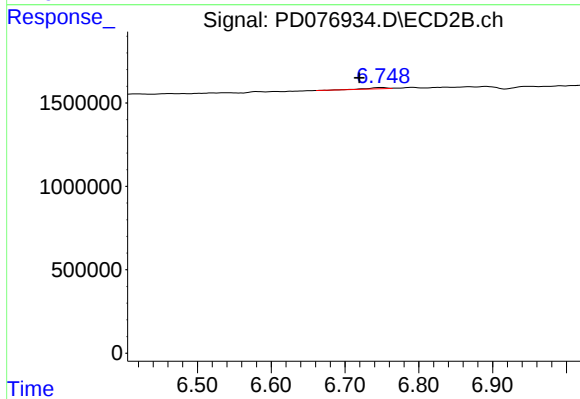

#26 Toxaphene-5

R.T.: 6.749 min
Delta R.T.: 0.030 min
Response: 139689
Conc: 3.77 ng/ml

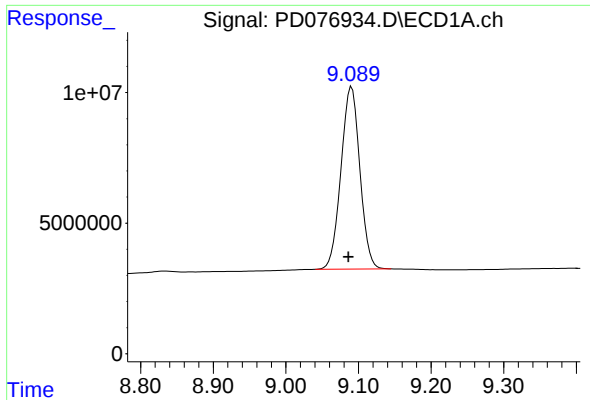

#27 Decachlorobiphenyl


R.T.: 9.091 min

Delta R.T.: 0.005 min

Response: 126305937

Conc: 51.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

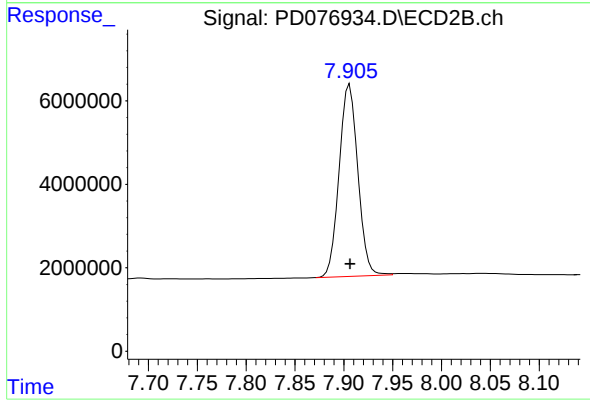

#27 Decachlorobiphenyl

R.T.: 7.906 min

Delta R.T.: 0.000 min

Response: 61409130

Conc: 57.29 ng/ml