

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072123\
 Data File : PD076937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2023 09:24
 Operator : AR\AJ
 Sample : 03534-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A4737DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/24/2023
 Supervised By : Ankita Jodhani 07/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 21:16:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.763	22487721	3573565	10.571	3.348 #
2)	SA Decachlor...	9.088	7.905	15012826	7336484	6.179m	6.844m
Target Compounds							
3)	MA gamma-BHC...	4.340	3.572	141.4E6	18764327	42.634m	12.525m#
7)	B delta-BHC	4.800	4.130	308.1E6	73978948	91.880m	48.469 #
10)	B trans-Chl...	5.973	4.944	60355513	43387013	19.629m	32.085m#
17)	MA 4,4'-DDT	7.012	6.021	37473232	20950854	16.783m	22.365 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072123\
Data File : PD076937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2023 09:24
Operator : AR\AJ
Sample : 03534-19DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 21:16:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

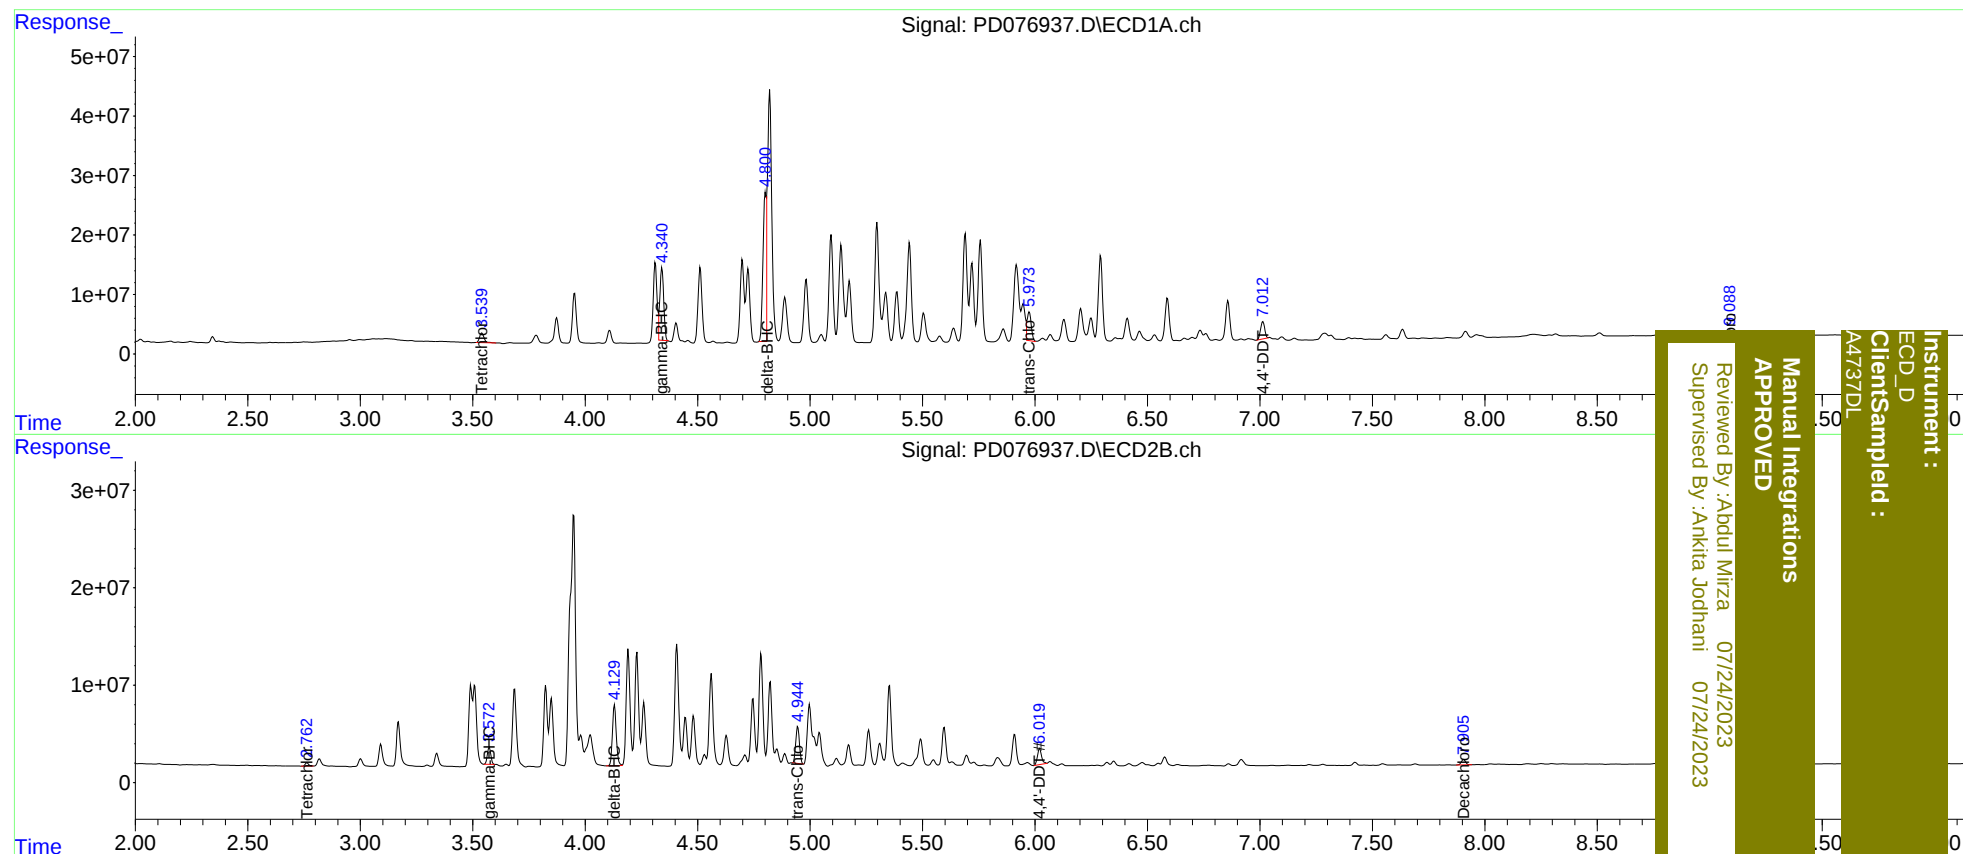

Instrument :
ECD_D
ClientSampled :
A4737DL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/24/2023
Supervised By :Ankita Jodhani 07/24/2023