

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072222\
 Data File : PD071085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2022 14:08
 Operator : AR\AJ
 Sample : N3214-09
 Misc : TOX MDL 50PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 14:34:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 05:25:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.473	4.125	46247913	474.6E6	18.329	18.939
7) SA Decachlor...	8.243	9.322	53864547	206.0E6	20.156	20.590
Target Compounds						
2) Toxaphene-1	5.736	6.154	1301156	1826976	56.827	48.777
3) Toxaphene-2	5.954	6.760	1624878	7130050	44.424	58.981 #
4) Toxaphene-3	6.341	7.442	2548341	11131127	46.999	49.878
5) Toxaphene-4	6.588	7.582	3080711	6026854	53.856	54.127
6) Toxaphene-5	7.076	7.865	4202773	7253078	69.860	48.932 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072222\
Data File : PD071085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 14:08
Operator : AR\AJ
Sample : N3214-09
Misc : TOX MDL 50PPB
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 14:34:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 05:25:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

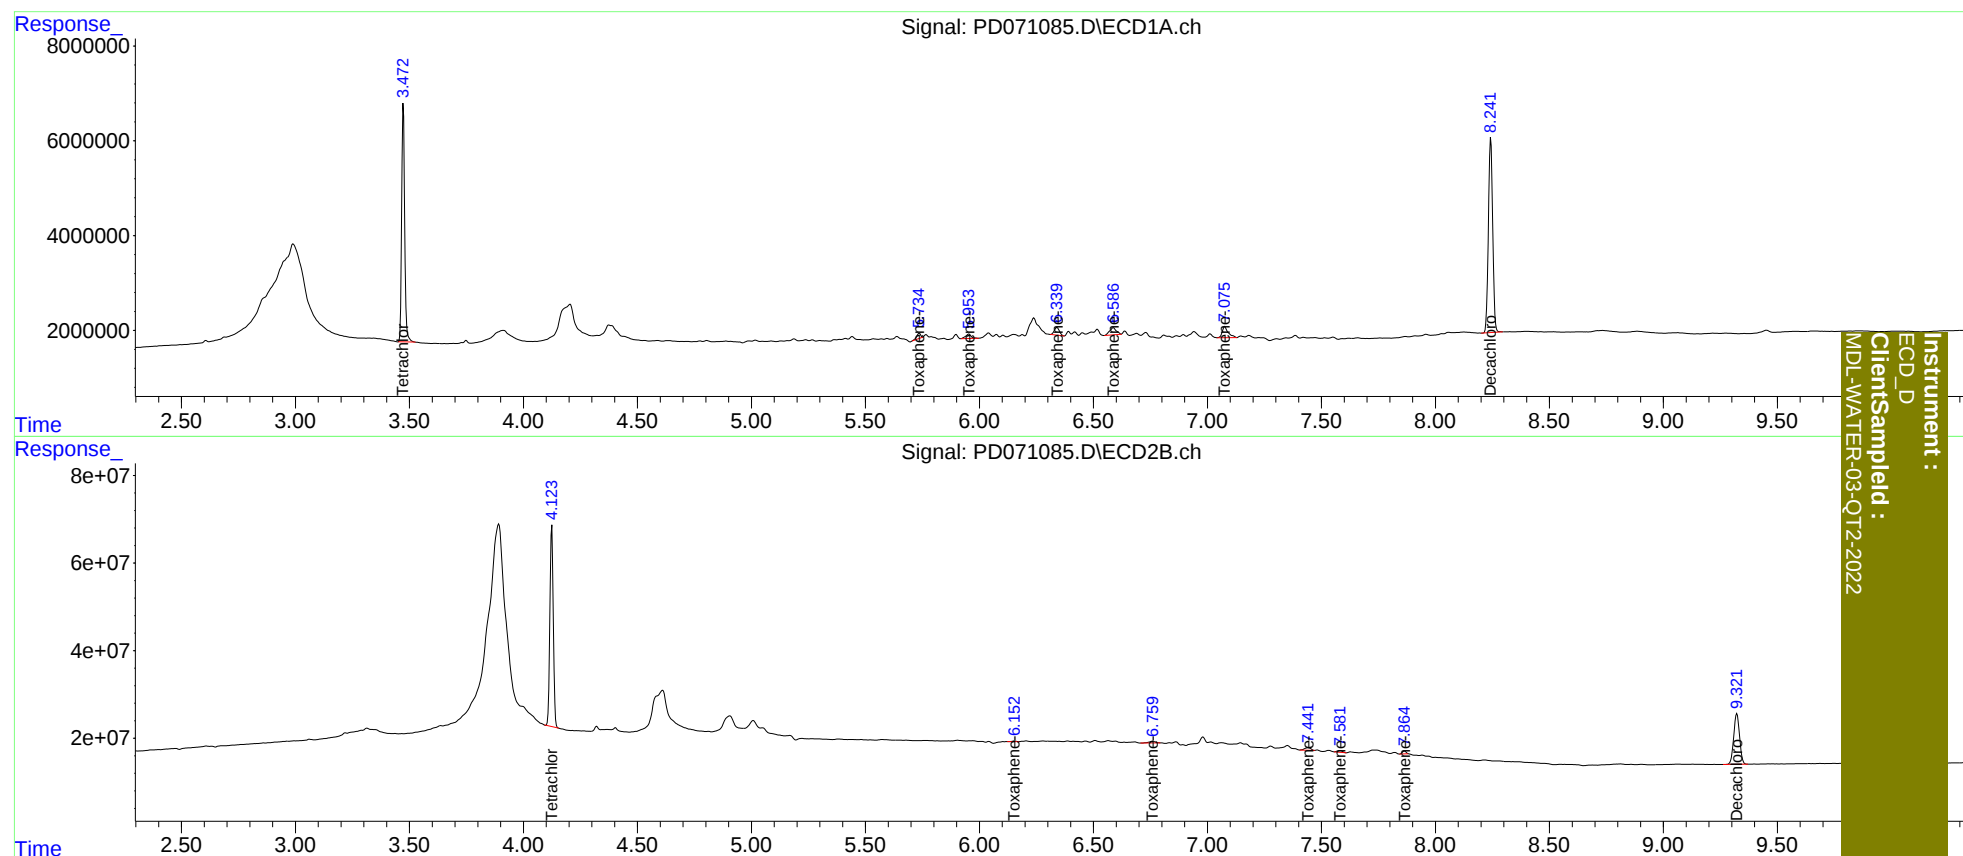


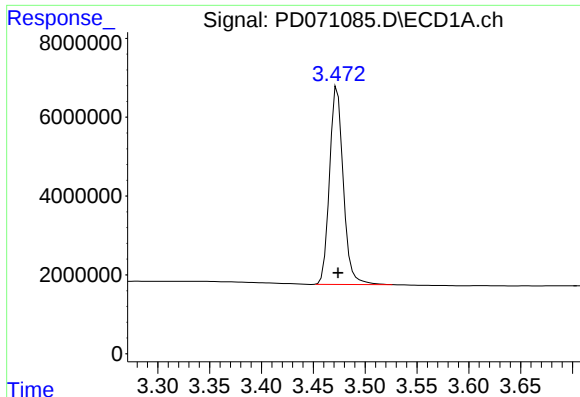

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 46247913
Conc: 18.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT2-2022

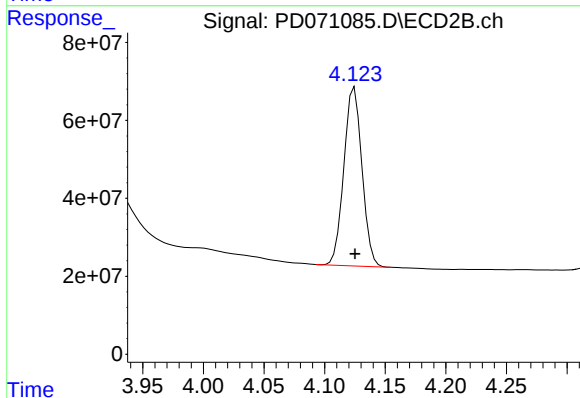


#1 Tetrachloro-m-xylene

R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 474552137
Conc: 18.94 ng/ml

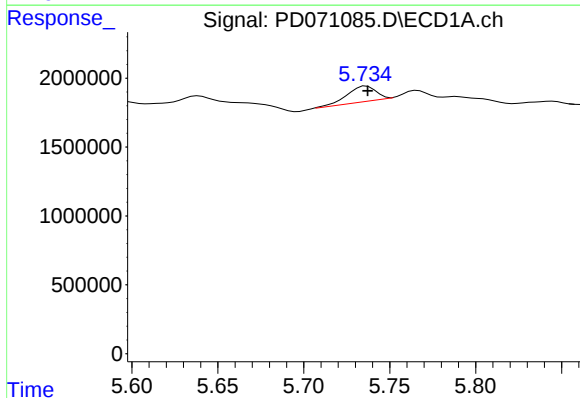


#2 Toxaphene-1

R.T.: 5.736 min
Delta R.T.: 0.000 min
Response: 1301156
Conc: 56.83 ng/ml

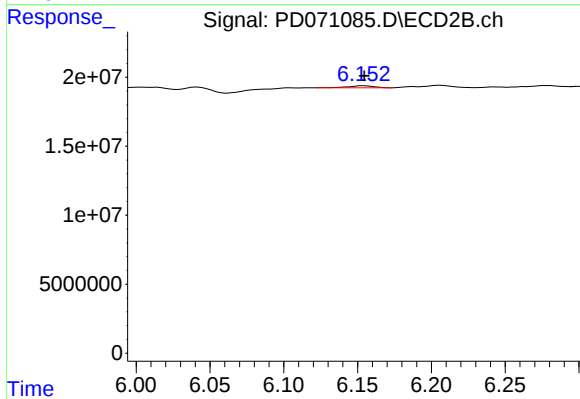

#2 Toxaphene-1


R.T.: 6.154 min
Delta R.T.: 0.000 min
Response: 1826976
Conc: 48.78 ng/ml

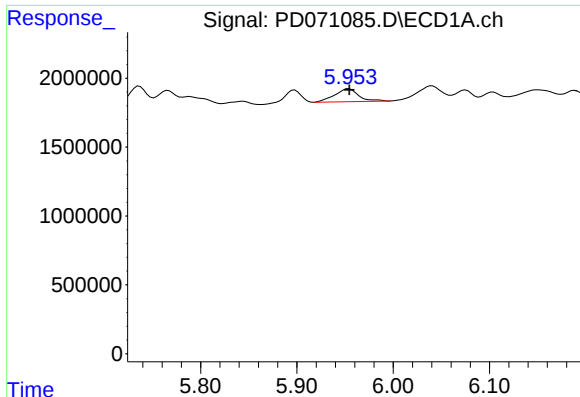

#3 Toxaphene-2


R.T.: 5.954 min
Delta R.T.: 0.000 min
Response: 1624878
Conc: 44.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT2-2022

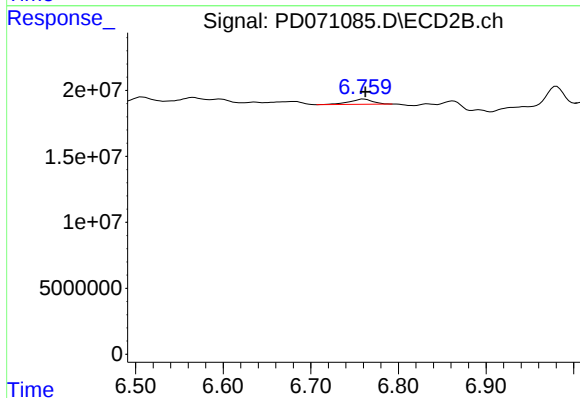


#3 Toxaphene-2

R.T.: 6.760 min
Delta R.T.: -0.002 min
Response: 7130050
Conc: 58.98 ng/ml

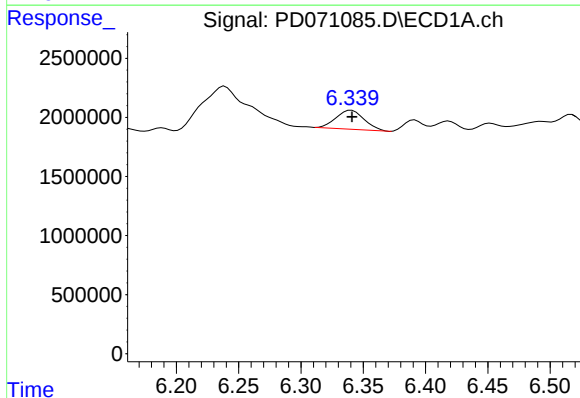


#4 Toxaphene-3

R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 2548341
Conc: 47.00 ng/ml

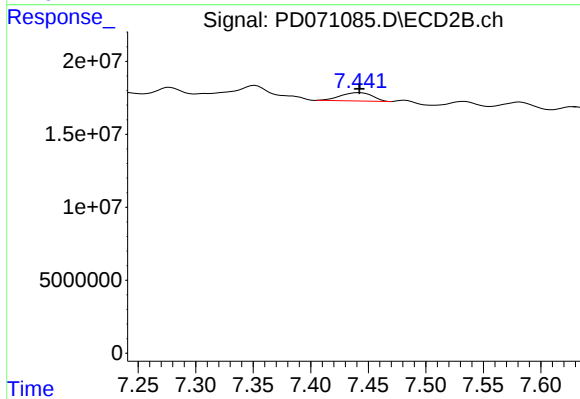

#4 Toxaphene-3


R.T.: 7.442 min
Delta R.T.: 0.000 min
Response: 11131127
Conc: 49.88 ng/ml

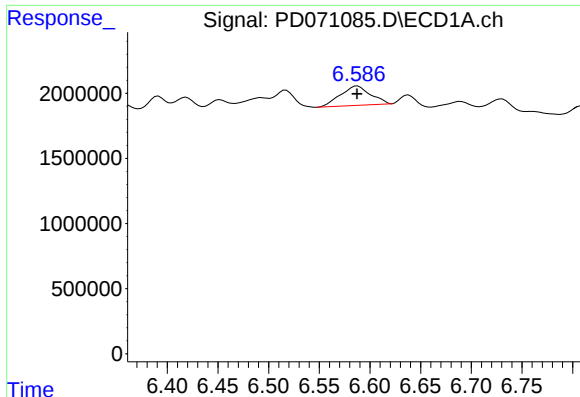

#5 Toxaphene-4


R.T.: 6.588 min
Delta R.T.: 0.000 min
Response: 3080711
Conc: 53.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT2-2022

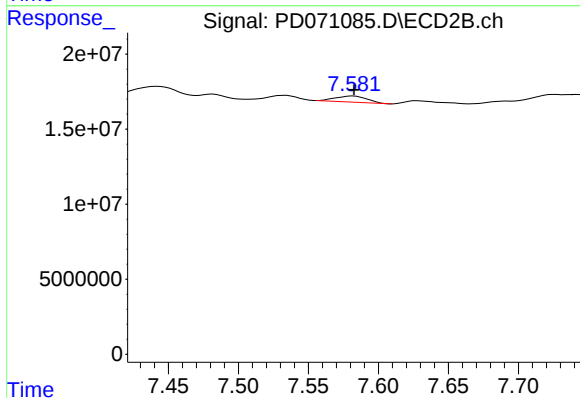


#5 Toxaphene-4

R.T.: 7.582 min
Delta R.T.: 0.000 min
Response: 6026854
Conc: 54.13 ng/ml

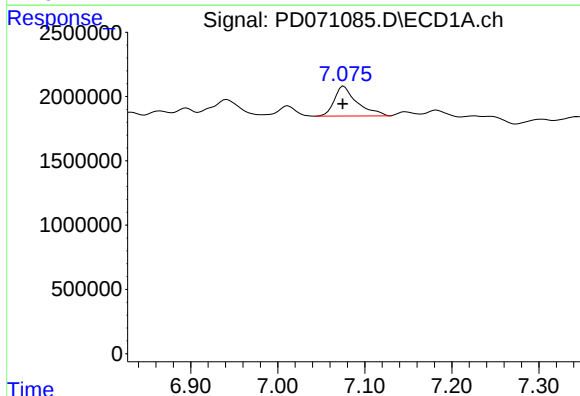


#6 Toxaphene-5

R.T.: 7.076 min
Delta R.T.: 0.002 min
Response: 4202773
Conc: 69.86 ng/ml

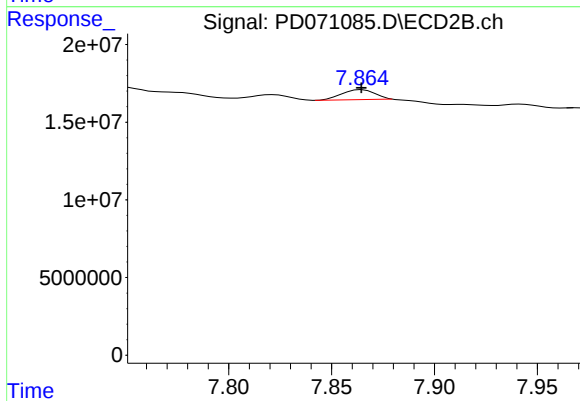

#6 Toxaphene-5


R.T.: 7.865 min
Delta R.T.: 0.000 min
Response: 7253078
Conc: 48.93 ng/ml

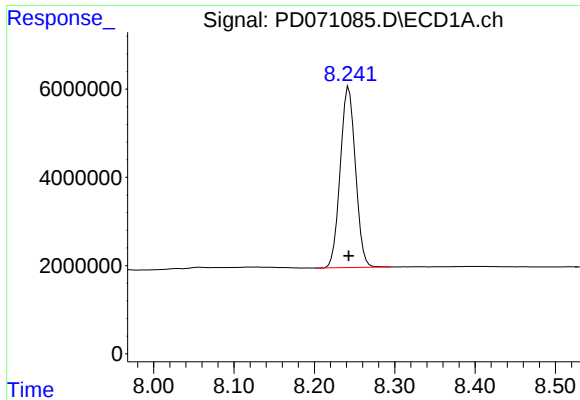

#7 Decachlorobiphenyl

R.T.: 8.243 min
Delta R.T.: 0.000 min
Response: 53864547
Conc: 20.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT2-2022

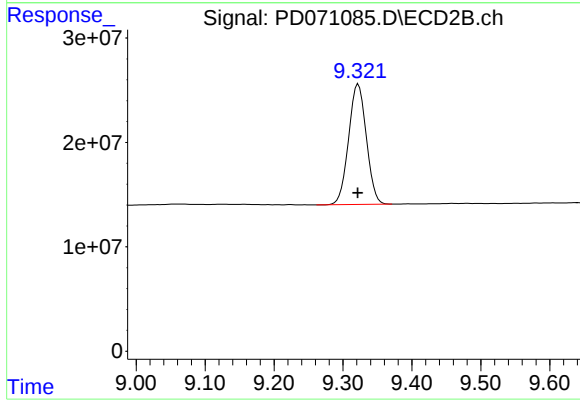

#7 Decachlorobiphenyl

R.T.: 9.322 min
Delta R.T.: 0.001 min
Response: 206005638
Conc: 20.59 ng/ml