

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072222\
 Data File : PD071090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2022 15:58
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 23:51:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 05:30:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.473	4.125	169.7E6	1276.0E6	58.544	44.134
28)	SA Decachlor...	8.243	9.323	144.9E6	531.6E6	47.411	46.608
Target Compounds							
23)	Chlordane-1	4.347	5.146	54491714	416.5E6	505.213	510.321
24)	Chlordane-2	4.849	5.625	65074148	304.8E6	527.892	511.108
25)	Chlordane-3	5.419	6.284	184.7E6	1032.1E6	518.494	522.614
26)	Chlordane-4	5.478	6.358	153.0E6	1197.1E6	518.797	521.912
27)	Chlordane-5	6.316	7.181	66637479	255.7E6	544.224	523.325



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072222\
Data File : PD071090.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 15:58
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 23:51:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 05:30:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

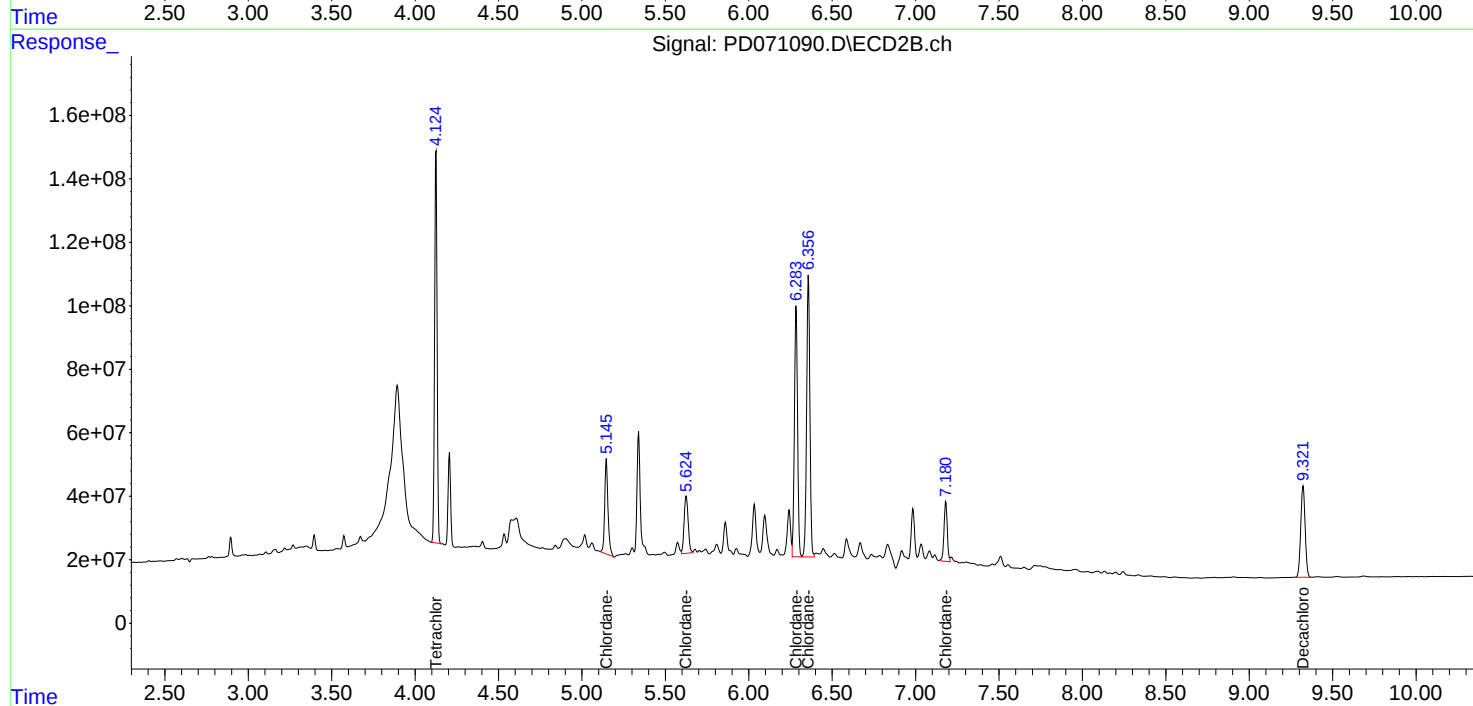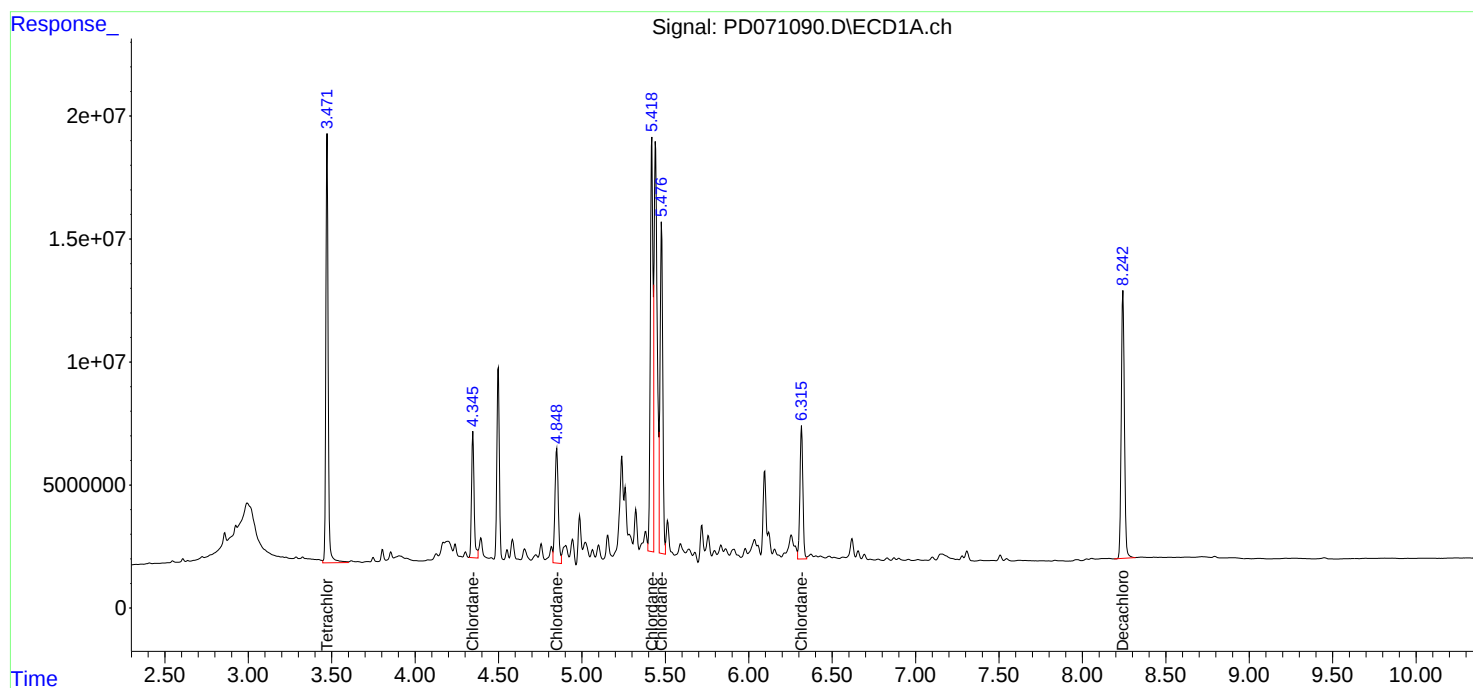


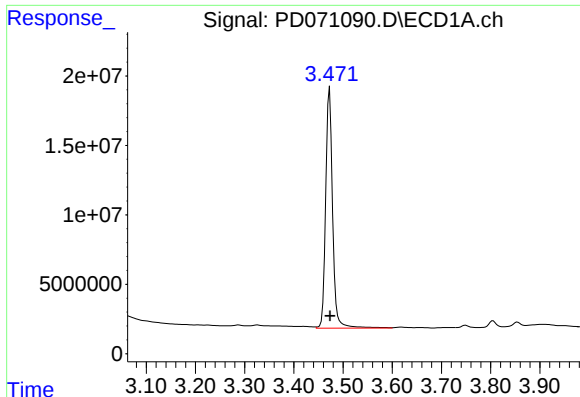

#1 Tetrachloro-m-xylene


R.T.: 3.473 min
Delta R.T.: -0.001 min
Response: 169654556
Conc: 58.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

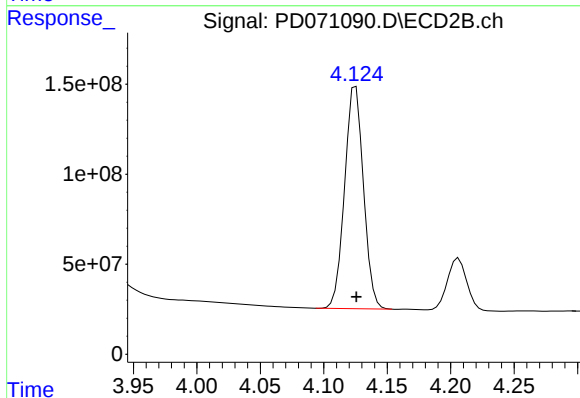


#1 Tetrachloro-m-xylene

R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 1276008855
Conc: 44.13 ng/ml

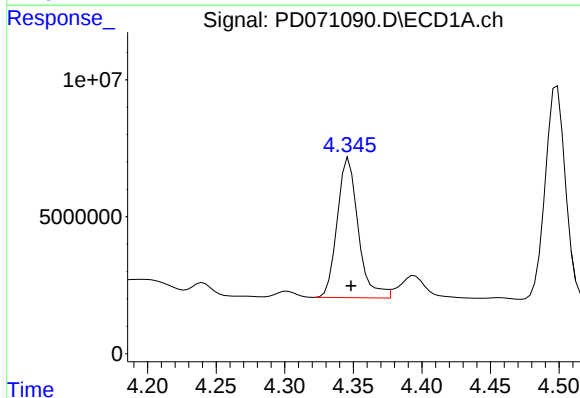


#23 Chlordane-1

R.T.: 4.347 min
Delta R.T.: -0.001 min
Response: 54491714
Conc: 505.21 ng/ml

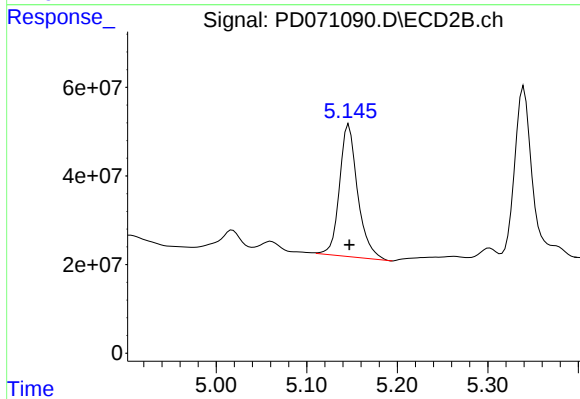

#23 Chlordane-1


R.T.: 5.146 min
Delta R.T.: 0.000 min
Response: 416532500
Conc: 510.32 ng/ml

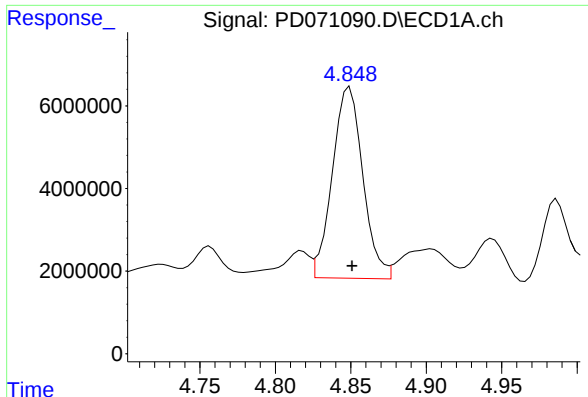

#24 Chlordane-2


R.T.: 4.849 min
Delta R.T.: -0.002 min
Response: 65074148
Conc: 527.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

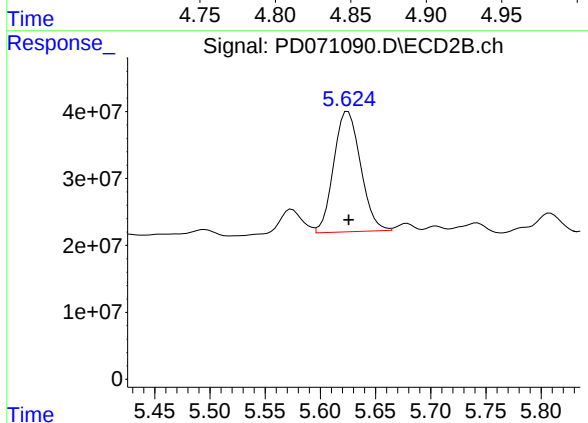


#24 Chlordane-2

R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 304813301
Conc: 511.11 ng/ml

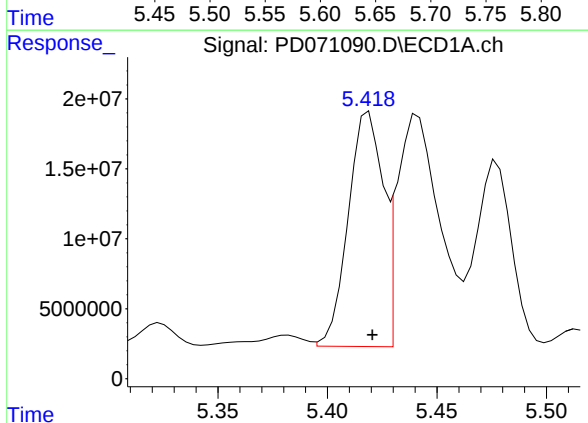


#25 Chlordane-3

R.T.: 5.419 min
Delta R.T.: -0.002 min
Response: 184661922
Conc: 518.49 ng/ml

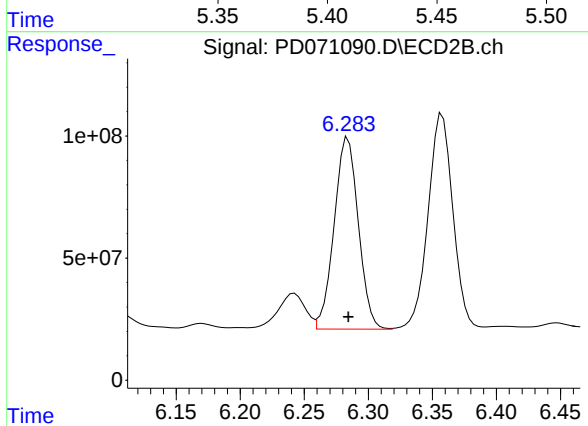

#25 Chlordane-3


R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 1032069731
Conc: 522.61 ng/ml

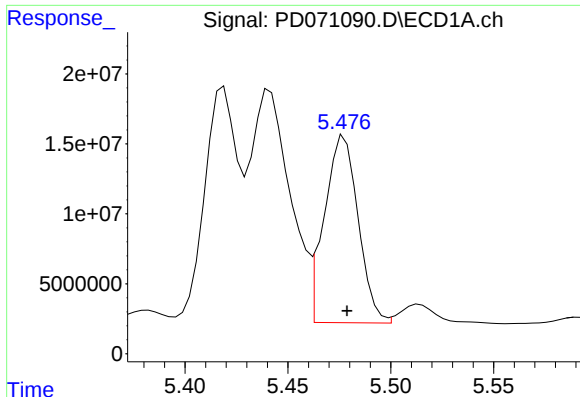

#26 Chlordane-4


R.T.: 5.478 min
Delta R.T.: -0.001 min
Response: 153004169
Conc: 518.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

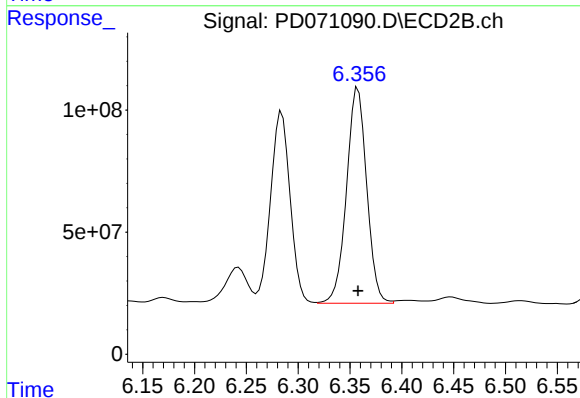


#26 Chlordane-4

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 1197131810
Conc: 521.91 ng/ml

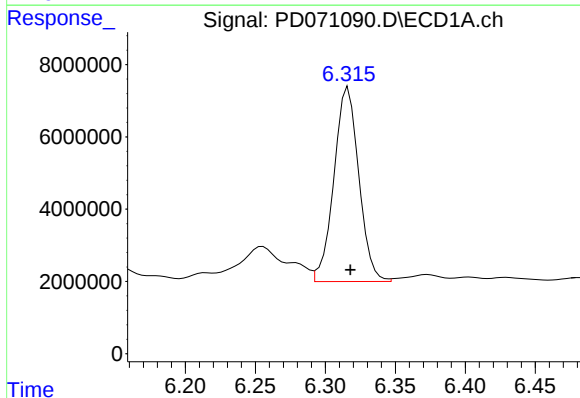


#27 Chlordane-5

R.T.: 6.316 min
Delta R.T.: -0.002 min
Response: 66637479
Conc: 544.22 ng/ml

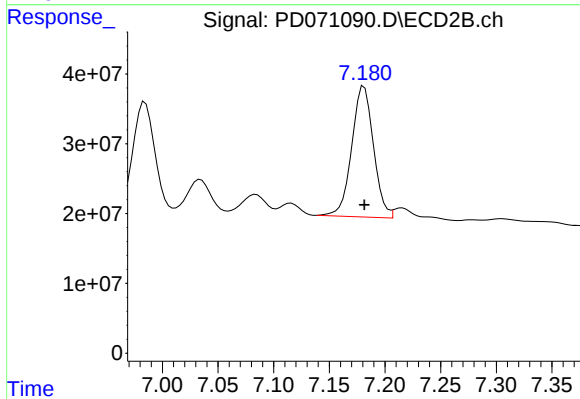

#27 Chlordane-5


R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 255703881
Conc: 523.32 ng/ml

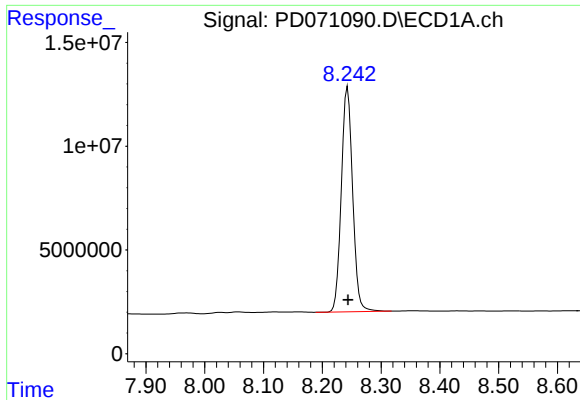

#28 Decachlorobiphenyl

R.T.: 8.243 min
Delta R.T.: 0.000 min
Response: 144855088
Conc: 47.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

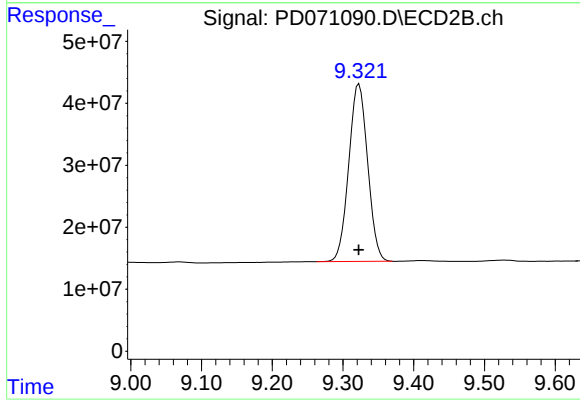

#28 Decachlorobiphenyl

R.T.: 9.323 min
Delta R.T.: 0.000 min
Response: 531566107
Conc: 46.61 ng/ml