

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072222\
 Data File : PD071094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2022 17:54
 Operator : AR\AJ
 Sample : N3786-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 0718-WC-TP-12EA

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/22/2022
 Supervised By : Ankita Jodhani 07/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 23:52:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 05:30:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.472	4.125	27773518	303.3E6	9.584m	10.491
2) SA Decachlor...	8.244	9.324	33398484	131.9E6	10.931	11.566

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072222\
Data File : PD071094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 17:54
Operator : AR\AJ
Sample : N3786-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
0718-WC-TP-12EA


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/22/2022
Supervised By :Ankita Jodhani 07/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 23:52:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 05:30:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

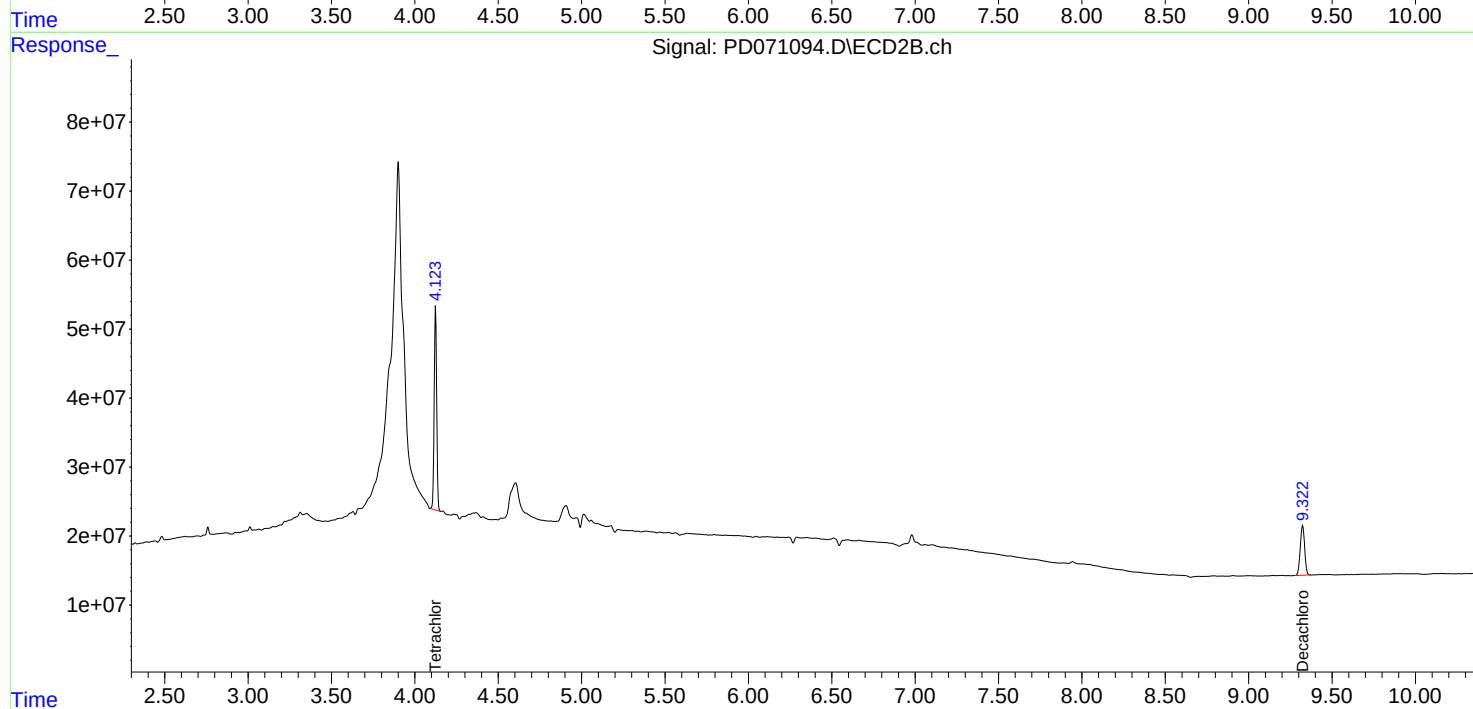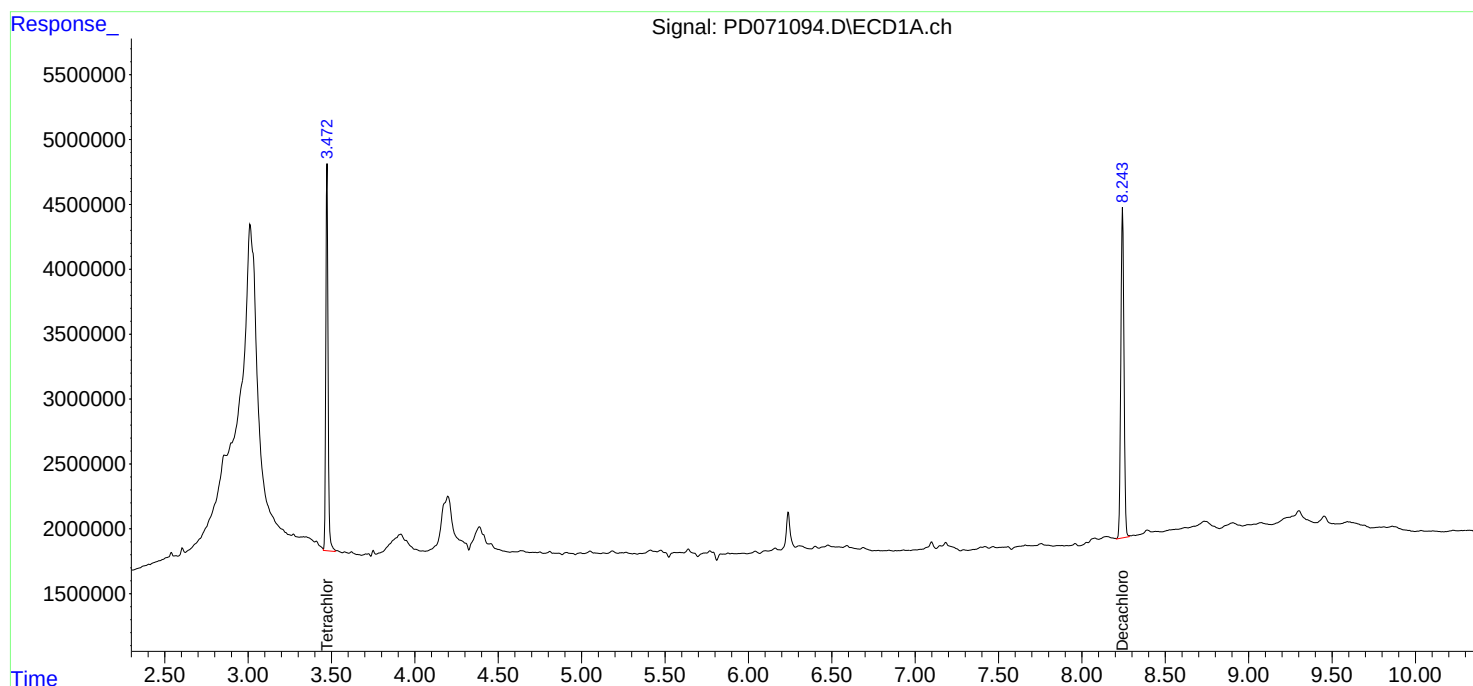

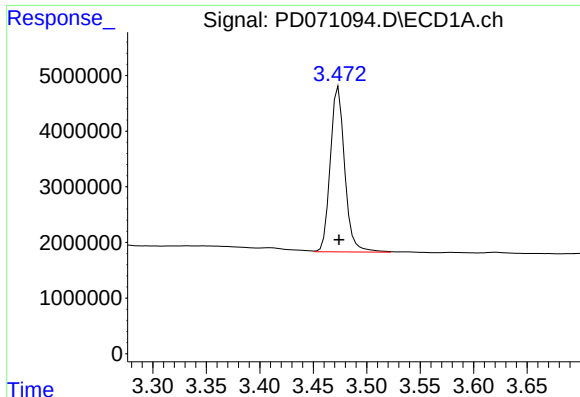


#1 Tetrachloro-m-xylene

R.T.: 3.472 min
Delta R.T.: -0.002 min
Response: 27773518
Conc: 9.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
0718-WC-TP-12EA


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/22/2022
Supervised By :Ankita Jodhani 07/22/2022

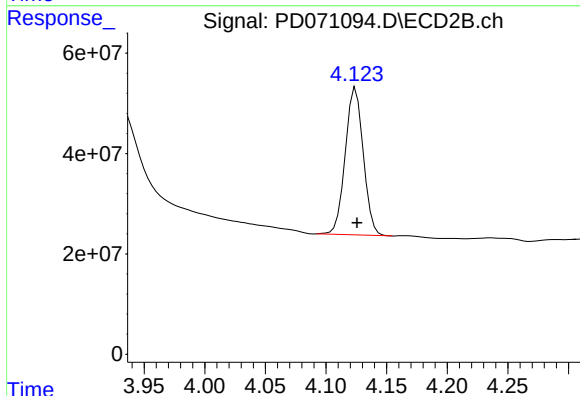


#1 Tetrachloro-m-xylene

R.T.: 4.125 min
Delta R.T.: -0.001 min
Response: 303317312
Conc: 10.49 ng/ml

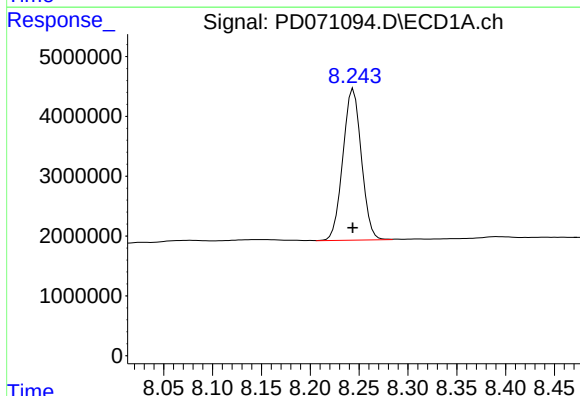

#28 Decachlorobiphenyl

R.T.: 8.244 min
Delta R.T.: 0.000 min
Response: 33398484
Conc: 10.93 ng/ml

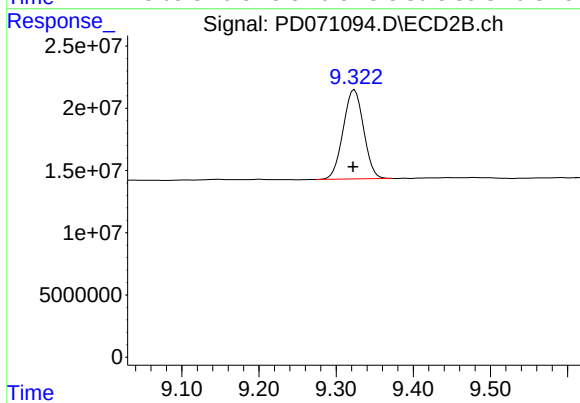

#28 Decachlorobiphenyl

R.T.: 9.324 min
Delta R.T.: 0.002 min
Response: 131904871
Conc: 11.57 ng/ml