

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072222\
 Data File : PD071103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2022 21:19
 Operator : AR\AJ
 Sample : N3786-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 0718-WC-TP-WC3EB

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/22/2022
 Supervised By :Ankita Jodhani 07/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 23:56:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 20 05:30:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.471	4.124	47223691	488.3E6	16.296m	16.889
2) SA Decachlor...	8.242	9.321	44097507	177.5E6	14.433	15.568

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072222\
Data File : PD071103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 21:19
Operator : AR\AJ
Sample : N3786-09
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
0718-WC-TP-WC3EB


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/22/2022
Supervised By : Ankita Jodhani 07/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 23:56:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071922.M
Quant Title : GC Extractables
QLast Update : Wed Jul 20 05:30:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

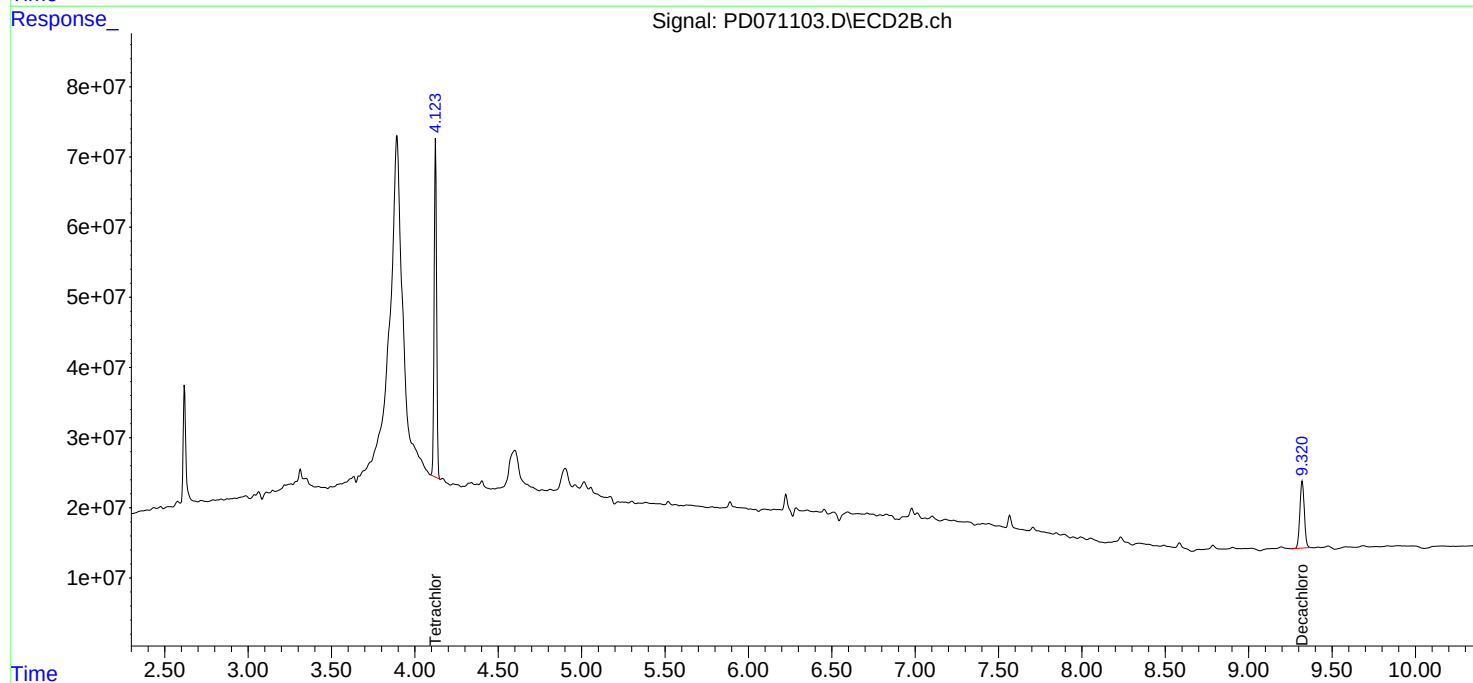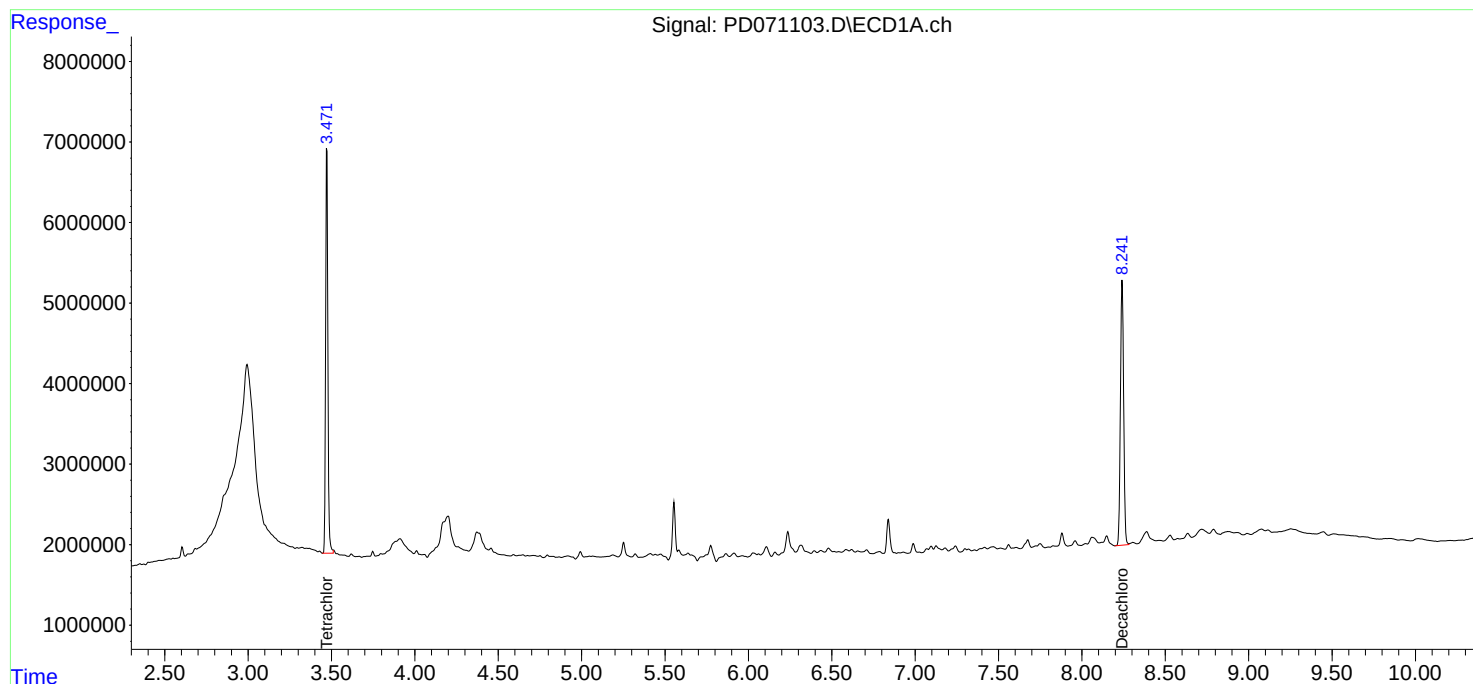

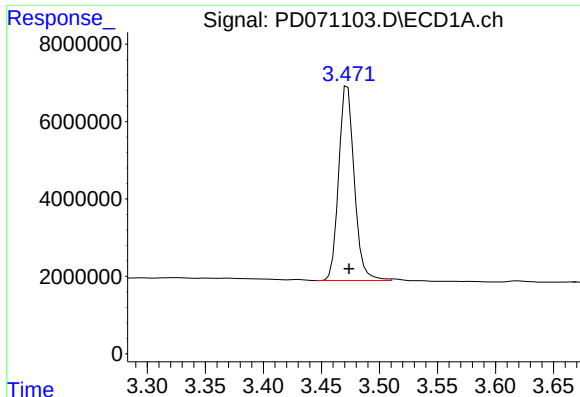


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: -0.003 min
Response: 47223691
Conc: 16.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
0718-WC-TP-WC3EB


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/22/2022
Supervised By :Ankita Jodhani 07/22/2022

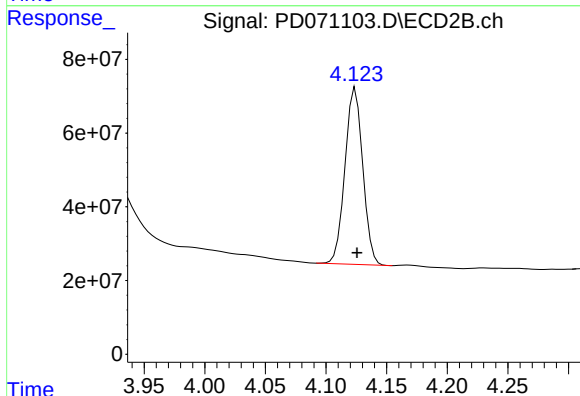


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: -0.001 min
Response: 488287179
Conc: 16.89 ng/ml

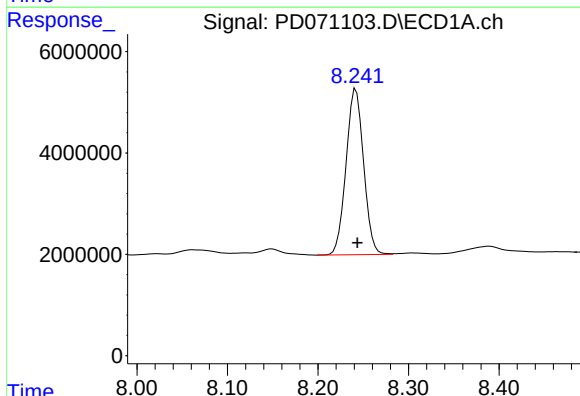

#28 Decachlorobiphenyl

R.T.: 8.242 min
Delta R.T.: -0.002 min
Response: 44097507
Conc: 14.43 ng/ml

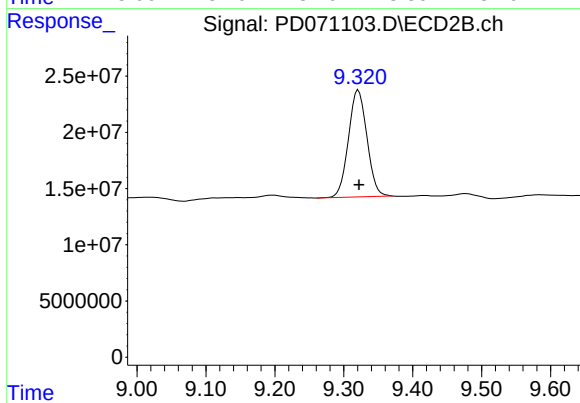

#28 Decachlorobiphenyl

R.T.: 9.321 min
Delta R.T.: 0.000 min
Response: 177546678
Conc: 15.57 ng/ml