

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072224\
 Data File : PD084021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2024 10:44
 Operator : AR\AJ
 Sample : P3287-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 XB501

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/24/2024
 Supervised By :Ankita Jodhani 07/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:24:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.791	17561123	98128570	17.297	18.106
27)	SA Decachlor...	9.128	7.917	35030030	105.0E6	16.440	15.722m
Target Compounds							
2)	A alpha-BHC	4.028	3.289	1300.9E6	3919.9E6	687.640	434.827m#
3)	MA gamma-BHC...	4.362	3.618	1558.5E6	4947.7E6	844.485m	577.959m#
4)	MA Heptachlor	4.954	3.956	757.1E6	2432.7E6	377.670m	288.912m
5)	MB Aldrin	5.299	4.236	885.1E6	2433.1E6	435.737	288.399 #
6)	B beta-BHC	4.560	3.915	682.4E6	2555.5E6	812.465	674.031m
7)	B delta-BHC	4.810	4.144	463.0E6	1668.9E6	218.401	182.834m
8)	B Heptachlo...	5.725	4.737	399.1E6	1329.3E6	204.992m	169.252m
9)	A Endosulfan I	6.112	5.107	582.2E6	1647.7E6	314.360m	237.122m
10)	B trans-Chl...	5.984	4.988	2068.0E6	5707.6E6	1086.115	738.677 #
11)	B cis-Chlor...	6.061	5.051	2043.7E6	5679.1E6	1044.060m	721.506m#
12)	B 4,4'-DDE	6.234	5.239	2262.7E6	5987.6E6	1142.309m	799.710m#
13)	MA Dieldrin	6.390	5.372	1101.9E6	3015.6E6	550.284	389.516 #
14)	MA Endrin	6.621	5.648	336.2E6	1085.9E6	203.289	163.968
15)	B Endosulfa...	6.839	5.940	309.1E6	928.0E6	169.571m	139.072m
16)	A 4,4'-DDD	6.753	5.793	1749.2E6	4327.2E6	1212.415m	726.344m#
17)	MA 4,4'-DDT	7.069	6.044	1780.3E6	4318.4E6	1177.331	738.665 #
18)	B Endrin al...	6.971	6.120	567.5E6	1587.6E6	414.961	316.534
19)	B Endosulfa...	7.205	6.341	1003.1E6	2632.3E6	565.995m	405.184m#
20)	A Methoxychlor	7.546	6.619	693.0E6	1546.7E6	778.926	523.463 #
21)	B Endrin ke...	7.693	6.847	1665.5E6	3977.4E6	853.057	566.197m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072224\
Data File : PD084021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2024 10:44
Operator : AR\AJ
Sample : P3287-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 01:24:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

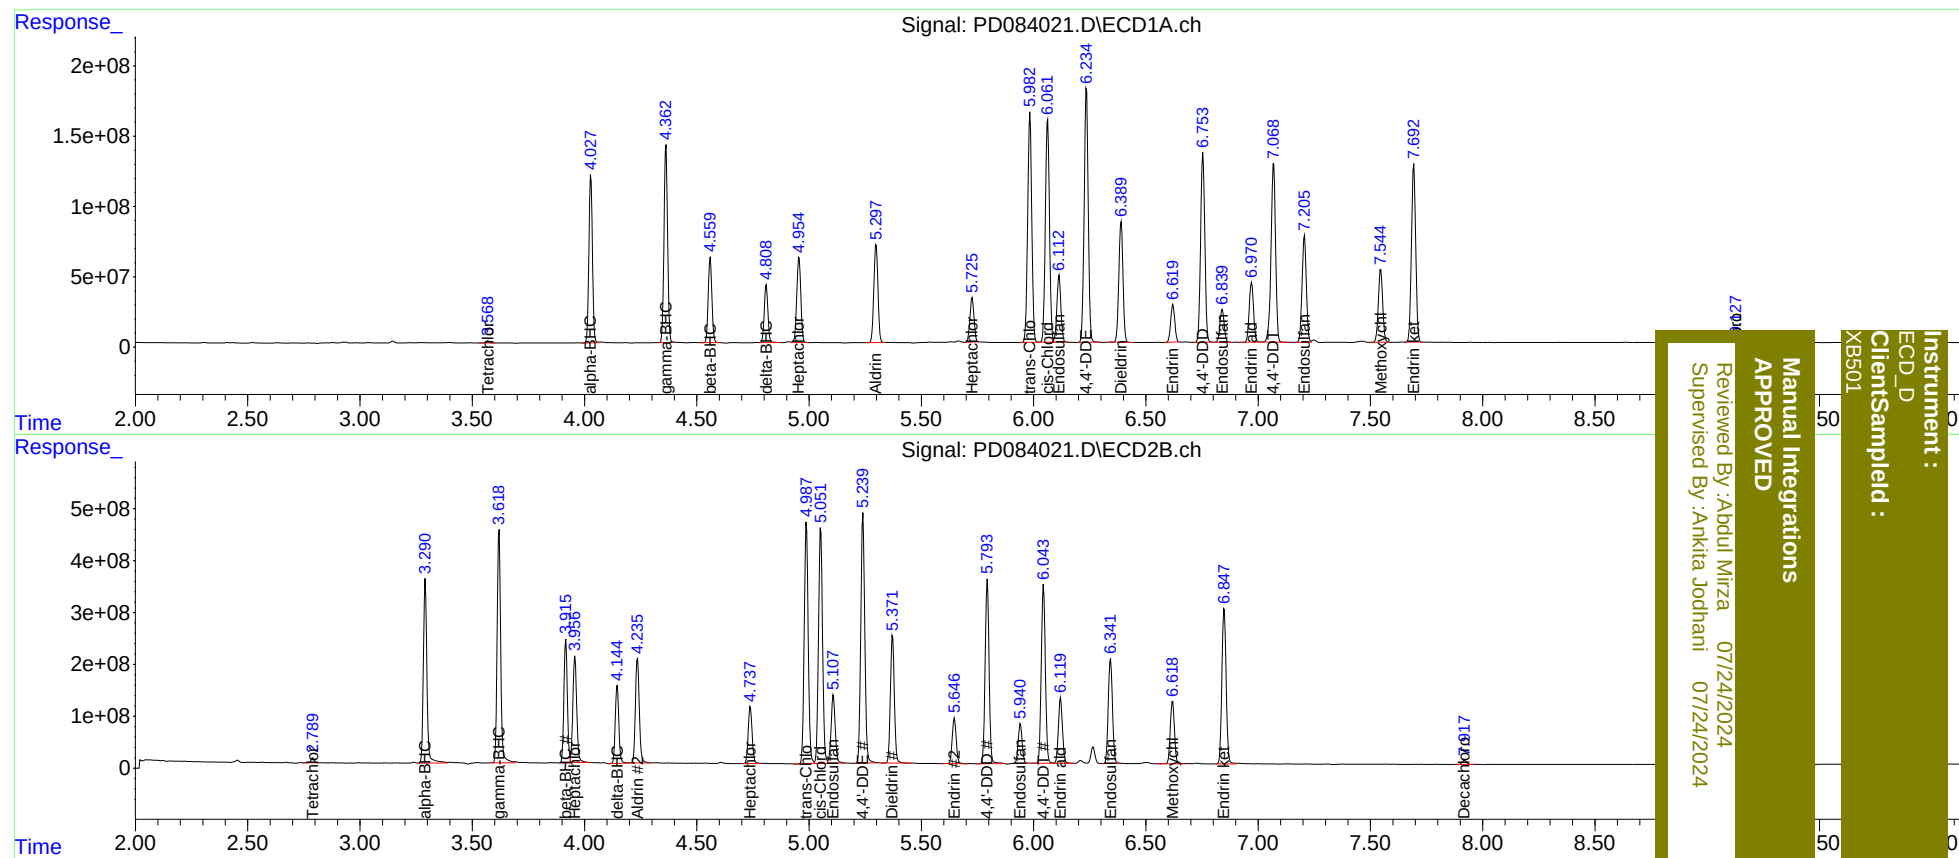

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 07/24/2024
Supervised By: Ankita Jodhani 07/24/2024

Instrument :
ECD_D
Client Sampled :
XB501