

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072224\
 Data File : PD084023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2024 11:10
 Operator : AR\AJ
 Sample : P3287-02DL2 20X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 XB501DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/24/2024
 Supervised By : Ankita Jodhani 07/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:27:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.769	899054	7035483	0.886m	1.298m#
2)	SA Decachlor...	9.117	7.896	2081705	6491069	0.977	0.972m
Target Compounds							
2)	A alpha-BHC	4.019	3.270	54647883	266.8E6	28.886	29.593
3)	MA gamma-BHC...	4.353	3.599	66771696	309.6E6	36.180	36.161
4)	MA Heptachlor	4.945	3.936	36095923	152.5E6	18.006	18.112
5)	MB Aldrin	5.289	4.215	41320203	169.5E6	20.342	20.088
6)	B beta-BHC	4.550	3.896	36178900	164.9E6	43.072	43.487
7)	B delta-BHC	4.799	4.123	23169843	99091759	10.931	10.856m
8)	B Heptachlo...	5.715	4.716	21227296	84407496	10.903m	10.747
9)	A Endosulfan I	6.103	5.086	31032748	114.3E6	16.755m	16.445
10)	B trans-Chl...	5.974	4.966	97899565	371.1E6	51.417	48.025
11)	B cis-Chlor...	6.052	5.030	99076888	371.4E6	50.616m	47.190
12)	B 4,4'-DDE	6.226	5.218	108.5E6	391.7E6	54.790	52.317
13)	MA Dieldrin	6.380	5.350	52259662	194.9E6	26.099	25.180
14)	MA Endrin	6.612	5.625	16828244	65424757	10.175	9.879
15)	B Endosulfa...	6.831	5.919	16236089	58517196	8.906	8.770
16)	A 4,4'-DDD	6.745	5.770	80206547	302.0E6	55.593	50.692m
17)	MA 4,4'-DDT	7.059	6.023	77685444	258.8E6	51.374	44.266
18)	B Endrin al...	6.962	6.099	30392077	107.1E6	22.223	21.362
19)	B Endosulfa...	7.196	6.320	51858023	181.1E6	29.261m	27.883m
20)	A Methoxychlor	7.537	6.597	38714760	116.8E6	43.514	39.529
21)	B Endrin ke...	7.685	6.826	83722987	293.0E6	42.882	41.712m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072224\
Data File : PD084023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2024 11:10
Operator : AR\AJ
Sample : P3287-02DL2 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 01:27:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

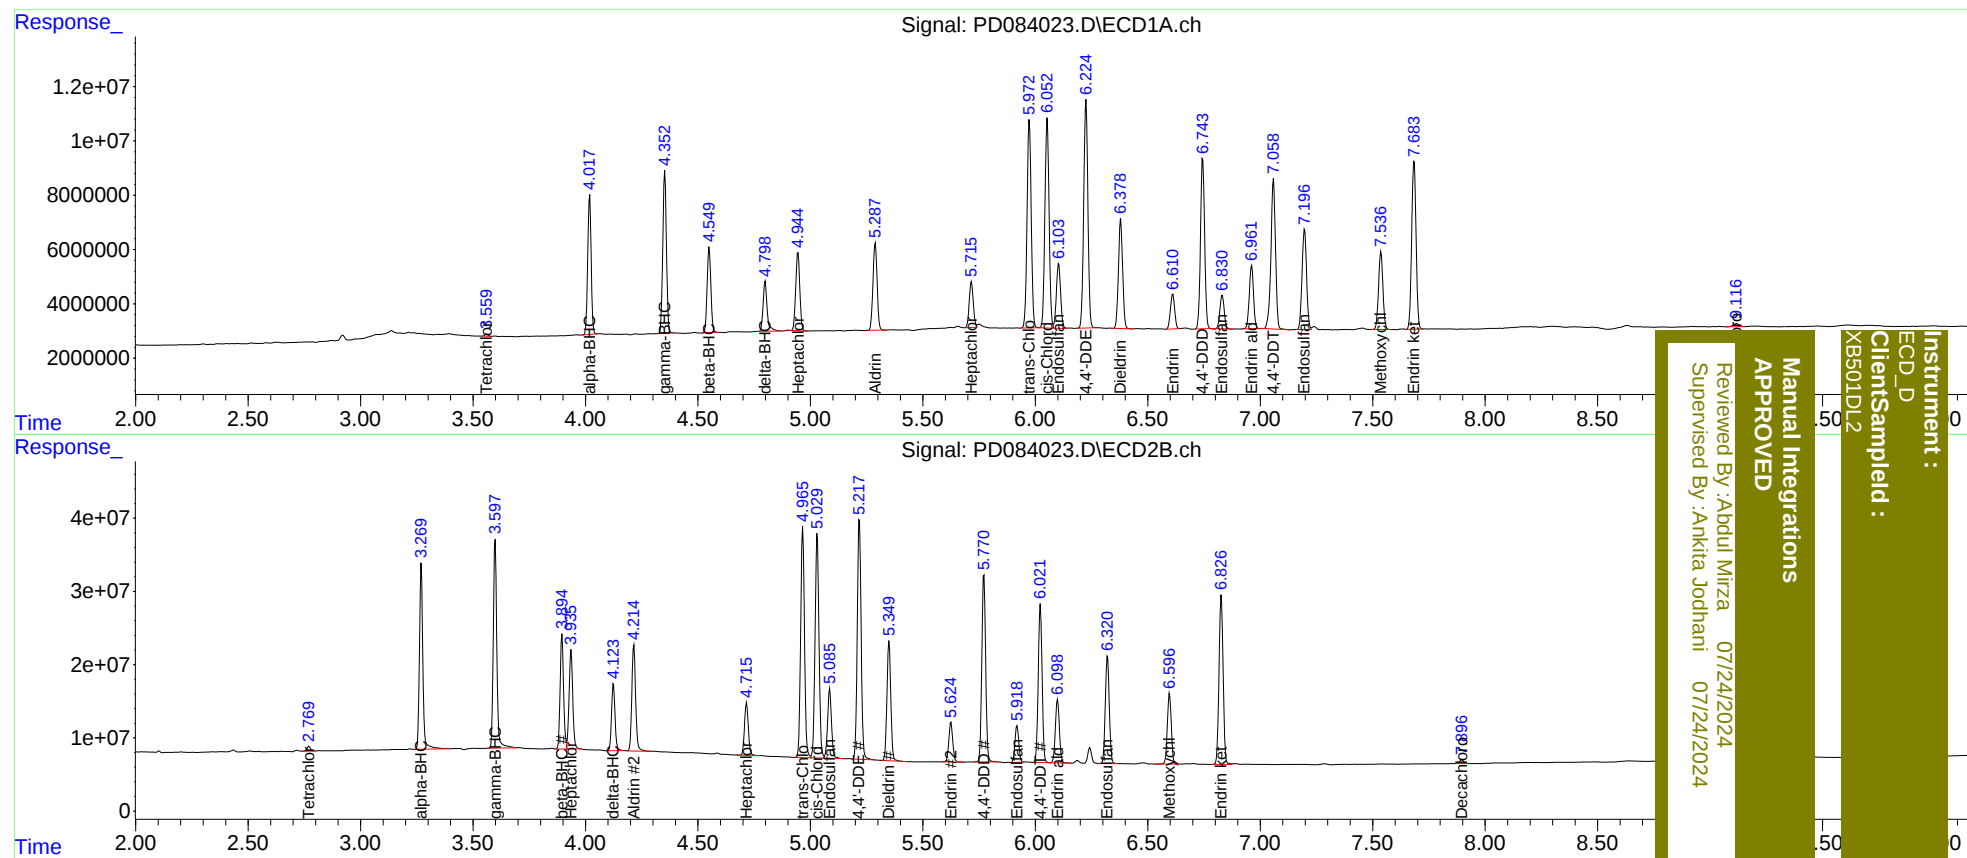

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 07/24/2024
Supervised By: Ankita Jodhani 07/24/2024

Instrument :
ECD_D
Client Sampled :
XB501DL2