

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD072224\  
 Data File : PD084025.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 22 Jul 2024 11:37  
 Operator : AR\AJ  
 Sample : INDA331  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 INDA3220

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 07/23/2024  
 Supervised By : Ankita Jodhani 07/23/2024

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 23 03:12:50 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD062624CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jun 27 04:33:52 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|---------|---------|---------|
| -----                       |                 |       |       |          |         |         |         |
| System Monitoring Compounds |                 |       |       |          |         |         |         |
| 1)                          | SA Tetrachlo... | 3.562 | 2.772 | 20563961 | 114.0E6 | 20.254  | 21.028  |
| 27)                         | SA Decachlor... | 9.117 | 7.897 | 82917107 | 248.6E6 | 38.915  | 37.212  |
| Target Compounds            |                 |       |       |          |         |         |         |
| 2)                          | A alpha-BHC     | 4.019 | 3.271 | 38480526 | 185.1E6 | 20.340  | 20.532  |
| 3)                          | MA gamma-BHC... | 4.353 | 3.599 | 38024834 | 180.2E6 | 20.604  | 21.045  |
| 4)                          | MA Heptachlor   | 4.946 | 3.936 | 41972051 | 167.9E6 | 20.938  | 19.935m |
| 9)                          | A Endosulfan I  | 6.105 | 5.086 | 39362944 | 121.8E6 | 21.253  | 17.527  |
| 13)                         | MA Dieldrin     | 6.381 | 5.349 | 84522821 | 309.7E6 | 42.211  | 39.997m |
| 14)                         | MA Endrin       | 6.612 | 5.625 | 70025386 | 266.4E6 | 42.338  | 40.222  |
| 16)                         | A 4,4'-DDD      | 6.745 | 5.771 | 59906326 | 228.8E6 | 41.522  | 38.404m |
| 17)                         | MA 4,4'-DDT     | 7.060 | 6.023 | 61403006 | 226.0E6 | 40.606  | 38.655  |
| 20)                         | A Methoxychlor  | 7.536 | 6.597 | 176.5E6  | 516.3E6 | 198.329 | 174.739 |
| -----                       |                 |       |       |          |         |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD072224\  
Data File : PD084025.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 22 Jul 2024 11:37  
Operator : AR\AJ  
Sample : INDA331  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 23 03:12:50 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD062624CLP.M  
Quant Title : GC Extractables  
QLast Update : Thu Jun 27 04:33:52 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

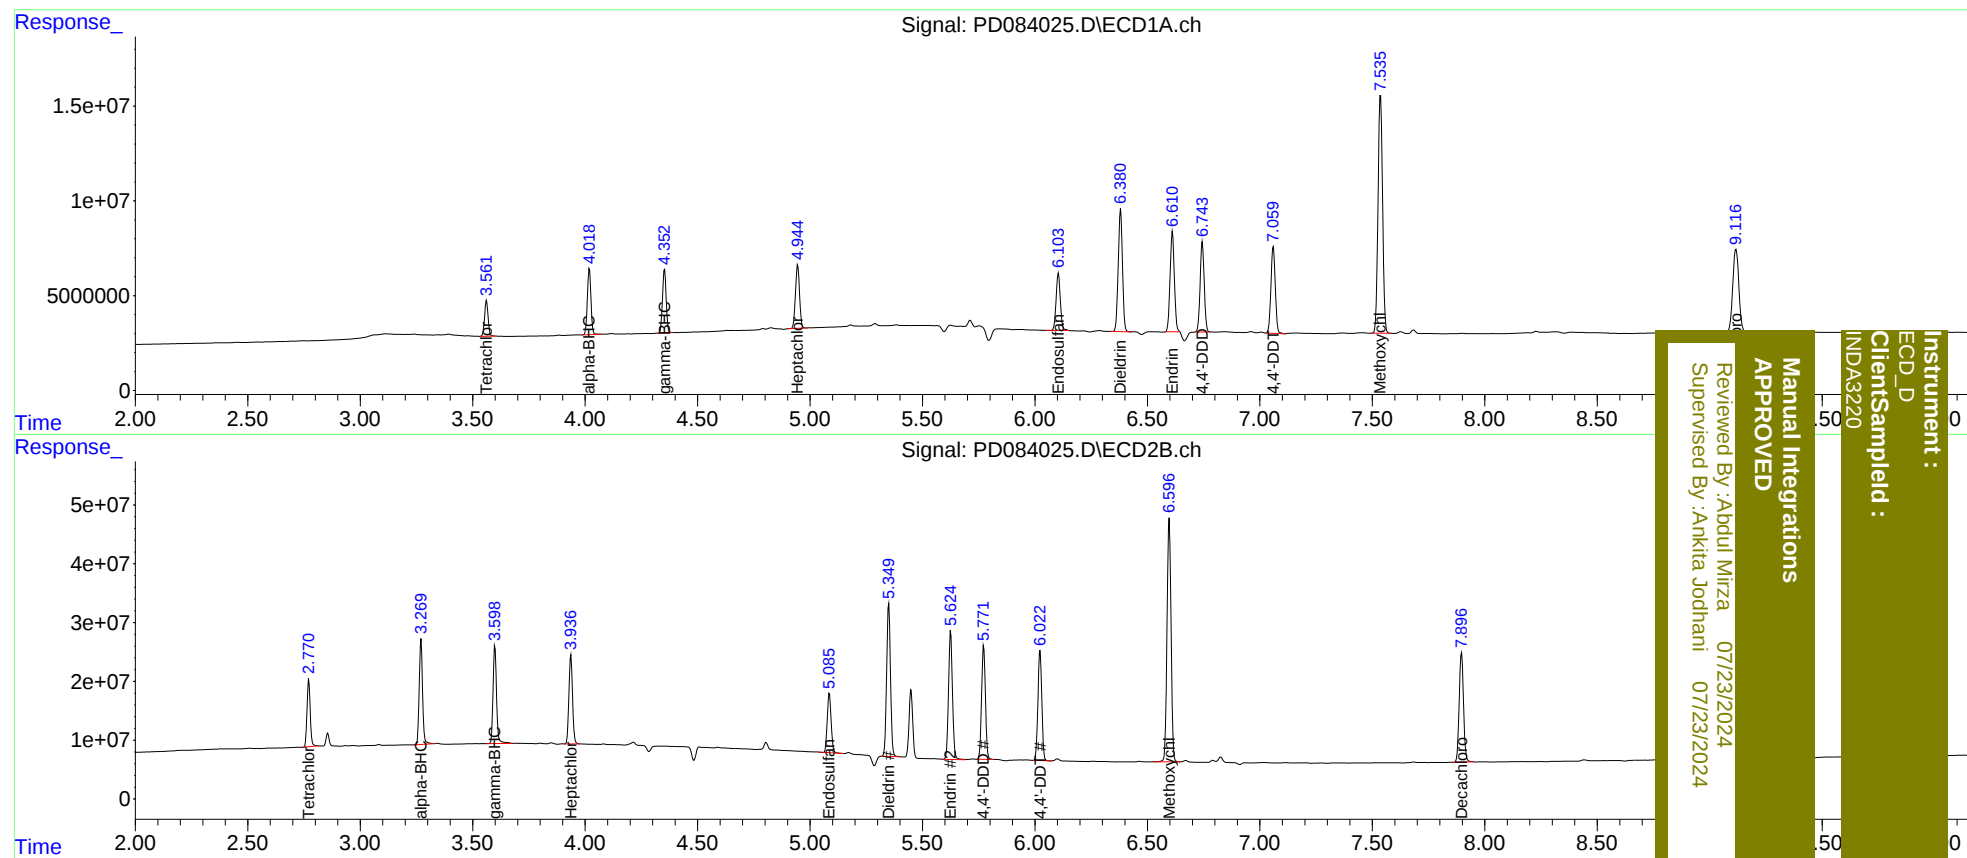

Reviewed By: Abdul Mirza 07/23/2024  
Supervised By: Ankita Jodhani 07/23/2024

Manual Integrations  
APPROVED

Instrument :  
ECD\_D  
ClientSampled :  
INDA3220