

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072324\
 Data File : PD084034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 03:13
 Operator : AR\AJ
 Sample : P3300-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 06:05:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.772	18248114	96090730	17.973	17.730
2)	SA Decachlor...	9.114	7.895	32749890	97964799	15.370	14.663
Target Compounds							
4)	MA Heptachlor	4.932	0.000	2332842	0	1.164	N.D. #
5)	MB Aldrin	0.000	4.237	0	38043596	N.D.	4.509
6)	B beta-BHC	0.000	3.850f	0	210.5E6	N.D.	55.512
7)	B delta-BHC	4.789	0.000	77993610	0	36.794	N.D. #
10)	B trans-Chl...	5.959	0.000	1390900	0	0.731	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD072324\
Data File : PD084034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2024 03:13
Operator : AR\AJ
Sample : P3300-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 06:05:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

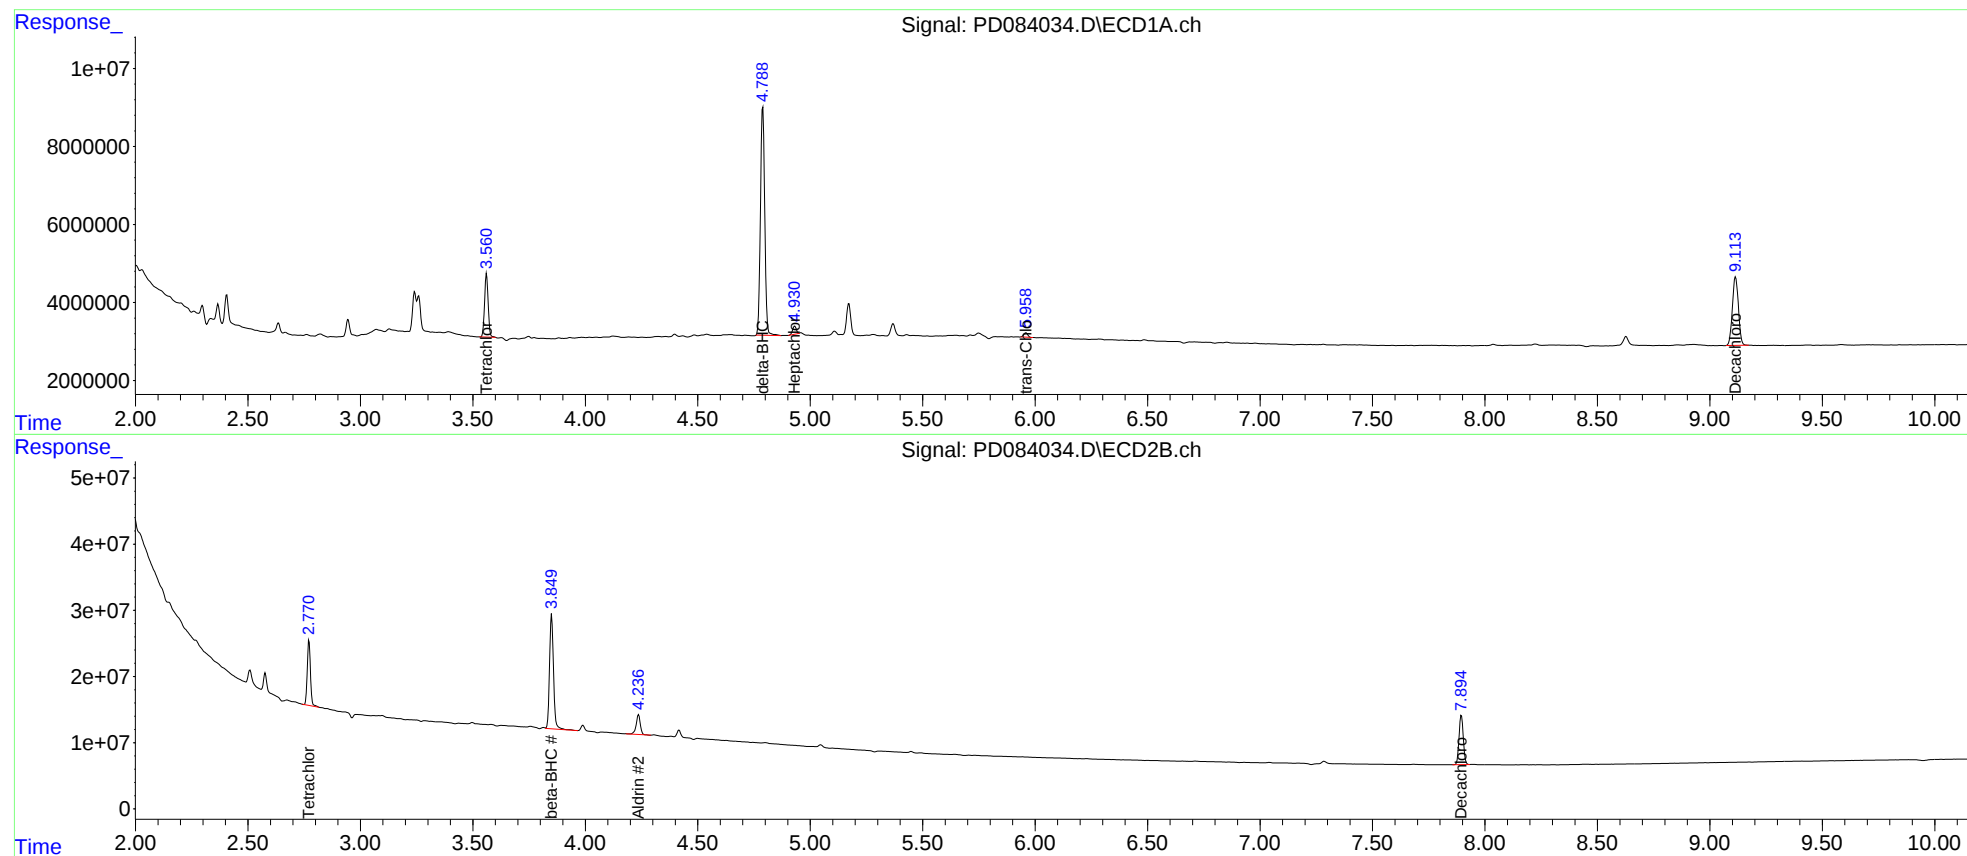

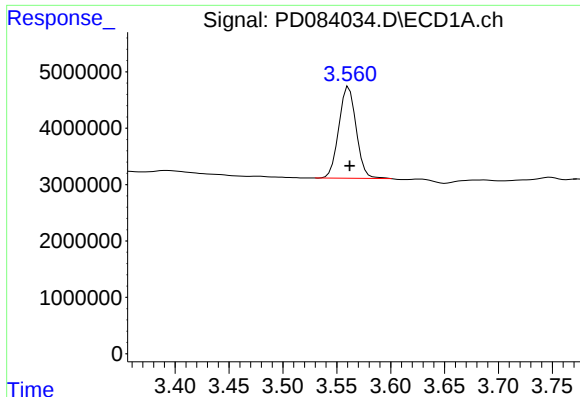


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 18248114
Conc: 17.97 ng/ml

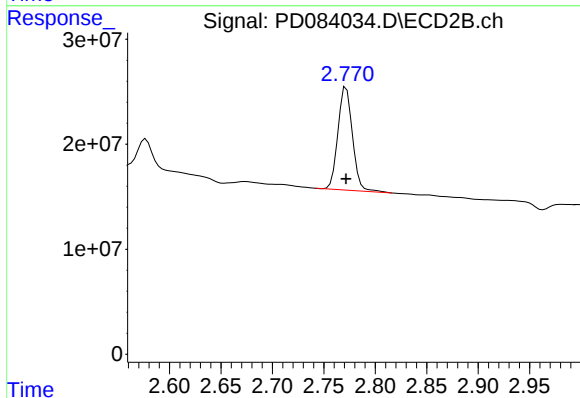


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 96090730
Conc: 17.73 ng/ml

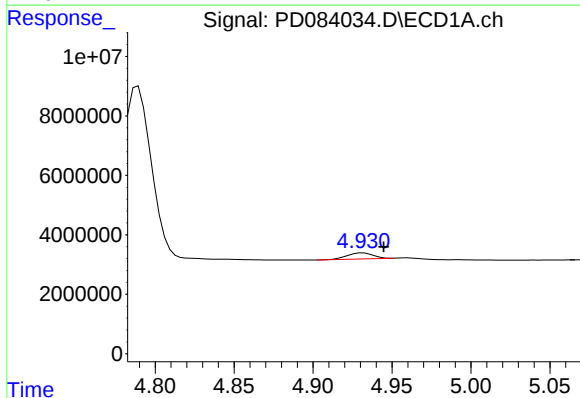


#4 Heptachlor

R.T.: 4.932 min
Delta R.T.: -0.013 min
Response: 2332842
Conc: 1.16 ng/ml

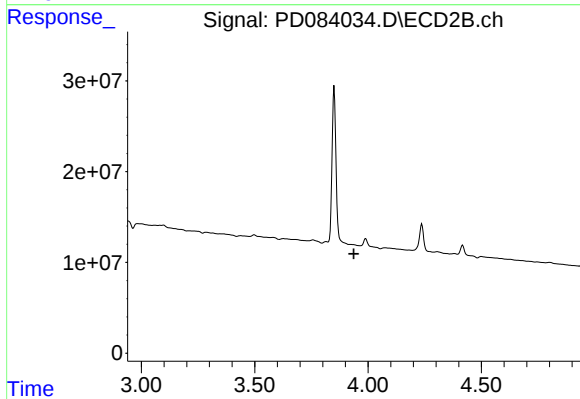


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 3.937 min
Response: 0
Conc: N.D.

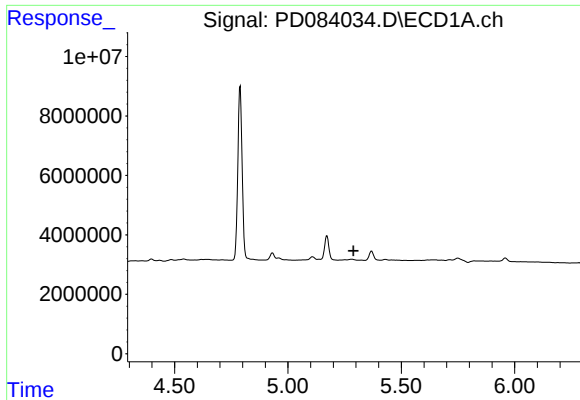


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.290 min
Response: 0
Conc: N.D.

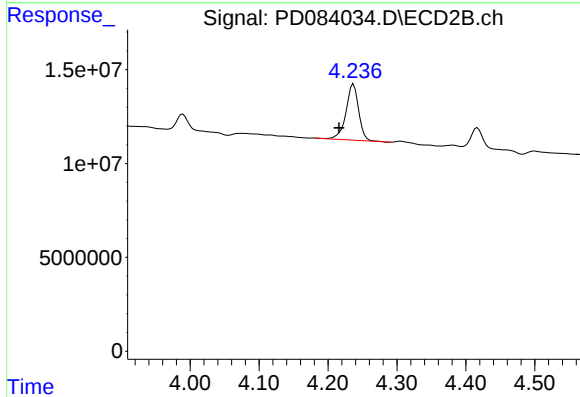


#5 Aldrin

R.T.: 4.237 min
Delta R.T.: 0.021 min
Response: 38043596
Conc: 4.51 ng/ml

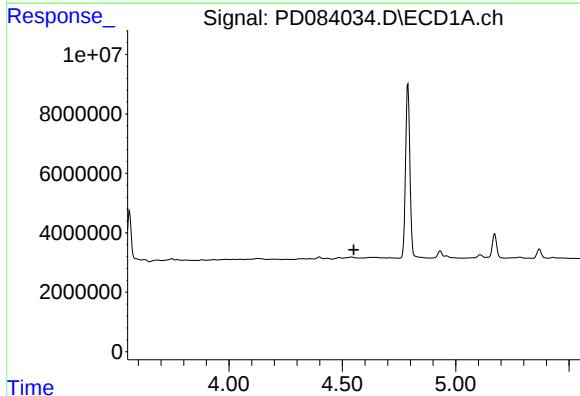


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

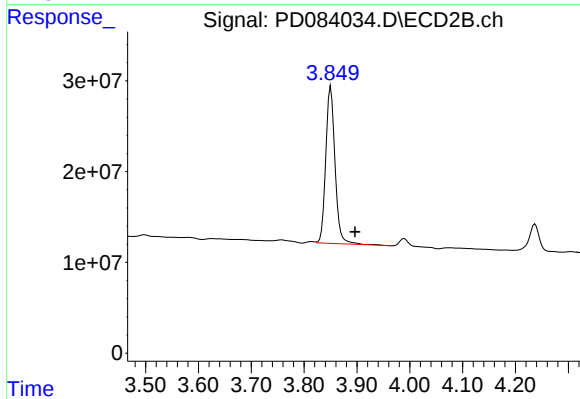


#6 beta-BHC

R.T.: 3.850 min
Delta R.T.: -0.046 min
Response: 210464599
Conc: 55.51 ng/ml

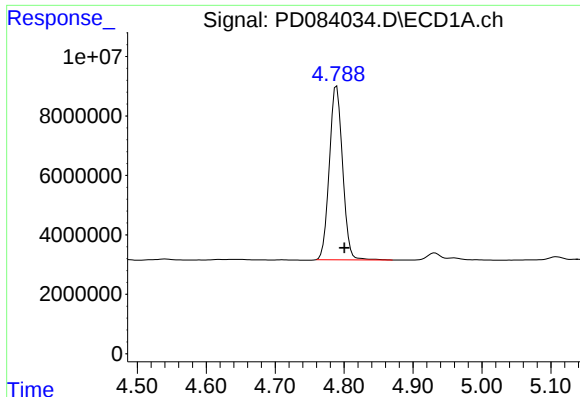


#7 delta-BHC

R.T.: 4.789 min
Delta R.T.: -0.011 min
Response: 77993610
Conc: 36.79 ng/ml

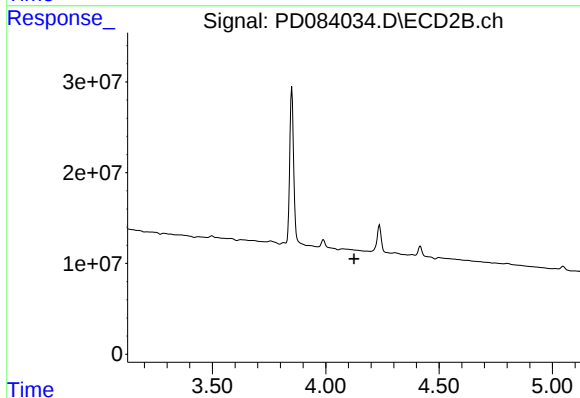


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.125 min
Response: 0
Conc: N.D.

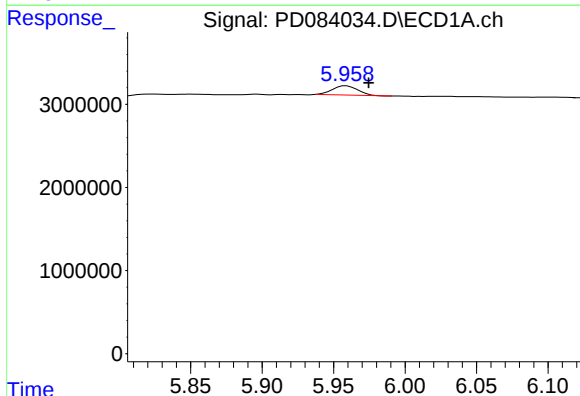


#10 trans-Chlordane

R.T.: 5.959 min
Delta R.T.: -0.016 min
Response: 1390900
Conc: 0.73 ng/ml

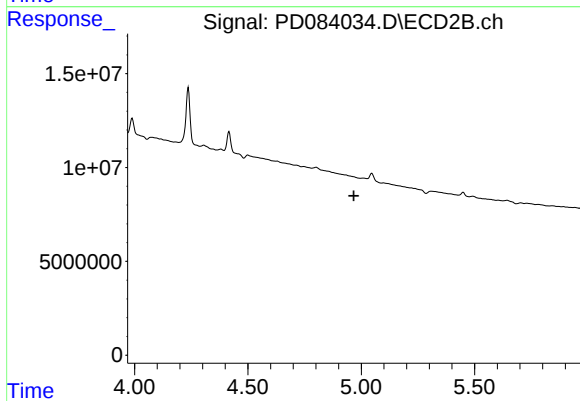


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.967 min
Response: 0
Conc: N.D.

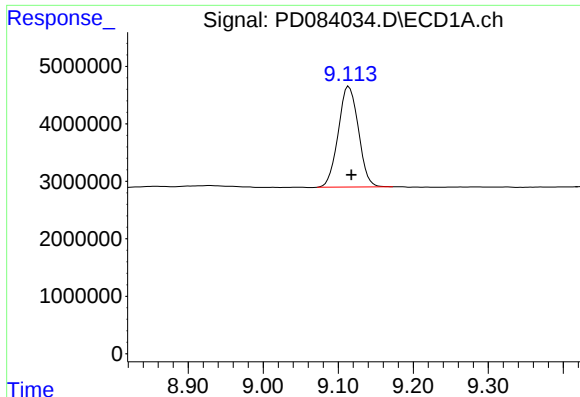

#27 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: -0.003 min
Response: 32749890
Conc: 15.37 ng/ml

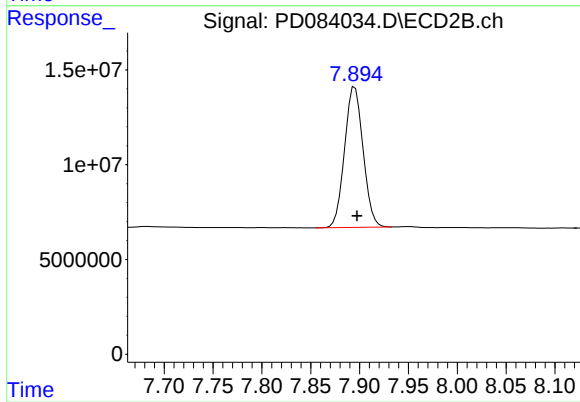

#27 Decachlorobiphenyl

R.T.: 7.895 min
Delta R.T.: -0.002 min
Response: 97964799
Conc: 14.66 ng/ml